

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033504.D
 Acq On : 20 Dec 2023 12:14
 Operator : SY/MD
 Sample : 05850-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VW033504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	93	rVB	161485	172447	3.54%	1.150%
2	1.536	146	154	165	rBV	148497	173526	3.57%	1.157%
3	2.063	306	318	328	rBV	275194	406880	8.36%	2.713%
4	2.548	462	469	470	rBV6	3000	3113	0.06%	0.021%
5	2.783	538	542	544	rBV3	1161	928	0.02%	0.006%
6	2.802	547	548	551	rVB3	1452	662	0.01%	0.004%
7	2.822	551	554	555	rBV2	659	372	0.01%	0.002%
8	2.847	560	562	566	rBV4	1003	877	0.02%	0.006%
9	2.915	579	583	586	rBV6	1100	1008	0.02%	0.007%
10	2.992	605	607	611	rBV3	814	440	0.01%	0.003%
11	3.047	620	624	627	rBV5	1419	1509	0.03%	0.010%
12	3.089	635	637	642	rVB5	1641	914	0.02%	0.006%
13	3.233	679	682	683	rBV3	995	471	0.01%	0.003%
14	3.259	688	690	691	rBV2	739	167	0.00%	0.001%
15	3.455	749	751	754	rBV4	1625	1078	0.02%	0.007%
16	3.507	765	767	768	rBV2	898	330	0.01%	0.002%
17	3.545	777	779	783	rBV4	1266	914	0.02%	0.006%
18	3.645	808	810	812	rBV2	661	316	0.01%	0.002%
19	3.654	812	813	816	rVV3	796	286	0.01%	0.002%
20	3.709	827	830	831	rBV3	885	400	0.01%	0.003%
21	3.748	839	842	843	rBV3	1371	798	0.02%	0.005%
22	3.786	845	854	880	rVV2	65037	186863	3.84%	1.246%
23	4.249	986	998	1022	rVB	173885	442268	9.09%	2.949%
24	4.761	1155	1157	1159	rBV2	808	372	0.01%	0.002%
25	4.899	1198	1200	1201	rBV2	1401	727	0.01%	0.005%
26	4.957	1202	1218	1261	rVV2	421374	1166170	23.97%	7.776%
27	5.535	1386	1398	1417	rBV	327731	679897	13.97%	4.533%
28	5.989	1528	1539	1567	rBV	247776	505181	10.38%	3.368%
29	6.281	1627	1630	1631	rBV3	1236	558	0.01%	0.004%
30	6.867	1811	1812	1815	rBV3	1049	465	0.01%	0.003%
31	6.915	1817	1827	1847	rVV	118235	226090	4.65%	1.508%
32	7.117	1888	1890	1892	rBV3	1485	623	0.01%	0.004%
33	7.243	1918	1929	1951	rBV	470387	832070	17.10%	5.548%
34	7.551	2017	2025	2043	rBV	85539	156672	3.22%	1.045%
35	7.767	2089	2092	2094	rBV2	1573	865	0.02%	0.006%
36	7.950	2144	2149	2150	rBV5	1584	1325	0.03%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033504.D
 Acq On : 20 Dec 2023 12:14
 Operator : SY/MD
 Sample : 05850-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.024	2163	2172	2210	rBV2	193879	410554	8.44%	2.737%
38	8.413	2291	2293	2297	rBV5	1395	995	0.02%	0.007%
39	8.522	2325	2327	2328	rBV2	1188	509	0.01%	0.003%
40	8.735	2391	2393	2396	rBV4	1255	641	0.01%	0.004%
41	8.786	2398	2409	2414	rBV	575830	959638	19.72%	6.399%
42	9.137	2516	2518	2521	rBV3	1424	1028	0.02%	0.007%
43	9.326	2574	2577	2579	rBV5	1188	940	0.02%	0.006%
44	9.349	2583	2584	2585	rBV	741	184	0.00%	0.001%
45	9.410	2602	2603	2608	rBV4	1367	666	0.01%	0.004%
46	9.490	2626	2628	2630	rBV3	1141	533	0.01%	0.004%
47	9.526	2635	2639	2644	rVB7	1193	1209	0.02%	0.008%
48	9.555	2646	2648	2650	rBV3	938	385	0.01%	0.003%
49	9.715	2696	2698	2700	rBV3	1177	572	0.01%	0.004%
50	9.883	2746	2750	2753	rBV5	1522	1485	0.03%	0.010%
51	10.104	2817	2819	2822	rBV3	1329	713	0.01%	0.005%
52	10.153	2822	2834	2856	rVV	311322	501208	10.30%	3.342%
53	10.400	2909	2911	2916	rBV5	1094	1021	0.02%	0.007%
54	10.590	2968	2970	2971	rBV	1392	479	0.01%	0.003%
55	10.751	3018	3020	3021	rBV	1180	531	0.01%	0.004%
56	11.037	3107	3109	3113	rVB5	1398	908	0.02%	0.006%
57	11.056	3113	3115	3116	rBV2	1203	466	0.01%	0.003%
58	11.120	3124	3135	3145	rBV	89896	147060	3.02%	0.981%
59	11.185	3145	3155	3179	rVB2	570339	1378400	28.33%	9.191%
60	11.471	3241	3244	3249	rBV7	1345	1189	0.02%	0.008%
61	11.577	3260	3277	3301	rBV2	2768691	4865354	100.00%	32.441%
62	12.017	3412	3414	3416	rBV3	829	311	0.01%	0.002%
63	12.194	3464	3469	3471	rBV4	2600	2714	0.06%	0.018%
64	12.468	3551	3554	3557	rVB5	1633	1089	0.02%	0.007%
65	12.500	3560	3564	3569	rBV5	1984	2005	0.04%	0.013%
66	12.526	3569	3572	3573	rBV2	1281	706	0.01%	0.005%
67	12.580	3578	3589	3607	rBV3	25087	51315	1.05%	0.342%
68	12.673	3616	3618	3619	rBV	2308	995	0.02%	0.007%
69	12.989	3713	3716	3719	rBV5	790	696	0.01%	0.005%
70	13.050	3733	3735	3737	rBV3	908	349	0.01%	0.002%
71	13.117	3754	3756	3757	rBV2	830	322	0.01%	0.002%
72	13.198	3766	3781	3798	rBV	691872	1044024	21.46%	6.961%
73	13.429	3849	3853	3854	rBV4	1299	969	0.02%	0.006%
74	13.519	3877	3881	3882	rBV4	958	586	0.01%	0.004%
75	13.680	3920	3931	3947	rBV	350400	551266	11.33%	3.676%
76	13.808	3969	3971	3973	rBV2	1060	513	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033504.D
Acq On : 20 Dec 2023 12:14
Operator : SY/MD
Sample : 05850-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

77	13.895	3996	3998	3999	rBV2	1176	439	0.01%	0.003%
78	14.255	4108	4110	4112	rVB3	1552	630	0.01%	0.004%
79	14.268	4112	4114	4115	rBV2	1030	406	0.01%	0.003%
80	14.632	4226	4227	4228	rBV	754	275	0.01%	0.002%
81	14.760	4257	4267	4274	rBV6	13068	20577	0.42%	0.137%
82	14.882	4303	4305	4306	rBV3	1084	370	0.01%	0.002%
83	15.088	4366	4369	4372	rBV5	1590	973	0.02%	0.006%
84	15.336	4436	4446	4455	rBV2	43231	71701	1.47%	0.478%




Sum of corrected areas: 14997481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033504.D
Acq On : 20 Dec 2023 12:14
Operator : SY/MD
Sample : 05850-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

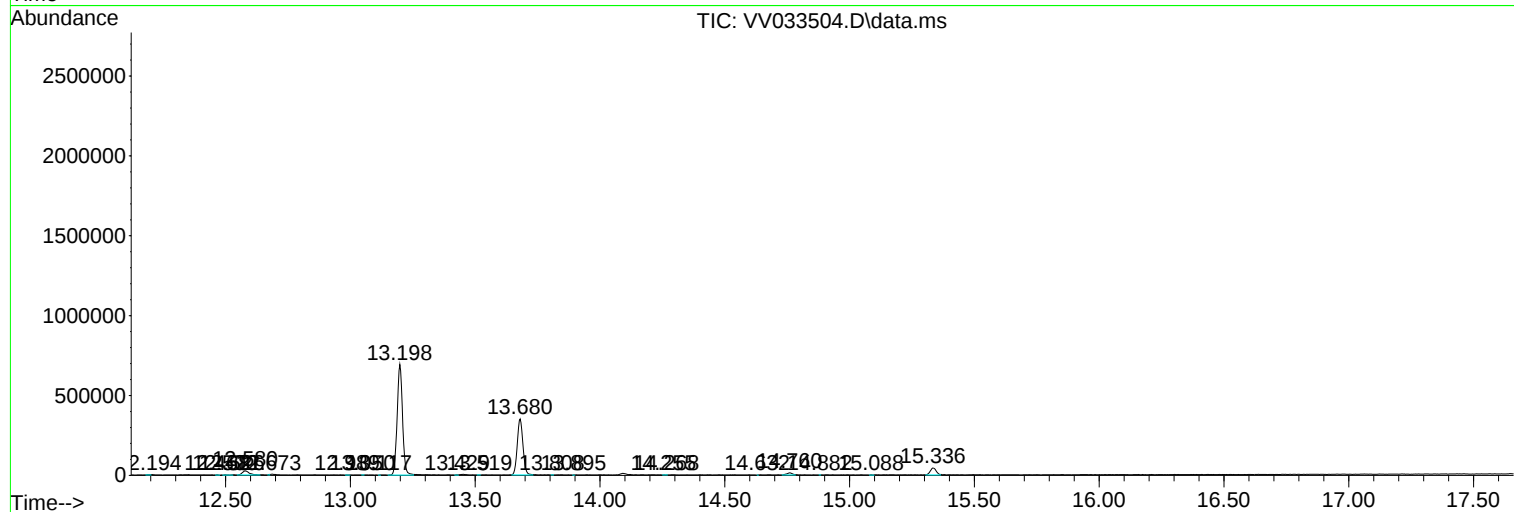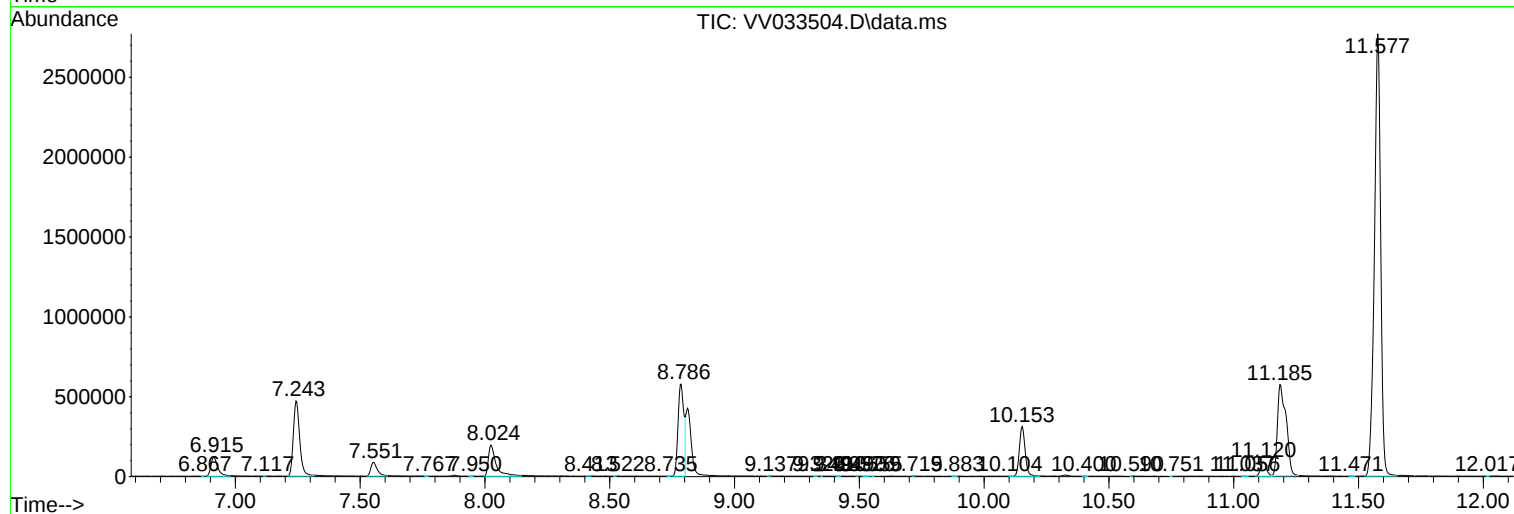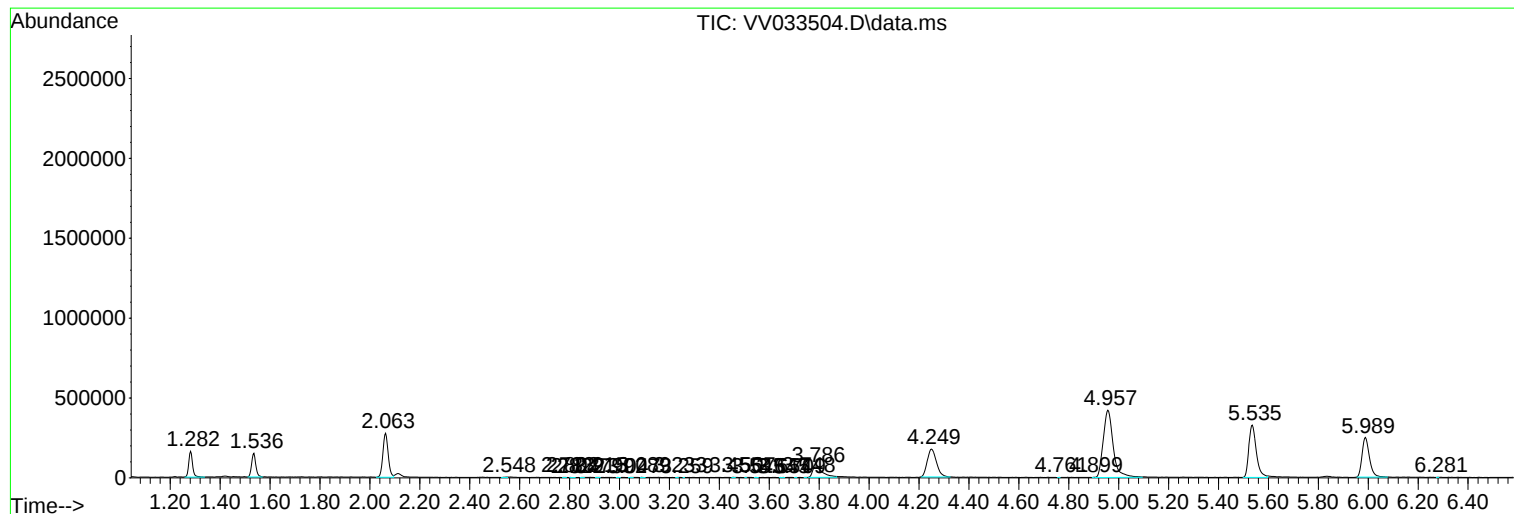

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033504.D
Acq On : 20 Dec 2023 12:14
Operator : SY/MD
Sample : 05850-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033504.D
Acq On : 20 Dec 2023 12:14
Operator : SY/MD
Sample : 05850-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc