

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033505.D
 Acq On : 20 Dec 2023 12:37
 Operator : SY/MD
 Sample : 05850-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	162495	172273	3.09%	0.947%
2	1.535	147	154	171	rVB	143712	170213	3.05%	0.936%
3	2.063	309	318	330	rBV	274132	397295	7.12%	2.185%
4	2.397	420	422	424	rBV3	1447	670	0.01%	0.004%
5	2.523	456	461	462	rBV4	850	736	0.01%	0.004%
6	2.773	537	539	543	rBV4	778	430	0.01%	0.002%
7	2.844	558	561	563	rBV5	1170	576	0.01%	0.003%
8	2.879	568	572	575	rBV4	708	624	0.01%	0.003%
9	2.960	595	597	598	rBV2	865	445	0.01%	0.002%
10	2.992	606	607	610	rBV2	981	446	0.01%	0.002%
11	3.005	610	611	613	rBV3	1062	531	0.01%	0.003%
12	3.095	635	639	640	rBV4	899	504	0.01%	0.003%
13	3.182	664	666	670	rBV4	847	458	0.01%	0.003%
14	3.256	685	689	692	rBV4	832	633	0.01%	0.003%
15	3.288	697	699	702	rVV4	801	478	0.01%	0.003%
16	3.333	709	713	715	rVB4	709	598	0.01%	0.003%
17	3.362	720	722	725	rBV4	1344	719	0.01%	0.004%
18	3.481	757	759	761	rBV3	942	424	0.01%	0.002%
19	3.574	786	788	793	rBV6	1420	990	0.02%	0.005%
20	3.600	793	796	799	rVB4	1387	810	0.01%	0.004%
21	3.619	799	802	803	rBV3	948	648	0.01%	0.004%
22	3.667	814	817	820	rBV5	1396	1278	0.02%	0.007%
23	3.732	834	837	839	rBV4	1073	604	0.01%	0.003%
24	3.744	839	841	844	rBV4	1186	942	0.02%	0.005%
25	3.786	844	854	879	rBV3	69926	199859	3.58%	1.099%
26	4.249	983	998	1024	rBV2	179620	480414	8.60%	2.642%
27	4.661	1121	1126	1127	rBV4	1430	1428	0.03%	0.008%
28	4.844	1179	1183	1184	rBV4	1643	903	0.02%	0.005%
29	4.960	1198	1219	1227	rBV2	428331	1098771	19.68%	6.043%
30	5.535	1386	1398	1425	rBV	338839	709602	12.71%	3.903%
31	5.989	1527	1539	1561	rBV	251296	516612	9.25%	2.841%
32	6.609	1727	1732	1735	rBV6	2121	1691	0.03%	0.009%
33	6.670	1748	1751	1753	rVB4	1187	740	0.01%	0.004%
34	6.686	1753	1756	1757	rBV3	1329	860	0.02%	0.005%
35	6.748	1771	1775	1778	rVB5	1714	1330	0.02%	0.007%
36	6.825	1795	1799	1800	rBV4	1507	1028	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033505.D
 Acq On : 20 Dec 2023 12:37
 Operator : SY/MD
 Sample : 05850-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.915	1816	1827	1849	rBV	121792	233174	4.18%	1.282%
38	7.243	1918	1929	1949	rBV	472052	843878	15.11%	4.641%
39	7.510	2009	2012	2014	rBV3	1409	1030	0.02%	0.006%
40	7.551	2017	2025	2047	rVV	87025	159534	2.86%	0.877%
41	7.735	2080	2082	2088	rVB6	1643	965	0.02%	0.005%
42	7.837	2109	2114	2117	rBV6	1444	1336	0.02%	0.007%
43	7.960	2150	2152	2155	rVB4	1470	677	0.01%	0.004%
44	7.976	2155	2157	2161	rBV4	1413	949	0.02%	0.005%
45	8.024	2163	2172	2205	rBV	206807	433615	7.77%	2.385%
46	8.365	2276	2278	2280	rBV3	1157	619	0.01%	0.003%
47	8.423	2295	2296	2299	rVB2	1020	500	0.01%	0.003%
48	8.538	2330	2332	2339	rBV6	1542	1343	0.02%	0.007%
49	8.641	2358	2364	2367	rBV4	989	1107	0.02%	0.006%
50	8.661	2368	2370	2375	rVB5	1814	1148	0.02%	0.006%
51	8.812	2397	2417	2442	rBV2	2922352	5583472	100.00%	30.708%
52	9.365	2587	2589	2593	rBV5	1501	858	0.02%	0.005%
53	9.567	2648	2652	2653	rBV3	1373	1182	0.02%	0.007%
54	9.635	2668	2673	2677	rBV8	1351	1595	0.03%	0.009%
55	9.741	2701	2706	2708	rBV5	2204	1649	0.03%	0.009%
56	9.789	2714	2721	2723	rBV7	1118	1284	0.02%	0.007%
57	9.825	2731	2732	2735	rBV3	1003	557	0.01%	0.003%
58	9.895	2750	2754	2756	rBV3	1249	970	0.02%	0.005%
59	10.062	2801	2806	2807	rBV5	998	716	0.01%	0.004%
60	10.111	2818	2821	2822	rBV2	1417	736	0.01%	0.004%
61	10.153	2823	2834	2852	rVV	316985	495359	8.87%	2.724%
62	10.400	2908	2911	2912	rBV3	1002	501	0.01%	0.003%
63	10.497	2935	2941	2942	rBV5	818	852	0.02%	0.005%
64	10.632	2980	2983	2986	rVV4	1040	662	0.01%	0.004%
65	10.683	2995	2999	3004	rVB6	1599	1287	0.02%	0.007%
66	10.709	3004	3007	3008	rBV2	1003	555	0.01%	0.003%
67	10.747	3017	3019	3022	rVB2	1143	674	0.01%	0.004%
68	10.770	3022	3026	3030	rBV5	1777	1464	0.03%	0.008%
69	10.818	3037	3041	3042	rBV3	865	577	0.01%	0.003%
70	10.976	3087	3090	3092	rVB4	907	446	0.01%	0.002%
71	11.014	3098	3102	3104	rBV3	1083	819	0.01%	0.005%
72	11.117	3124	3134	3145	rBV	153615	242940	4.35%	1.336%
73	11.207	3146	3162	3185	rVB2	801797	2020671	36.19%	11.113%
74	11.577	3257	3277	3298	rBV2	1996445	3738860	66.96%	20.563%
75	11.863	3364	3366	3367	rBV	1157	477	0.01%	0.003%
76	11.985	3402	3404	3407	rBV3	1032	681	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033505.D
 Acq On : 20 Dec 2023 12:37
 Operator : SY/MD
 Sample : 05850-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.011	3410	3412	3413	rBV2	1072	462	0.01%	0.003%
78	12.091	3434	3437	3439	rBV4	880	556	0.01%	0.003%
79	12.178	3462	3464	3466	rBV3	1209	688	0.01%	0.004%
80	12.400	3531	3533	3535	rBV3	1008	502	0.01%	0.003%
81	12.439	3543	3545	3549	rVB3	1147	721	0.01%	0.004%
82	12.535	3573	3575	3579	rBV3	1206	841	0.02%	0.005%
83	12.744	3637	3640	3643	rBV3	937	569	0.01%	0.003%
84	12.779	3649	3651	3653	rBV4	1063	468	0.01%	0.003%
85	12.908	3689	3691	3693	rBV3	1150	635	0.01%	0.003%
86	12.988	3711	3716	3721	rBV7	2317	2127	0.04%	0.012%
87	13.197	3768	3781	3801	rBV	265225	412334	7.38%	2.268%
88	13.339	3822	3825	3830	rBV6	1261	1266	0.02%	0.007%
89	13.426	3846	3852	3854	rBV5	1983	2125	0.04%	0.012%
90	13.680	3920	3931	3948	rBV	105746	174886	3.13%	0.962%
91	14.162	4078	4081	4082	rBV4	1041	643	0.01%	0.004%
92	14.291	4118	4121	4124	rBV4	865	619	0.01%	0.003%
93	14.516	4187	4191	4192	rBV3	1292	832	0.01%	0.005%
94	14.763	4261	4268	4275	rVB10	4306	5935	0.11%	0.033%
95	15.014	4342	4346	4349	rBV5	972	888	0.02%	0.005%
96	15.188	4398	4400	4404	rVB4	1385	737	0.01%	0.004%
97	15.207	4404	4406	4410	rBV5	843	651	0.01%	0.004%
98	15.336	4439	4446	4456	rVB6	16576	26006	0.47%	0.143%
99	15.496	4494	4496	4498	rBV3	1537	763	0.01%	0.004%
100	15.525	4503	4505	4509	rBV5	1390	980	0.02%	0.005%




Sum of corrected areas: 18182516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033505.D
Acq On : 20 Dec 2023 12:37
Operator : SY/MD
Sample : 05850-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

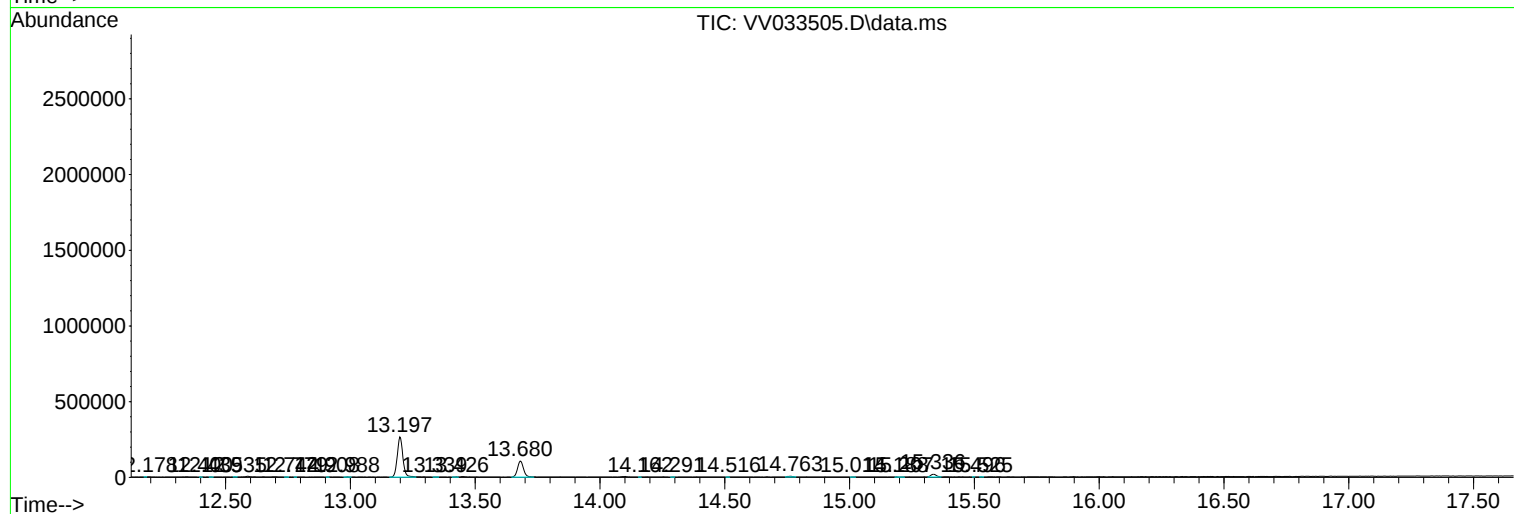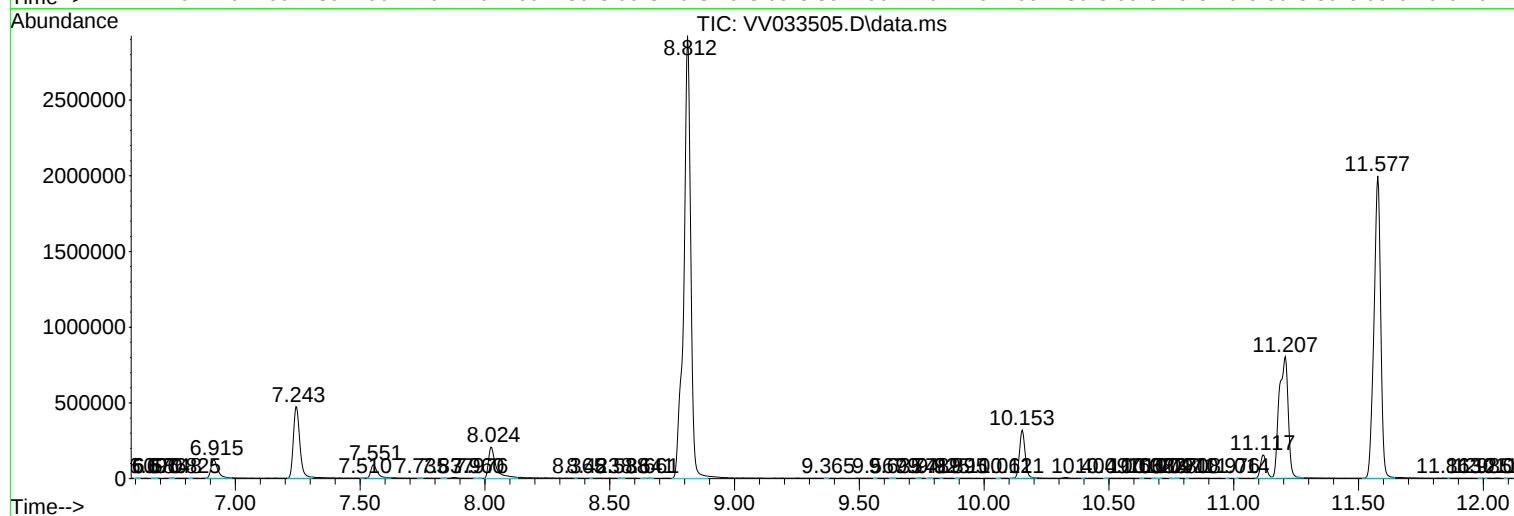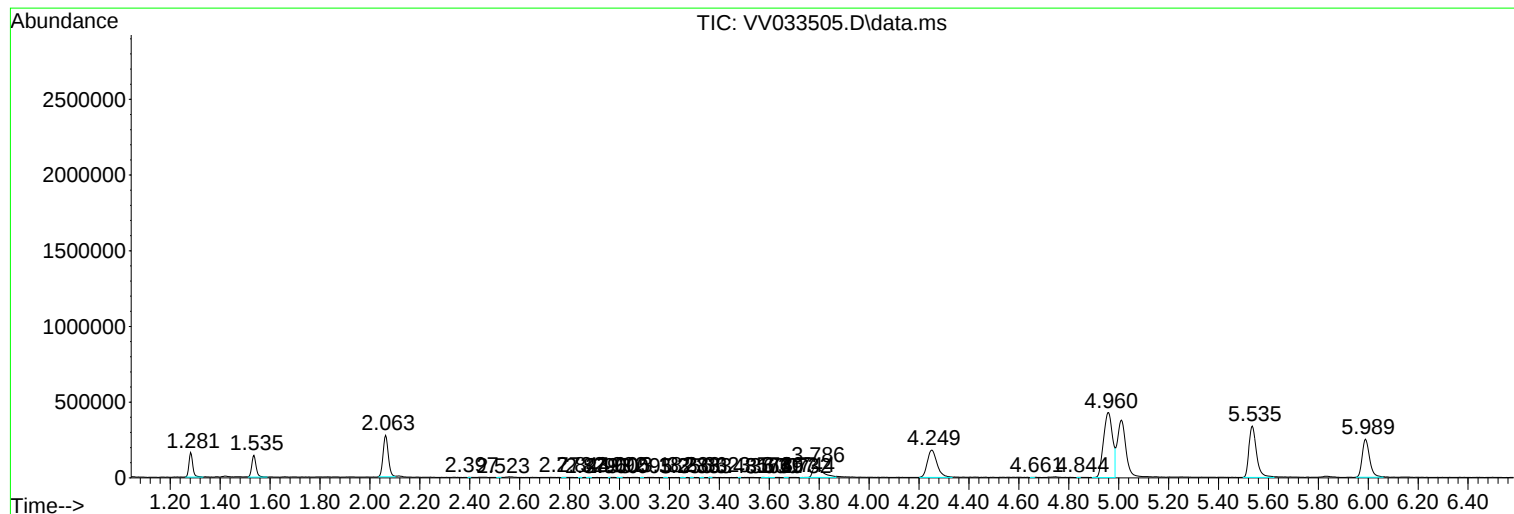

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033505.D
Acq On : 20 Dec 2023 12:37
Operator : SY/MD
Sample : 05850-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033505.D
Acq On : 20 Dec 2023 12:37
Operator : SY/MD
Sample : 05850-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc