

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033506.D
 Acq On : 20 Dec 2023 13:00
 Operator : SY/MD
 Sample : 05850-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	166186	170795	15.41%	2.056%
2	1.532	146	153	168	rVB	139855	165803	14.96%	1.996%
3	2.063	308	318	330	rBV	262589	388850	35.08%	4.681%
4	2.654	499	502	506	rBV6	1970	1915	0.17%	0.023%
5	2.867	566	568	575	rVB7	1711	1002	0.09%	0.012%
6	2.902	575	579	583	rBV6	1680	1580	0.14%	0.019%
7	3.024	613	617	619	rBV5	1206	691	0.06%	0.008%
8	3.069	626	631	633	rBV6	1188	1168	0.11%	0.014%
9	3.121	645	647	650	rVB3	1145	585	0.05%	0.007%
10	3.233	676	682	684	rBV4	1336	984	0.09%	0.012%
11	3.246	684	686	690	rVB5	1459	819	0.07%	0.010%
12	3.294	697	701	704	rBV4	1238	1026	0.09%	0.012%
13	3.365	721	723	726	rBV4	852	684	0.06%	0.008%
14	3.404	733	735	737	rVB3	1258	560	0.05%	0.007%
15	3.548	778	780	783	rVB2	997	509	0.05%	0.006%
16	3.600	795	796	798	rBV2	762	407	0.04%	0.005%
17	3.664	814	816	819	rVB3	1089	532	0.05%	0.006%
18	3.683	819	822	824	rBV3	1259	1024	0.09%	0.012%
19	3.722	829	834	839	rVB6	2252	2111	0.19%	0.025%
20	3.786	839	854	880	rBV2	72492	218074	19.67%	2.625%
21	4.188	977	979	981	rBV2	1272	684	0.06%	0.008%
22	4.249	985	998	1023	rVB	174728	453152	40.88%	5.455%
23	4.645	1118	1121	1125	rBV6	1616	1328	0.12%	0.016%
24	4.841	1178	1182	1185	rBV4	1415	1147	0.10%	0.014%
25	4.857	1185	1187	1189	rVV3	1292	645	0.06%	0.008%
26	4.957	1202	1218	1249	rBV2	413779	1108532	100.00%	13.344%
27	5.532	1386	1397	1426	rBV	309371	657334	59.30%	7.913%
28	5.789	1475	1477	1480	rBV4	1570	1081	0.10%	0.013%
29	5.989	1527	1539	1564	rBV	242710	506422	45.68%	6.096%
30	6.349	1648	1651	1656	rBV6	1696	1645	0.15%	0.020%
31	6.419	1670	1673	1676	rBV5	1460	994	0.09%	0.012%
32	6.532	1704	1708	1710	rBV4	1498	1087	0.10%	0.013%
33	6.603	1726	1730	1733	rBV5	1401	1048	0.09%	0.013%
34	6.625	1735	1737	1741	rVV3	1025	532	0.05%	0.006%
35	6.915	1816	1827	1846	rBV	116457	224358	20.24%	2.701%
36	7.243	1918	1929	1957	rBV	453184	822115	74.16%	9.896%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033506.D
 Acq On : 20 Dec 2023 13:00
 Operator : SY/MD
 Sample : 05850-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.554	2017	2026	2043	rBV	83121	149548	13.49%	1.800%
38	7.837	2112	2114	2115	rBV	1318	492	0.04%	0.006%
39	7.915	2136	2138	2142	rVB4	1404	1033	0.09%	0.012%
40	8.024	2163	2172	2211	rBV	192922	417519	37.66%	5.026%
41	8.599	2348	2351	2357	rVB9	1252	1170	0.11%	0.014%
42	8.638	2362	2363	2365	rBV2	1411	516	0.05%	0.006%
43	8.686	2376	2378	2381	rBV4	1177	582	0.05%	0.007%
44	8.783	2397	2408	2435	rBV	506600	872893	78.74%	10.507%
45	9.230	2545	2547	2551	rBV5	1245	709	0.06%	0.009%
46	9.400	2595	2600	2601	rBV4	1804	1543	0.14%	0.019%
47	9.596	2658	2661	2662	rBV3	1060	613	0.06%	0.007%
48	9.625	2666	2670	2671	rBV2	1270	721	0.07%	0.009%
49	9.728	2699	2702	2704	rBV4	1024	612	0.06%	0.007%
50	9.873	2744	2747	2749	rBV4	1118	879	0.08%	0.011%
51	9.886	2749	2751	2753	rBV3	1213	593	0.05%	0.007%
52	9.988	2781	2783	2785	rBV3	1002	599	0.05%	0.007%
53	10.066	2803	2807	2808	rBV3	1227	973	0.09%	0.012%
54	10.152	2823	2834	2854	rBV	304727	483415	43.61%	5.819%
55	10.326	2879	2888	2897	rBV	4803	8648	0.78%	0.104%
56	10.381	2903	2905	2907	rVB3	1273	646	0.06%	0.008%
57	10.484	2935	2937	2940	rVB4	1559	646	0.06%	0.008%
58	10.561	2957	2961	2963	rBV4	1658	1098	0.10%	0.013%
59	10.577	2963	2966	2968	rBV3	874	626	0.06%	0.008%
60	10.805	3034	3037	3039	rBV3	862	463	0.04%	0.006%
61	10.853	3048	3052	3053	rBV4	932	671	0.06%	0.008%
62	10.998	3095	3097	3105	rVB7	1925	1720	0.16%	0.021%
63	11.030	3105	3107	3110	rVB3	803	409	0.04%	0.005%
64	11.185	3144	3155	3181	rBV	470319	753091	67.94%	9.065%
65	11.419	3225	3228	3230	rBV3	1224	1000	0.09%	0.012%
66	11.503	3252	3254	3256	rVB2	1226	504	0.05%	0.006%
67	11.561	3261	3272	3304	rVV	476995	791421	71.39%	9.527%
68	11.898	3374	3377	3380	rBV4	1032	784	0.07%	0.009%
69	11.995	3404	3407	3408	rBV3	1084	578	0.05%	0.007%
70	12.101	3437	3440	3443	rBV4	1022	820	0.07%	0.010%
71	12.172	3458	3462	3465	rBV6	1701	1456	0.13%	0.018%
72	12.381	3519	3527	3531	rBV10	1599	2037	0.18%	0.025%
73	12.410	3535	3536	3539	rBV3	1241	559	0.05%	0.007%
74	12.741	3637	3639	3642	rVB3	1014	504	0.05%	0.006%
75	12.757	3642	3644	3647	rBV3	931	575	0.05%	0.007%
76	12.860	3674	3676	3678	rBV3	1050	557	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033506.D
 Acq On : 20 Dec 2023 13:00
 Operator : SY/MD
 Sample : 05850-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.037	3728	3731	3734	rBV4	920	635	0.06%	0.008%
78	13.062	3734	3739	3743	rBV6	1601	1608	0.15%	0.019%
79	13.114	3752	3755	3759	rBV5	1170	761	0.07%	0.009%
80	13.204	3774	3783	3792	rBV5	15817	25700	2.32%	0.309%
81	13.313	3814	3817	3820	rVB5	1011	565	0.05%	0.007%
82	13.332	3820	3823	3824	rBV3	1090	580	0.05%	0.007%
83	13.381	3833	3838	3840	rBV5	1379	1274	0.11%	0.015%
84	13.474	3864	3867	3869	rBV4	1239	697	0.06%	0.008%
85	13.522	3880	3882	3884	rVB3	1310	508	0.05%	0.006%
86	13.548	3888	3890	3893	rBV3	767	573	0.05%	0.007%
87	13.628	3913	3915	3921	rBV5	1217	1246	0.11%	0.015%
88	13.686	3924	3933	3946	rVB5	8056	15965	1.44%	0.192%
89	13.783	3961	3963	3966	rBV3	887	491	0.04%	0.006%
90	13.882	3992	3994	3996	rBV3	1030	441	0.04%	0.005%
91	14.082	4054	4056	4060	rBV4	1242	893	0.08%	0.011%
92	14.127	4068	4070	4071	rBV2	1461	444	0.04%	0.005%
93	14.265	4111	4113	4115	rBV3	1260	586	0.05%	0.007%
94	14.294	4118	4122	4123	rBV3	939	704	0.06%	0.008%
95	14.397	4151	4154	4159	rBV7	1190	955	0.09%	0.011%
96	14.815	4281	4284	4289	rBV7	1073	1130	0.10%	0.014%
97	14.860	4296	4298	4302	rBV3	1214	930	0.08%	0.011%
98	15.336	4441	4446	4453	rVB8	3851	5098	0.46%	0.061%
99	15.805	4589	4592	4593	rBV2	1269	713	0.06%	0.009%
100	15.869	4610	4612	4613	rBV	1448	560	0.05%	0.007%




Sum of corrected areas: 8307503

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033506.D
Acq On : 20 Dec 2023 13:00
Operator : SY/MD
Sample : 05850-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

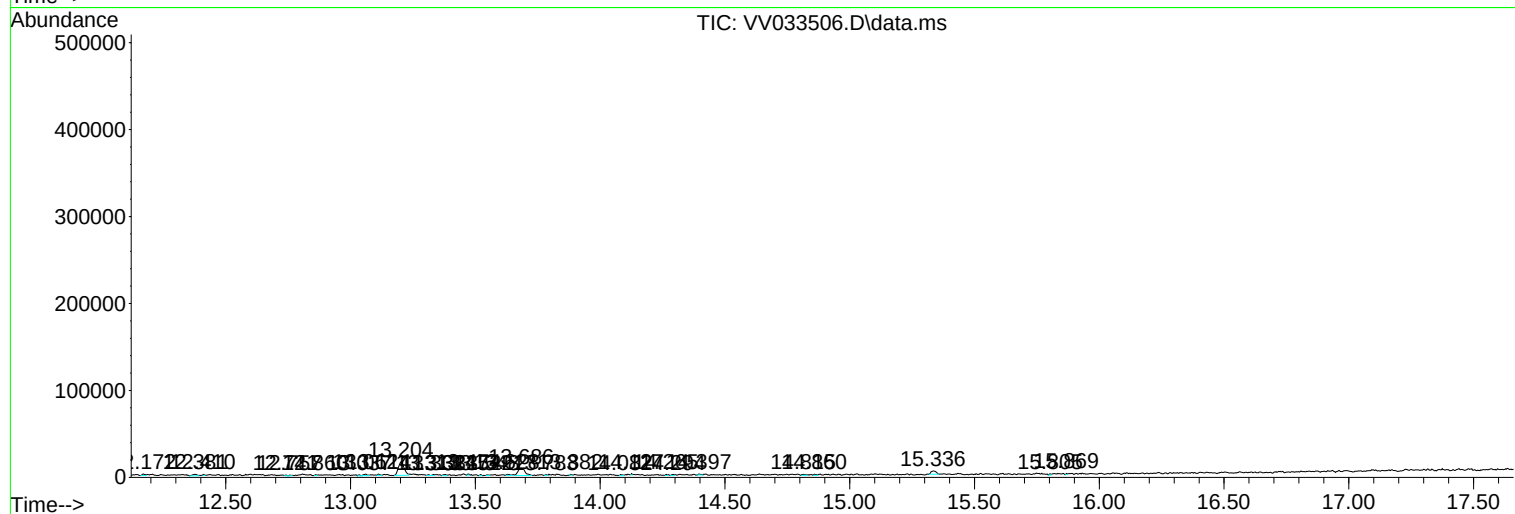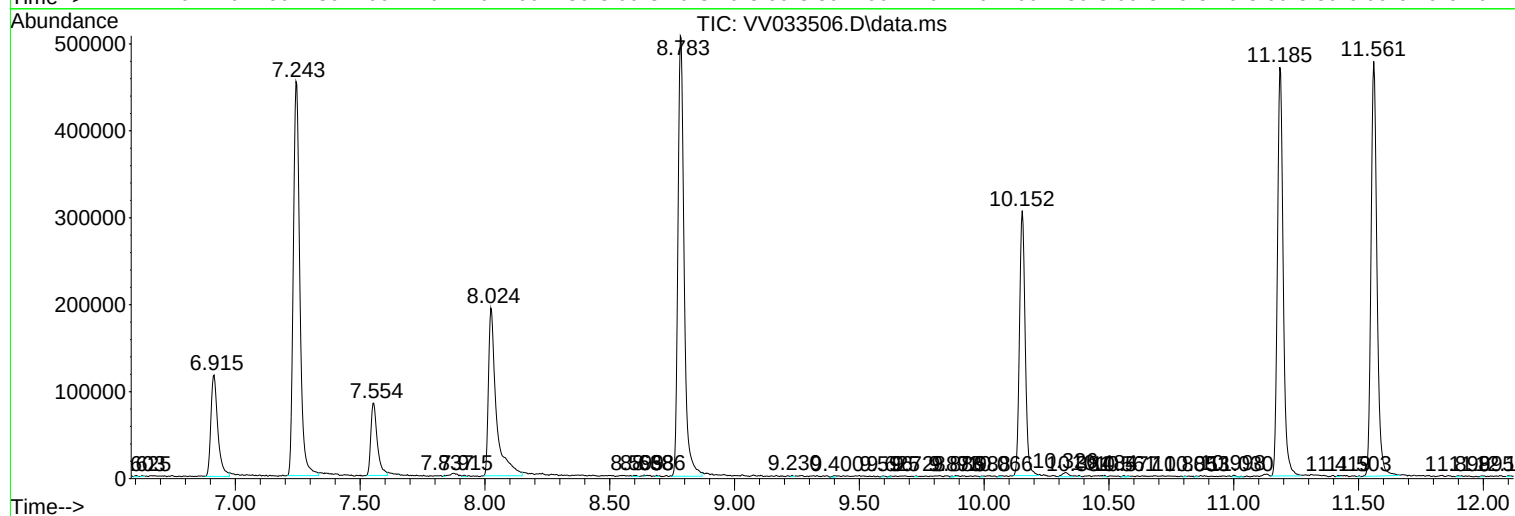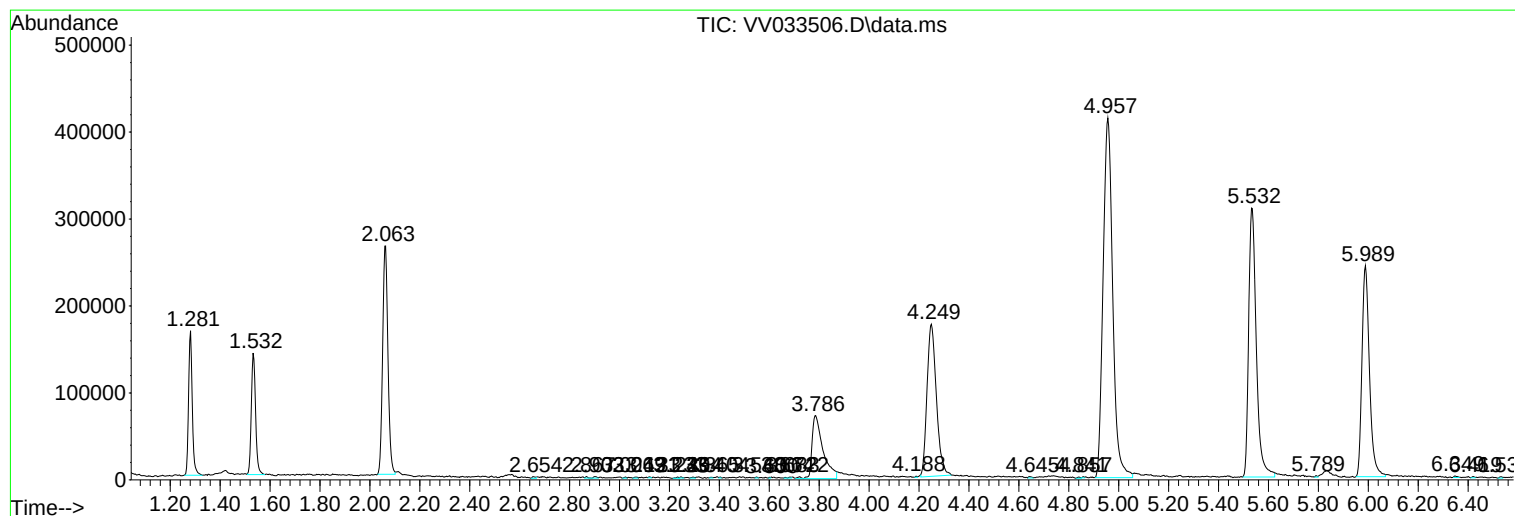

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033506.D
Acq On : 20 Dec 2023 13:00
Operator : SY/MD
Sample : 05850-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033506.D
Acq On : 20 Dec 2023 13:00
Operator : SY/MD
Sample : 05850-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc