

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033507.D
 Acq On : 20 Dec 2023 13:23
 Operator : SY/MD
 Sample : 05850-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033507.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	163622	171057	15.30%	2.101%
2	1.532	146	153	168	rVB	141958	168371	15.06%	2.068%
3	2.060	308	317	332	rBV	267840	391164	34.98%	4.805%
4	2.368	410	413	414	rBV2	1062	621	0.06%	0.008%
5	2.513	455	458	462	rBV5	1449	960	0.09%	0.012%
6	2.645	495	499	500	rBV3	888	549	0.05%	0.007%
7	2.696	513	515	516	rBV2	901	294	0.03%	0.004%
8	2.770	534	538	540	rBV4	1061	739	0.07%	0.009%
9	2.815	550	552	553	rBV2	515	216	0.02%	0.003%
10	2.825	553	555	556	rVV	740	244	0.02%	0.003%
11	2.889	573	575	576	rBV	1144	395	0.04%	0.005%
12	3.047	622	624	628	rBV4	734	594	0.05%	0.007%
13	3.066	628	630	631	rBV2	908	380	0.03%	0.005%
14	3.092	636	638	640	rBV3	793	365	0.03%	0.004%
15	3.330	710	712	713	rBV2	670	224	0.02%	0.003%
16	3.410	733	737	741	rBV6	1314	1505	0.13%	0.018%
17	3.449	746	749	750	rBV3	717	399	0.04%	0.005%
18	3.458	750	752	753	rBV2	541	203	0.02%	0.002%
19	3.474	756	757	762	rVV5	1171	861	0.08%	0.011%
20	3.519	767	771	773	rBV4	1171	1070	0.10%	0.013%
21	3.535	773	776	783	rVB6	1550	1472	0.13%	0.018%
22	3.568	783	786	787	rBV2	666	473	0.04%	0.006%
23	3.613	795	800	803	rVB6	1556	1331	0.12%	0.016%
24	3.667	815	817	820	rVB4	1366	665	0.06%	0.008%
25	3.693	823	825	826	rBV	804	425	0.04%	0.005%
26	3.725	834	835	839	rBV4	803	461	0.04%	0.006%
27	3.744	839	841	842	rBV2	801	301	0.03%	0.004%
28	3.783	844	853	879	rBV2	70893	201632	18.03%	2.477%
29	4.249	984	998	1022	rBV2	175085	453598	40.56%	5.572%
30	4.957	1199	1218	1248	rBV2	416198	1118224	100.00%	13.736%
31	5.436	1361	1367	1370	rBV8	1641	1989	0.18%	0.024%
32	5.532	1387	1397	1423	rBV	308173	637865	57.04%	7.835%
33	5.989	1527	1539	1567	rBV2	240198	502395	44.93%	6.171%
34	6.416	1670	1672	1674	rBV3	1017	399	0.04%	0.005%
35	6.539	1708	1710	1712	rVB3	1243	392	0.04%	0.005%
36	6.603	1728	1730	1731	rBV2	944	315	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033507.D
 Acq On : 20 Dec 2023 13:23
 Operator : SY/MD
 Sample : 05850-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.786	1785	1787	1789	rVB2	1238	328	0.03%	0.004%
38	6.863	1807	1811	1812	rBV3	1000	508	0.05%	0.006%
39	6.912	1816	1826	1845	rBV	117821	223198	19.96%	2.742%
40	7.243	1918	1929	1950	rBV	461825	820057	73.34%	10.073%
41	7.551	2018	2025	2043	rBV	83273	142607	12.75%	1.752%
42	7.821	2107	2109	2115	rVB7	1523	1155	0.10%	0.014%
43	7.973	2153	2156	2158	rBV5	1320	790	0.07%	0.010%
44	8.024	2162	2172	2202	rBV	197486	423654	37.89%	5.204%
45	8.413	2291	2293	2294	rBV2	963	281	0.03%	0.003%
46	8.497	2317	2319	2323	rBV5	1268	904	0.08%	0.011%
47	8.590	2344	2348	2350	rBV4	1005	761	0.07%	0.009%
48	8.786	2398	2409	2433	rBV	507666	850951	76.10%	10.453%
49	9.091	2502	2504	2505	rBV2	789	419	0.04%	0.005%
50	9.220	2541	2544	2546	rBV3	1535	894	0.08%	0.011%
51	9.236	2547	2549	2552	rVB4	1594	785	0.07%	0.010%
52	9.632	2670	2672	2675	rBV3	881	673	0.06%	0.008%
53	9.709	2695	2696	2698	rBV2	1143	633	0.06%	0.008%
54	9.786	2718	2720	2724	rBV4	1230	1111	0.10%	0.014%
55	9.831	2732	2734	2735	rBV2	1386	511	0.05%	0.006%
56	9.876	2744	2748	2751	rBV6	1311	1092	0.10%	0.013%
57	10.079	2809	2811	2815	rBV4	776	440	0.04%	0.005%
58	10.153	2823	2834	2854	rBV	306045	484937	43.37%	5.957%
59	10.252	2863	2865	2868	rVB3	1211	406	0.04%	0.005%
60	10.291	2875	2877	2879	rBV3	1265	633	0.06%	0.008%
61	10.394	2906	2909	2911	rBV3	1080	552	0.05%	0.007%
62	10.435	2921	2922	2926	rVB3	855	404	0.04%	0.005%
63	10.567	2961	2963	2966	rVB4	876	507	0.05%	0.006%
64	10.583	2966	2968	2969	rBV2	1033	426	0.04%	0.005%
65	10.706	3003	3006	3007	rBV3	1047	557	0.05%	0.007%
66	10.757	3020	3022	3024	rBV4	686	290	0.03%	0.004%
67	10.808	3037	3038	3040	rBV3	886	289	0.03%	0.004%
68	10.950	3080	3082	3083	rBV2	709	313	0.03%	0.004%
69	11.124	3132	3136	3138	rBV5	1930	1580	0.14%	0.019%
70	11.185	3144	3155	3175	rBV	464970	734748	65.71%	9.025%
71	11.464	3240	3242	3245	rVB3	821	388	0.03%	0.005%
72	11.561	3260	3272	3292	rBV	484710	761791	68.13%	9.357%
73	11.751	3329	3331	3333	rBV2	777	238	0.02%	0.003%
74	12.101	3439	3440	3442	rBV2	1104	348	0.03%	0.004%
75	12.140	3446	3452	3454	rBV6	1512	1378	0.12%	0.017%
76	12.345	3514	3516	3517	rBV2	658	234	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033507.D
 Acq On : 20 Dec 2023 13:23
 Operator : SY/MD
 Sample : 05850-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.400	3531	3533	3536	rBV4	901	648	0.06%	0.008%
78	12.474	3554	3556	3559	rVB3	1159	623	0.06%	0.008%
79	12.503	3563	3565	3567	rBV3	1079	431	0.04%	0.005%
80	12.712	3625	3630	3632	rBV5	1433	1258	0.11%	0.015%
81	12.789	3652	3654	3659	rVB5	918	549	0.05%	0.007%
82	12.950	3700	3704	3706	rBV5	803	600	0.05%	0.007%
83	12.979	3712	3713	3717	rVB5	1071	515	0.05%	0.006%
84	13.001	3717	3720	3723	rBV3	1301	1022	0.09%	0.013%
85	13.024	3723	3727	3729	rVB4	1062	795	0.07%	0.010%
86	13.149	3762	3766	3768	rBV5	828	667	0.06%	0.008%
87	13.268	3800	3803	3805	rBV3	1309	857	0.08%	0.011%
88	13.384	3837	3839	3841	rBV2	727	301	0.03%	0.004%
89	13.496	3872	3874	3880	rVB5	1179	674	0.06%	0.008%
90	13.561	3891	3894	3897	rBV5	1124	702	0.06%	0.009%
91	13.667	3924	3927	3928	rBV3	1471	830	0.07%	0.010%
92	13.779	3958	3962	3964	rBV5	839	493	0.04%	0.006%
93	13.812	3967	3972	3974	rBV5	1769	1605	0.14%	0.020%
94	14.017	4033	4036	4038	rVB4	1167	659	0.06%	0.008%
95	14.400	4152	4155	4156	rBV3	1226	582	0.05%	0.007%
96	14.731	4255	4258	4259	rBV3	1354	763	0.07%	0.009%
97	14.918	4312	4316	4317	rBV2	1140	783	0.07%	0.010%
98	14.972	4331	4333	4334	rBV2	816	317	0.03%	0.004%
99	15.085	4366	4368	4369	rBV2	1021	501	0.04%	0.006%
100	15.541	4507	4510	4512	rBV2	1554	978	0.09%	0.012%

Sum of corrected areas: 8141072




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033507.D
Acq On : 20 Dec 2023 13:23
Operator : SY/MD
Sample : 05850-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

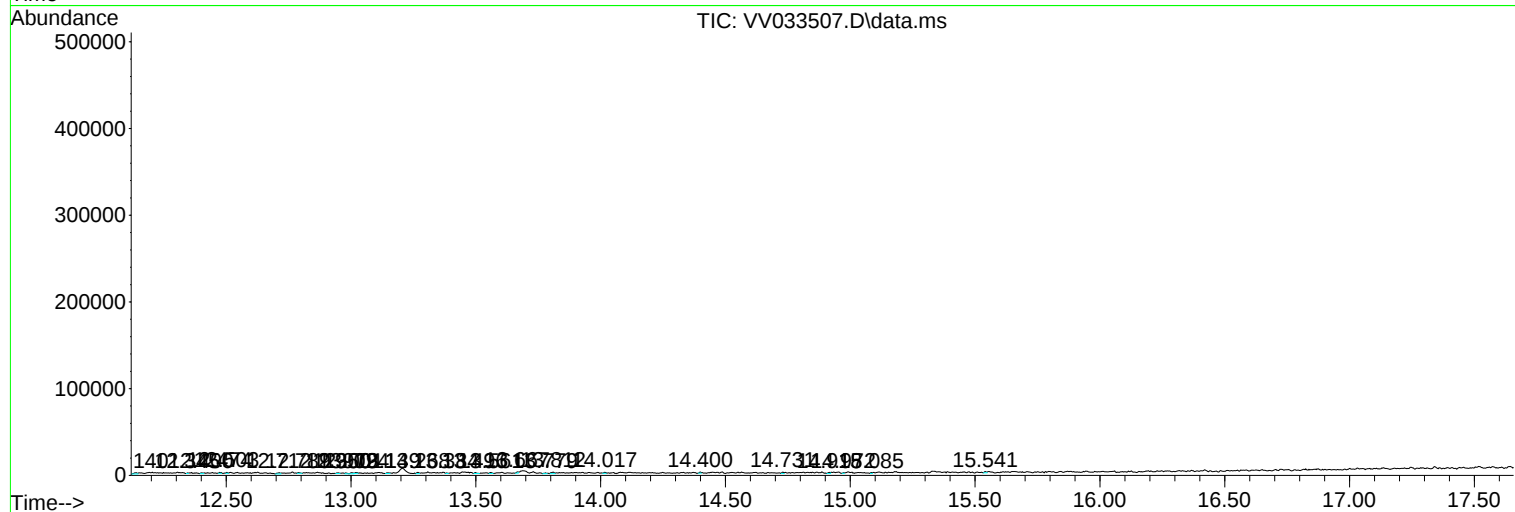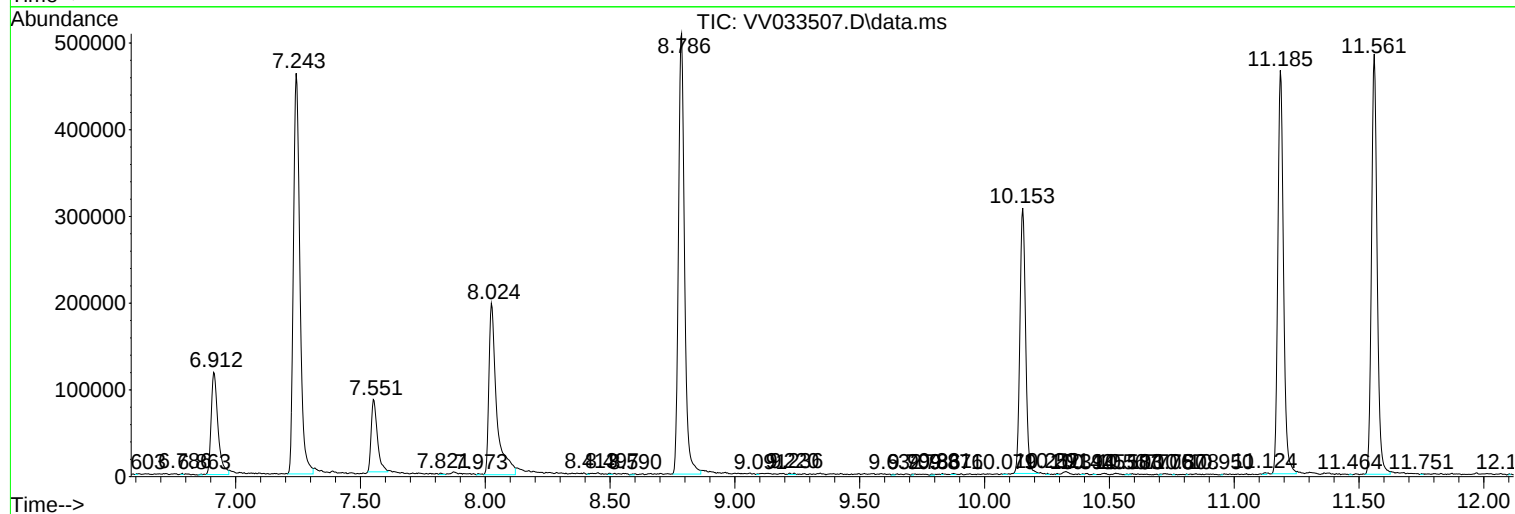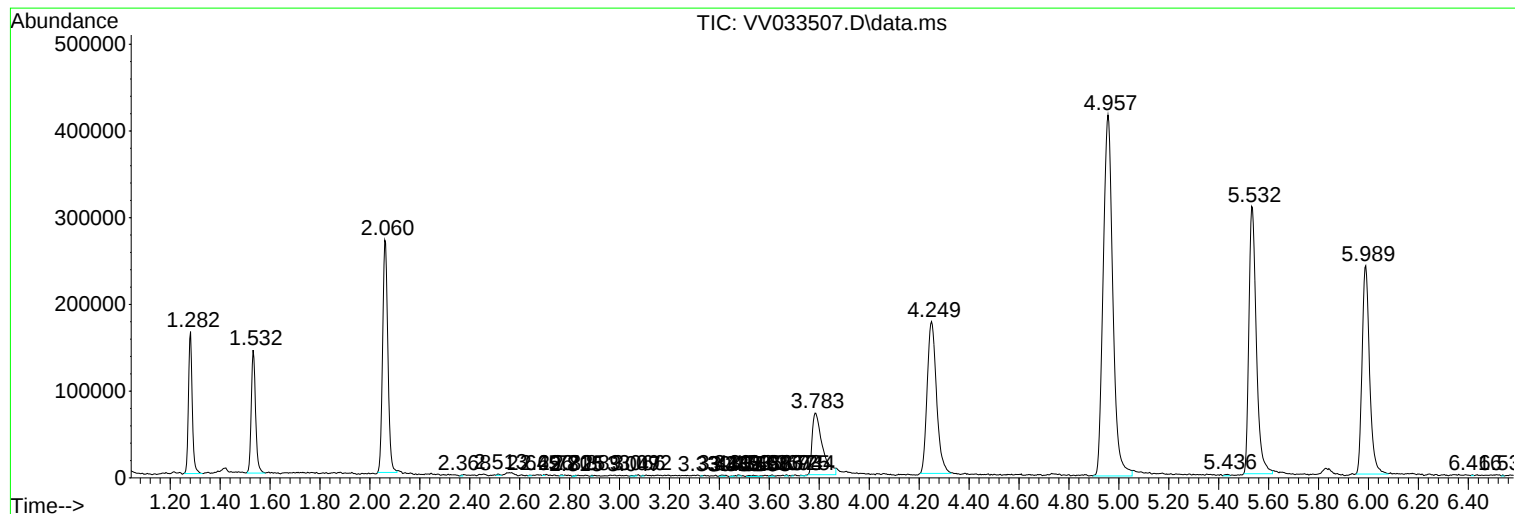

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033507.D
Acq On : 20 Dec 2023 13:23
Operator : SY/MD
Sample : 05850-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033507.D
Acq On : 20 Dec 2023 13:23
Operator : SY/MD
Sample : 05850-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc