

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033508.D
 Acq On : 20 Dec 2023 13:46
 Operator : SY/MD
 Sample : 05850-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	153615	156450	1.88%	0.633%
2	1.532	146	153	168	rVB	139807	165314	1.99%	0.669%
3	2.060	308	317	334	rBV	259970	383668	4.61%	1.552%
4	2.407	423	425	429	rBV4	785	491	0.01%	0.002%
5	2.642	493	498	500	rBV4	962	685	0.01%	0.003%
6	2.677	507	509	512	rBV3	1110	515	0.01%	0.002%
7	2.722	521	523	528	rVB5	1532	1197	0.01%	0.005%
8	2.767	534	537	540	rVV4	969	810	0.01%	0.003%
9	2.796	544	546	549	rVB4	1046	628	0.01%	0.003%
10	2.838	557	559	562	rBV3	791	530	0.01%	0.002%
11	2.857	562	565	568	rVB3	777	557	0.01%	0.002%
12	2.947	591	593	597	rBV4	972	735	0.01%	0.003%
13	2.995	605	608	612	rVB5	1209	713	0.01%	0.003%
14	3.060	626	628	631	rBV3	888	569	0.01%	0.002%
15	3.272	692	694	697	rVB3	1150	659	0.01%	0.003%
16	3.291	697	700	701	rBV2	795	481	0.01%	0.002%
17	3.352	716	719	722	rVB5	1355	927	0.01%	0.004%
18	3.429	740	743	745	rBV5	887	600	0.01%	0.002%
19	3.507	760	767	770	rBV7	989	1068	0.01%	0.004%
20	3.603	792	797	801	rBV5	922	1089	0.01%	0.004%
21	3.783	845	853	881	rBV	57010	162215	1.95%	0.656%
22	4.140	961	964	966	rBV4	1690	1165	0.01%	0.005%
23	4.249	985	998	1027	rVB	173024	442620	5.31%	1.791%
24	4.648	1120	1122	1126	rBV4	926	885	0.01%	0.004%
25	4.706	1138	1140	1143	rBV3	1329	914	0.01%	0.004%
26	4.822	1174	1176	1180	rVB4	1357	780	0.01%	0.003%
27	4.854	1183	1186	1188	rBV4	1330	729	0.01%	0.003%
28	4.957	1202	1218	1227	rBV2	411996	1063381	12.77%	4.302%
29	5.535	1387	1398	1423	rBV	320555	659973	7.92%	2.670%
30	5.989	1527	1539	1560	rBV	238855	493952	5.93%	1.998%
31	6.310	1637	1639	1642	rBV3	1266	1016	0.01%	0.004%
32	6.394	1663	1665	1671	rVB4	1587	1231	0.01%	0.005%
33	6.471	1686	1689	1690	rBV3	1210	677	0.01%	0.003%
34	6.548	1709	1713	1715	rBV5	1058	982	0.01%	0.004%
35	6.609	1729	1732	1734	rVB2	1051	508	0.01%	0.002%
36	6.664	1746	1749	1752	rBV4	1005	717	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033508.D
 Acq On : 20 Dec 2023 13:46
 Operator : SY/MD
 Sample : 05850-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.912	1815	1826	1852	rBV	113848	225242	2.70%	0.911%
38	7.243	1919	1929	1953	rBV	451457	797657	9.58%	3.227%
39	7.555	2016	2026	2043	rBV2	82842	154995	1.86%	0.627%
40	7.982	2157	2159	2162	rBV4	1005	495	0.01%	0.002%
41	8.024	2163	2172	2206	rBV	200622	421426	5.06%	1.705%
42	8.603	2349	2352	2355	rBV3	1822	1511	0.02%	0.006%
43	8.683	2374	2377	2378	rBV3	1188	744	0.01%	0.003%
44	8.725	2388	2390	2395	rVB5	1185	880	0.01%	0.004%
45	8.812	2395	2417	2468	rBV2	4665759	8328091	100.00%	33.693%
46	9.268	2557	2559	2562	rBV4	1294	703	0.01%	0.003%
47	9.413	2600	2604	2606	rBV5	1271	1213	0.01%	0.005%
48	9.471	2620	2622	2624	rBV3	1216	593	0.01%	0.002%
49	9.664	2679	2682	2684	rBV3	1124	514	0.01%	0.002%
50	9.725	2699	2701	2704	rVB3	1156	501	0.01%	0.002%
51	9.751	2708	2709	2712	rBV3	904	463	0.01%	0.002%
52	9.870	2744	2746	2750	rVB4	2161	1509	0.02%	0.006%
53	9.895	2750	2754	2755	rBV3	1166	649	0.01%	0.003%
54	9.918	2758	2761	2762	rBV3	899	546	0.01%	0.002%
55	10.153	2822	2834	2858	rBV	303229	487893	5.86%	1.974%
56	10.249	2861	2864	2867	rBV5	1408	943	0.01%	0.004%
57	10.481	2933	2936	2938	rBV3	1140	697	0.01%	0.003%
58	10.580	2965	2967	2971	rVB5	1315	734	0.01%	0.003%
59	10.628	2979	2982	2984	rVB3	1265	563	0.01%	0.002%
60	10.645	2984	2987	2991	rBV6	1359	1269	0.02%	0.005%
61	10.673	2994	2996	3000	rVB4	916	615	0.01%	0.002%
62	10.751	3016	3020	3022	rVV3	926	745	0.01%	0.003%
63	10.786	3028	3031	3037	rVV7	1406	1233	0.01%	0.005%
64	10.837	3042	3047	3049	rBV6	906	669	0.01%	0.003%
65	10.908	3066	3069	3071	rBV4	939	568	0.01%	0.002%
66	11.117	3120	3134	3145	rBV	232612	361455	4.34%	1.462%
67	11.207	3146	3162	3191	rVB2	2372398	4320617	51.88%	17.480%
68	11.493	3249	3251	3253	rBV3	1476	714	0.01%	0.003%
69	11.577	3258	3277	3296	rBV2	3014585	5276494	63.36%	21.347%
70	11.812	3348	3350	3353	rBV3	1245	625	0.01%	0.003%
71	12.059	3419	3427	3430	rBV7	1338	1428	0.02%	0.006%
72	12.114	3439	3444	3447	rBV7	1424	1354	0.02%	0.005%
73	12.252	3484	3487	3489	rBV4	1390	895	0.01%	0.004%
74	12.509	3565	3567	3569	rBV2	1447	845	0.01%	0.003%
75	12.677	3617	3619	3620	rBV	1724	606	0.01%	0.002%
76	12.760	3644	3645	3648	rBV2	708	484	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033508.D
 Acq On : 20 Dec 2023 13:46
 Operator : SY/MD
 Sample : 05850-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.789	3652	3654	3657	rBV3	781	477	0.01%	0.002%
78	12.853	3673	3674	3679	rVB2	1199	540	0.01%	0.002%
79	12.882	3681	3683	3688	rVB5	1370	804	0.01%	0.003%
80	12.934	3696	3699	3700	rBV2	1043	655	0.01%	0.003%
81	12.992	3715	3717	3723	rVB6	1422	900	0.01%	0.004%
82	13.017	3723	3725	3730	rVB5	1141	805	0.01%	0.003%
83	13.127	3757	3759	3764	rBV6	983	1066	0.01%	0.004%
84	13.197	3770	3781	3800	rBV	398749	620231	7.45%	2.509%
85	13.432	3850	3854	3855	rBV4	1029	774	0.01%	0.003%
86	13.519	3878	3881	3884	rBV5	1409	1043	0.01%	0.004%
87	13.680	3919	3931	3946	rBV	80344	131021	1.57%	0.530%
88	13.950	4013	4015	4019	rBV3	1029	667	0.01%	0.003%
89	13.976	4019	4023	4024	rBV4	1386	839	0.01%	0.003%
90	14.136	4070	4073	4077	rVB5	1833	1310	0.02%	0.005%
91	14.313	4125	4128	4132	rBV4	1149	736	0.01%	0.003%
92	14.342	4134	4137	4141	rBV5	1215	1025	0.01%	0.004%
93	14.374	4145	4147	4149	rBV2	941	549	0.01%	0.002%
94	14.741	4257	4261	4262	rBV4	1538	852	0.01%	0.003%
95	14.844	4291	4293	4296	rBV4	1204	491	0.01%	0.002%
96	14.879	4303	4304	4308	rVB3	975	521	0.01%	0.002%
97	15.030	4348	4351	4356	rBV7	1319	1015	0.01%	0.004%
98	15.159	4388	4391	4393	rVB3	1599	710	0.01%	0.003%
99	15.172	4393	4395	4397	rBV3	973	565	0.01%	0.002%
100	15.297	4428	4434	4437	rBV8	1505	1553	0.02%	0.006%




Sum of corrected areas: 24717758

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033508.D
Acq On : 20 Dec 2023 13:46
Operator : SY/MD
Sample : 05850-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

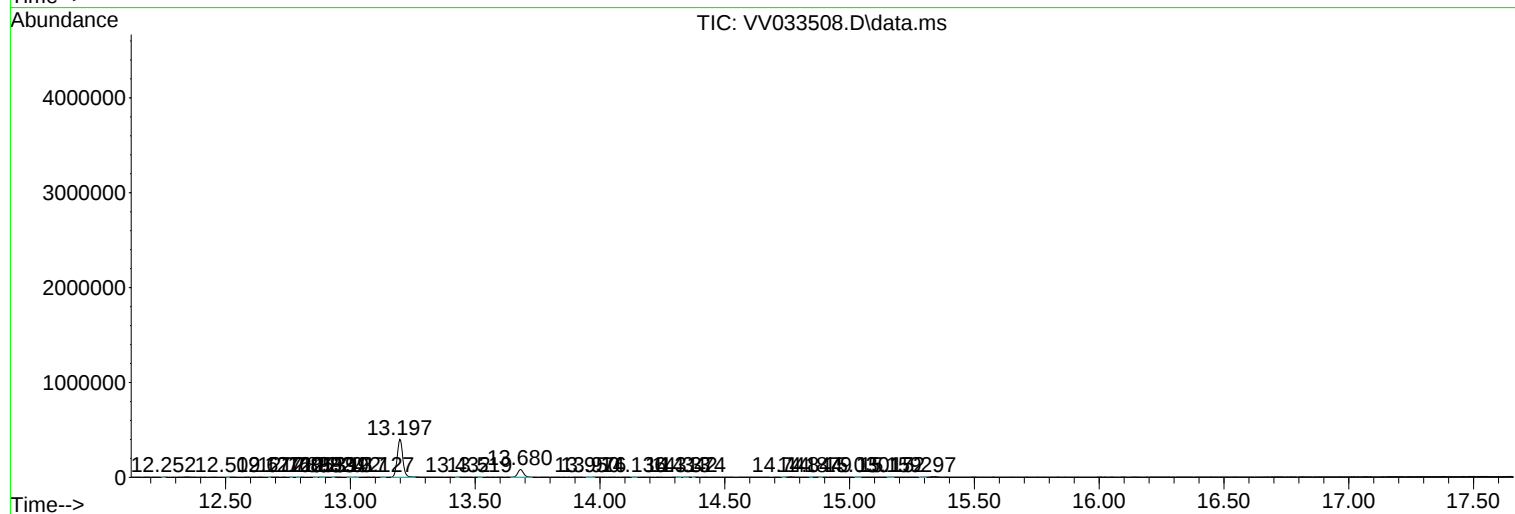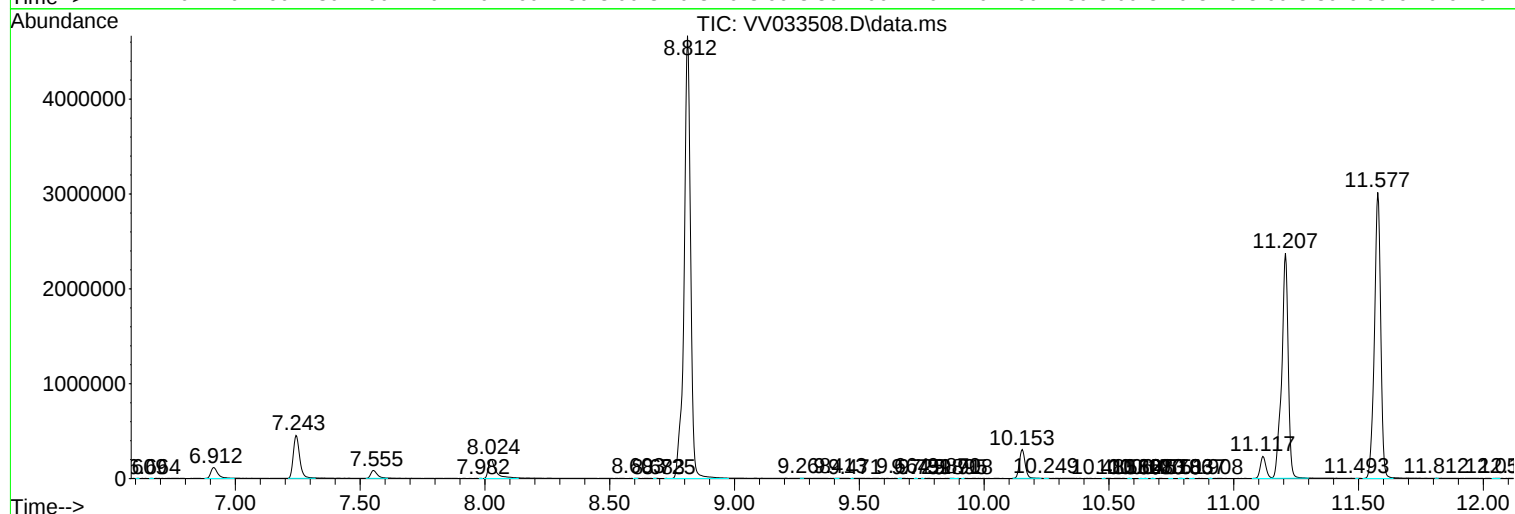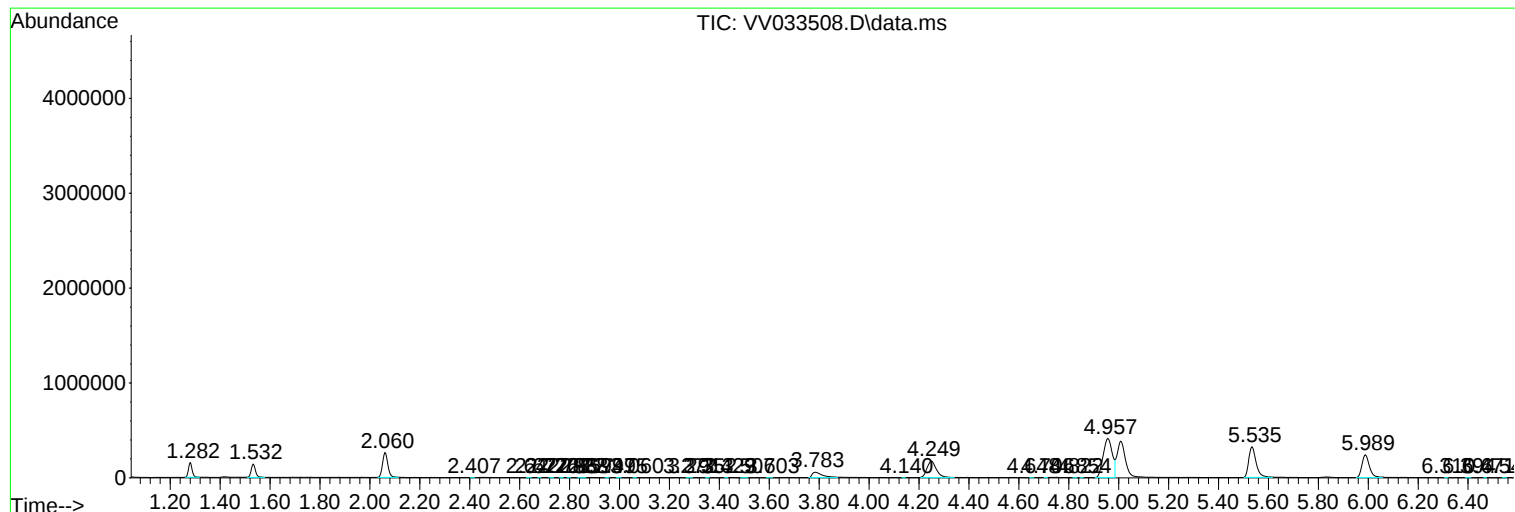

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033508.D
Acq On : 20 Dec 2023 13:46
Operator : SY/MD
Sample : 05850-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033508.D
Acq On : 20 Dec 2023 13:46
Operator : SY/MD
Sample : 05850-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc