

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033509.D
 Acq On : 20 Dec 2023 14:10
 Operator : SY/MD
 Sample : 05927-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	154561	164509	14.90%	1.998%
2	1.532	146	153	168	rVB	136586	161837	14.65%	1.966%
3	2.060	308	317	345	rVB	262942	402485	36.45%	4.889%
4	2.519	458	460	464	rBV4	770	644	0.06%	0.008%
5	2.539	464	466	467	rBV2	931	445	0.04%	0.005%
6	2.693	511	514	516	rBV3	1144	676	0.06%	0.008%
7	2.773	536	539	541	rBV4	1136	710	0.06%	0.009%
8	2.809	547	550	552	rBV2	1552	1066	0.10%	0.013%
9	2.979	600	603	605	rBV3	1402	876	0.08%	0.011%
10	3.053	623	626	629	rBV5	1242	870	0.08%	0.011%
11	3.191	665	669	670	rBV3	1055	768	0.07%	0.009%
12	3.275	693	695	697	rBV2	674	303	0.03%	0.004%
13	3.307	701	705	707	rBV4	863	826	0.07%	0.010%
14	3.529	773	774	775	rBV4	765	258	0.02%	0.003%
15	3.574	785	788	791	rBV4	1116	706	0.06%	0.009%
16	3.613	793	800	803	rVB6	1750	1643	0.15%	0.020%
17	3.629	803	805	808	rVB4	1146	590	0.05%	0.007%
18	3.645	808	810	812	rBV2	747	354	0.03%	0.004%
19	3.680	818	821	822	rBV3	967	493	0.04%	0.006%
20	3.786	845	854	885	rBV2	60616	207034	18.75%	2.515%
21	4.249	983	998	1026	rBV	174764	452117	40.94%	5.492%
22	4.809	1168	1172	1173	rBV4	762	456	0.04%	0.006%
23	4.957	1202	1218	1246	rBV2	411038	1104342	100.00%	13.415%
24	5.532	1386	1397	1422	rBV	307460	649664	58.83%	7.892%
25	5.989	1528	1539	1564	rBV	239264	488749	44.26%	5.937%
26	6.416	1670	1672	1674	rBV3	858	359	0.03%	0.004%
27	6.561	1715	1717	1719	rBV4	740	448	0.04%	0.005%
28	6.850	1805	1807	1810	rVB4	1414	602	0.05%	0.007%
29	6.911	1815	1826	1847	rBV	113885	224482	20.33%	2.727%
30	7.243	1918	1929	1953	rBV	457250	815318	73.83%	9.904%
31	7.555	2017	2026	2046	rBV	83637	153179	13.87%	1.861%
32	8.024	2163	2172	2212	rBV	178797	398508	36.09%	4.841%
33	8.442	2297	2302	2303	rBV4	1696	1151	0.10%	0.014%
34	8.522	2323	2327	2330	rBV6	1576	1235	0.11%	0.015%
35	8.622	2356	2358	2359	rBV2	1624	552	0.05%	0.007%
36	8.786	2398	2409	2432	rBV	501449	871440	78.91%	10.586%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033509.D
 Acq On : 20 Dec 2023 14:10
 Operator : SY/MD
 Sample : 05927-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.140	2518	2519	2522	rVB2	1194	522	0.05%	0.006%
38	9.165	2525	2527	2529	rBV2	1117	552	0.05%	0.007%
39	9.252	2551	2554	2555	rBV3	1135	530	0.05%	0.006%
40	9.316	2573	2574	2577	rBV2	1118	497	0.05%	0.006%
41	9.387	2592	2596	2599	rBV5	1346	868	0.08%	0.011%
42	9.616	2664	2667	2668	rBV3	844	458	0.04%	0.006%
43	9.657	2676	2680	2682	rBV4	1189	850	0.08%	0.010%
44	9.683	2687	2688	2690	rBV2	1303	541	0.05%	0.007%
45	9.754	2708	2710	2714	rVB5	1477	923	0.08%	0.011%
46	9.776	2714	2717	2719	rBV2	950	549	0.05%	0.007%
47	9.889	2749	2752	2755	rBV4	1267	993	0.09%	0.012%
48	9.924	2761	2763	2765	rBV3	1006	493	0.04%	0.006%
49	10.056	2800	2804	2806	rBV4	1430	1102	0.10%	0.013%
50	10.152	2822	2834	2848	rBV	305093	484211	43.85%	5.882%
51	10.316	2880	2885	2888	rBV6	2334	2783	0.25%	0.034%
52	10.522	2947	2949	2951	rBV2	1196	689	0.06%	0.008%
53	10.683	2997	2999	3001	rBV3	685	307	0.03%	0.004%
54	10.744	3014	3018	3020	rBV3	969	770	0.07%	0.009%
55	10.853	3051	3052	3054	rBV2	943	374	0.03%	0.005%
56	10.943	3078	3080	3082	rBV3	1096	439	0.04%	0.005%
57	10.988	3091	3094	3095	rBV3	1152	527	0.05%	0.006%
58	11.130	3130	3138	3145	rVV3	3572	6609	0.60%	0.080%
59	11.185	3145	3155	3183	rVV	468483	772079	69.91%	9.379%
60	11.561	3261	3272	3293	rBV	475245	791233	71.65%	9.612%
61	11.911	3378	3381	3384	rBV5	1160	1123	0.10%	0.014%
62	11.969	3396	3399	3403	rBV5	1212	1119	0.10%	0.014%
63	12.024	3412	3416	3418	rBV6	920	837	0.08%	0.010%
64	12.101	3437	3440	3443	rBV3	1254	783	0.07%	0.010%
65	12.239	3481	3483	3484	rBV2	894	334	0.03%	0.004%
66	12.307	3502	3504	3508	rBV6	1233	931	0.08%	0.011%
67	12.368	3522	3523	3525	rBV	924	387	0.04%	0.005%
68	12.419	3537	3539	3540	rBV2	983	328	0.03%	0.004%
69	12.451	3547	3549	3552	rBV2	905	546	0.05%	0.007%
70	12.522	3567	3571	3572	rBV4	1254	989	0.09%	0.012%
71	12.558	3580	3582	3584	rBV2	747	253	0.02%	0.003%
72	12.622	3600	3602	3605	rVB4	1543	889	0.08%	0.011%
73	12.667	3614	3616	3617	rBV	551	254	0.02%	0.003%
74	12.680	3618	3620	3623	rVB4	1353	614	0.06%	0.007%
75	12.696	3623	3625	3627	rBV	551	236	0.02%	0.003%
76	12.715	3629	3631	3632	rBV	755	234	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033509.D
 Acq On : 20 Dec 2023 14:10
 Operator : SY/MD
 Sample : 05927-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.734	3636	3637	3638	rBV	720	240	0.02%	0.003%
78	12.792	3653	3655	3656	rBV	955	293	0.03%	0.004%
79	12.837	3665	3669	3673	rVB6	1368	1422	0.13%	0.017%
80	12.992	3714	3717	3719	rBV3	1036	807	0.07%	0.010%
81	13.024	3725	3727	3728	rBV2	1059	431	0.04%	0.005%
82	13.136	3759	3762	3770	rBV8	1224	1232	0.11%	0.015%
83	13.168	3770	3772	3773	rVV2	1115	428	0.04%	0.005%
84	13.201	3775	3782	3794	rVV5	15168	25570	2.32%	0.311%
85	13.258	3798	3800	3803	rBV4	888	551	0.05%	0.007%
86	13.281	3803	3807	3808	rBV3	1228	884	0.08%	0.011%
87	13.326	3818	3821	3823	rBV3	1194	761	0.07%	0.009%
88	13.377	3834	3837	3840	rBV4	1714	1073	0.10%	0.013%
89	13.522	3877	3882	3885	rBV6	1602	1480	0.13%	0.018%
90	13.895	3994	3998	4001	rBV5	1220	1037	0.09%	0.013%
91	14.030	4039	4040	4042	rBV2	894	382	0.03%	0.005%
92	14.059	4047	4049	4055	rVB5	1043	837	0.08%	0.010%
93	14.088	4055	4058	4062	rBV7	1010	996	0.09%	0.012%
94	14.210	4093	4096	4099	rBV4	1009	888	0.08%	0.011%
95	14.339	4134	4136	4138	rBV2	1254	589	0.05%	0.007%
96	14.397	4152	4154	4155	rBV2	727	319	0.03%	0.004%
97	14.638	4226	4229	4231	rBV4	815	568	0.05%	0.007%
98	15.133	4381	4383	4385	rBV3	1107	479	0.04%	0.006%
99	15.265	4422	4424	4426	rBV3	1455	760	0.07%	0.009%
100	15.432	4473	4476	4481	rBV7	1534	1550	0.14%	0.019%




Sum of corrected areas: 8232028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033509.D
Acq On : 20 Dec 2023 14:10
Operator : SY/MD
Sample : 05927-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

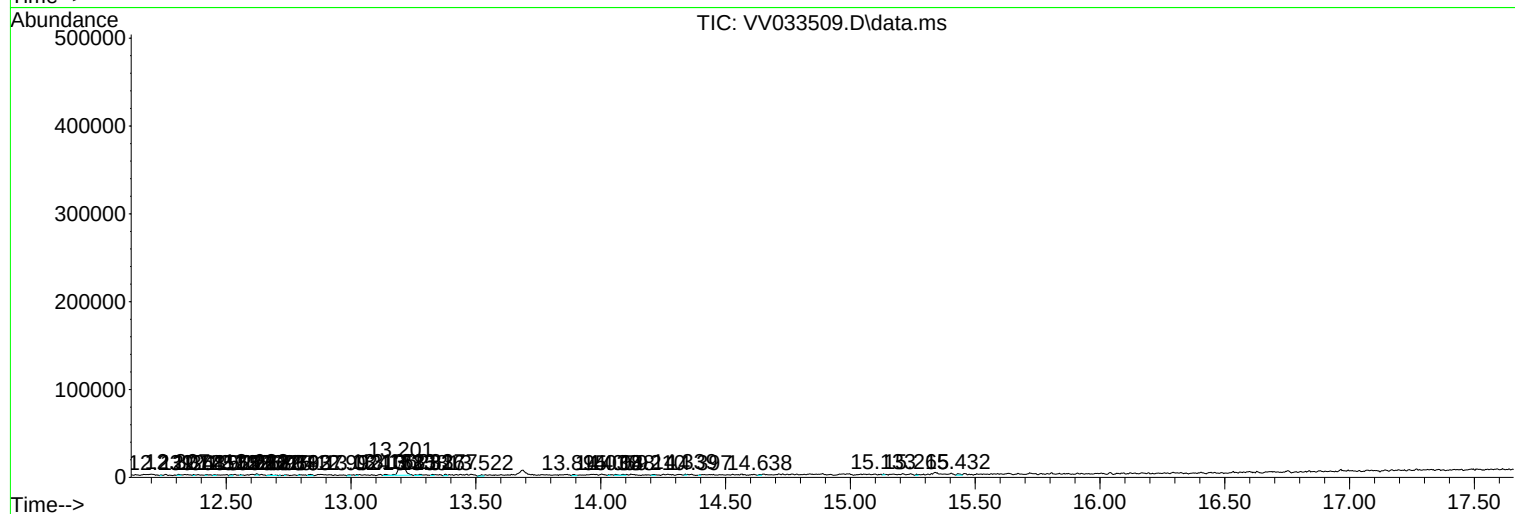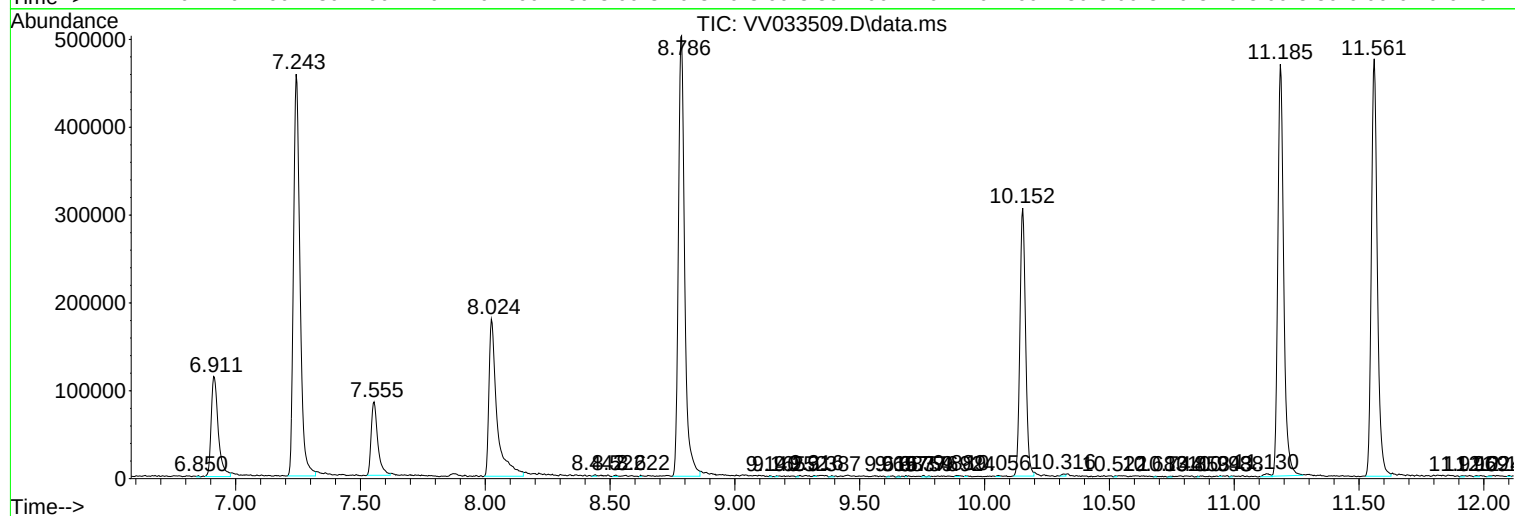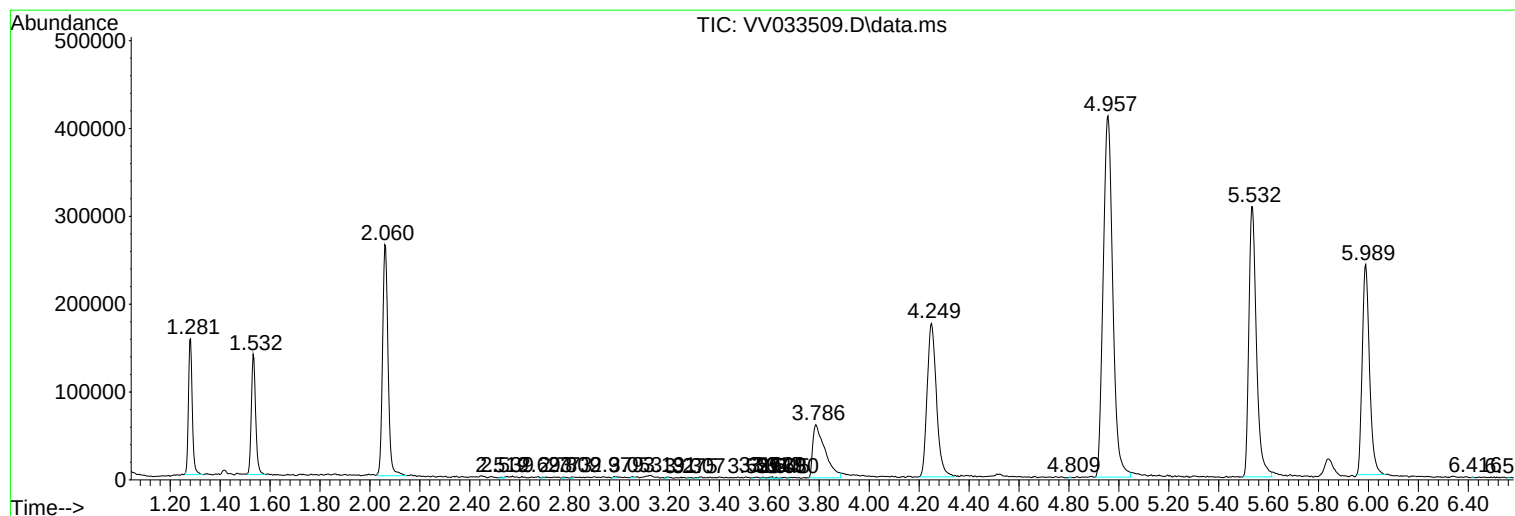

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033509.D
Acq On : 20 Dec 2023 14:10
Operator : SY/MD
Sample : 05927-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033509.D
Acq On : 20 Dec 2023 14:10
Operator : SY/MD
Sample : 05927-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------