

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033510.D
 Acq On : 20 Dec 2023 14:33
 Operator : SY/MD
 Sample : 05927-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	150522	160364	15.04%	1.965%
2	1.532	147	153	170	rVB	136772	165754	15.55%	2.031%
3	2.060	308	317	331	rBV	254213	378420	35.49%	4.636%
4	2.400	421	423	424	rBV2	1396	586	0.05%	0.007%
5	2.719	520	522	525	rVB3	1101	546	0.05%	0.007%
6	2.764	533	536	538	rBV4	1017	712	0.07%	0.009%
7	2.863	566	567	570	rVB2	1065	497	0.05%	0.006%
8	2.883	570	573	574	rBV2	1568	802	0.08%	0.010%
9	3.275	692	695	700	rVB7	1273	1062	0.10%	0.013%
10	3.298	700	702	706	rVB4	1115	652	0.06%	0.008%
11	3.336	711	714	716	rVB4	879	531	0.05%	0.007%
12	3.355	716	720	723	rBV4	1292	1093	0.10%	0.013%
13	3.458	750	752	755	rVB2	1471	737	0.07%	0.009%
14	3.478	755	758	763	rBV5	1299	1133	0.11%	0.014%
15	3.571	783	787	789	rBV5	1162	897	0.08%	0.011%
16	3.609	796	799	801	rBV4	1307	873	0.08%	0.011%
17	3.786	842	854	879	rBV3	94784	293531	27.53%	3.596%
18	4.249	985	998	1025	rVB	169796	430043	40.34%	5.269%
19	4.654	1121	1124	1125	rBV3	1130	722	0.07%	0.009%
20	4.706	1139	1140	1142	rBV	1191	659	0.06%	0.008%
21	4.764	1153	1158	1160	rBV3	1539	1236	0.12%	0.015%
22	4.815	1169	1174	1175	rBV5	1249	987	0.09%	0.012%
23	4.854	1183	1186	1189	rBV4	1363	898	0.08%	0.011%
24	4.876	1189	1193	1195	rBV6	1054	837	0.08%	0.010%
25	4.899	1198	1200	1202	rBV3	1236	679	0.06%	0.008%
26	4.957	1202	1218	1243	rBV2	400987	1066129	100.00%	13.061%
27	5.535	1386	1398	1431	rBV	314229	668619	62.71%	8.191%
28	5.989	1528	1539	1559	rBV2	233190	486404	45.62%	5.959%
29	6.484	1689	1693	1695	rBV4	1128	955	0.09%	0.012%
30	6.513	1700	1702	1705	rVV4	944	575	0.05%	0.007%
31	6.535	1705	1709	1713	rVB7	1616	1249	0.12%	0.015%
32	6.764	1777	1780	1782	rBV3	1588	995	0.09%	0.012%
33	6.847	1801	1806	1807	rBV4	1115	751	0.07%	0.009%
34	6.915	1817	1827	1850	rBV	112139	217623	20.41%	2.666%
35	7.185	1909	1911	1913	rBV3	1053	586	0.05%	0.007%
36	7.243	1919	1929	1958	rBV	443066	794466	74.52%	9.733%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033510.D
 Acq On : 20 Dec 2023 14:33
 Operator : SY/MD
 Sample : 05927-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.555	2017	2026	2047	rBV2	78691	149756	14.05%	1.835%
38	7.841	2111	2115	2118	rBV5	1696	1682	0.16%	0.021%
39	7.908	2134	2136	2140	rVB5	1875	1094	0.10%	0.013%
40	7.979	2157	2158	2161	rBV3	1041	561	0.05%	0.007%
41	8.024	2163	2172	2205	rBV	189240	410009	38.46%	5.023%
42	8.407	2286	2291	2292	rBV5	1931	1543	0.14%	0.019%
43	8.526	2322	2328	2330	rBV5	1592	1597	0.15%	0.020%
44	8.641	2359	2364	2365	rBV5	923	680	0.06%	0.008%
45	8.783	2398	2408	2433	rBV	518412	869390	81.55%	10.651%
46	8.976	2465	2468	2470	rBV4	2010	1357	0.13%	0.017%
47	9.423	2604	2607	2608	rBV3	1233	611	0.06%	0.007%
48	9.571	2650	2653	2657	rBV6	1089	861	0.08%	0.011%
49	9.715	2695	2698	2700	rBV3	1111	668	0.06%	0.008%
50	9.776	2710	2717	2718	rBV6	1109	1066	0.10%	0.013%
51	9.815	2724	2729	2732	rBV5	936	880	0.08%	0.011%
52	9.889	2750	2752	2756	rBV5	1224	691	0.06%	0.008%
53	9.963	2772	2775	2776	rVB3	1249	536	0.05%	0.007%
54	10.072	2806	2809	2812	rBV5	1427	1325	0.12%	0.016%
55	10.153	2822	2834	2850	rBV	304041	485243	45.51%	5.945%
56	10.378	2901	2904	2906	rVB4	1150	696	0.07%	0.009%
57	10.397	2906	2910	2911	rBV4	1354	1047	0.10%	0.013%
58	10.487	2936	2938	2942	rVB4	1505	877	0.08%	0.011%
59	10.574	2961	2965	2966	rBV3	1112	725	0.07%	0.009%
60	10.644	2983	2987	2988	rBV4	1280	589	0.06%	0.007%
61	10.773	3022	3027	3029	rBV5	1236	960	0.09%	0.012%
62	10.796	3031	3034	3038	rBV5	1323	970	0.09%	0.012%
63	10.947	3079	3081	3086	rVV6	1463	1176	0.11%	0.014%
64	10.982	3090	3092	3096	rVB2	1456	874	0.08%	0.011%
65	11.014	3100	3102	3107	rVB6	895	542	0.05%	0.007%
66	11.185	3144	3155	3177	rBV	481566	756954	71.00%	9.274%
67	11.561	3261	3272	3293	rBV	462575	744746	69.86%	9.124%
68	11.744	3327	3329	3330	rBV2	1410	549	0.05%	0.007%
69	11.985	3401	3404	3407	rBV4	1332	871	0.08%	0.011%
70	12.001	3407	3409	3411	rBV3	1075	654	0.06%	0.008%
71	12.046	3419	3423	3425	rBV5	1161	954	0.09%	0.012%
72	12.152	3451	3456	3459	rBV6	1712	1350	0.13%	0.017%
73	12.204	3467	3472	3476	rBV5	1622	1835	0.17%	0.022%
74	12.384	3525	3528	3533	rVB4	1634	1217	0.11%	0.015%
75	12.426	3538	3541	3543	rBV3	1004	573	0.05%	0.007%
76	12.725	3629	3634	3636	rBV4	1158	1211	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033510.D
 Acq On : 20 Dec 2023 14:33
 Operator : SY/MD
 Sample : 05927-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.847	3670	3672	3676	rVV4	971	652	0.06%	0.008%
78	12.866	3676	3678	3682	rVB4	1192	505	0.05%	0.006%
79	12.972	3709	3711	3716	rVB5	1051	800	0.08%	0.010%
80	13.001	3716	3720	3723	rBV5	1058	815	0.08%	0.010%
81	13.088	3743	3747	3751	rBV5	1375	979	0.09%	0.012%
82	13.117	3755	3756	3761	rVV5	1068	663	0.06%	0.008%
83	13.149	3764	3766	3768	rBV2	1064	515	0.05%	0.006%
84	13.207	3776	3784	3792	rBV10	6013	9334	0.88%	0.114%
85	13.268	3801	3803	3805	rBV3	952	573	0.05%	0.007%
86	13.361	3827	3832	3834	rVB7	1044	774	0.07%	0.009%
87	13.683	3926	3932	3933	rBV4	2569	2109	0.20%	0.026%
88	13.763	3954	3957	3958	rBV3	808	527	0.05%	0.006%
89	13.792	3962	3966	3969	rBV4	1419	1059	0.10%	0.013%
90	13.824	3974	3976	3978	rBV3	1093	603	0.06%	0.007%
91	13.988	4022	4027	4031	rBV7	1241	1114	0.10%	0.014%
92	14.008	4031	4033	4036	rBV4	1009	658	0.06%	0.008%
93	14.181	4083	4087	4090	rBV4	1260	1181	0.11%	0.014%
94	14.265	4109	4113	4117	rBV7	1486	1233	0.12%	0.015%
95	14.451	4168	4171	4176	rBV7	1662	1310	0.12%	0.016%
96	14.812	4278	4283	4284	rBV3	1424	1068	0.10%	0.013%
97	14.847	4290	4294	4297	rBV5	1940	1796	0.17%	0.022%
98	14.911	4311	4314	4316	rBV3	988	616	0.06%	0.008%
99	14.940	4321	4323	4329	rVB7	1503	1222	0.11%	0.015%
100	15.242	4413	4417	4418	rBV4	1472	826	0.08%	0.010%




Sum of corrected areas: 8162455

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033510.D
Acq On : 20 Dec 2023 14:33
Operator : SY/MD
Sample : 05927-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

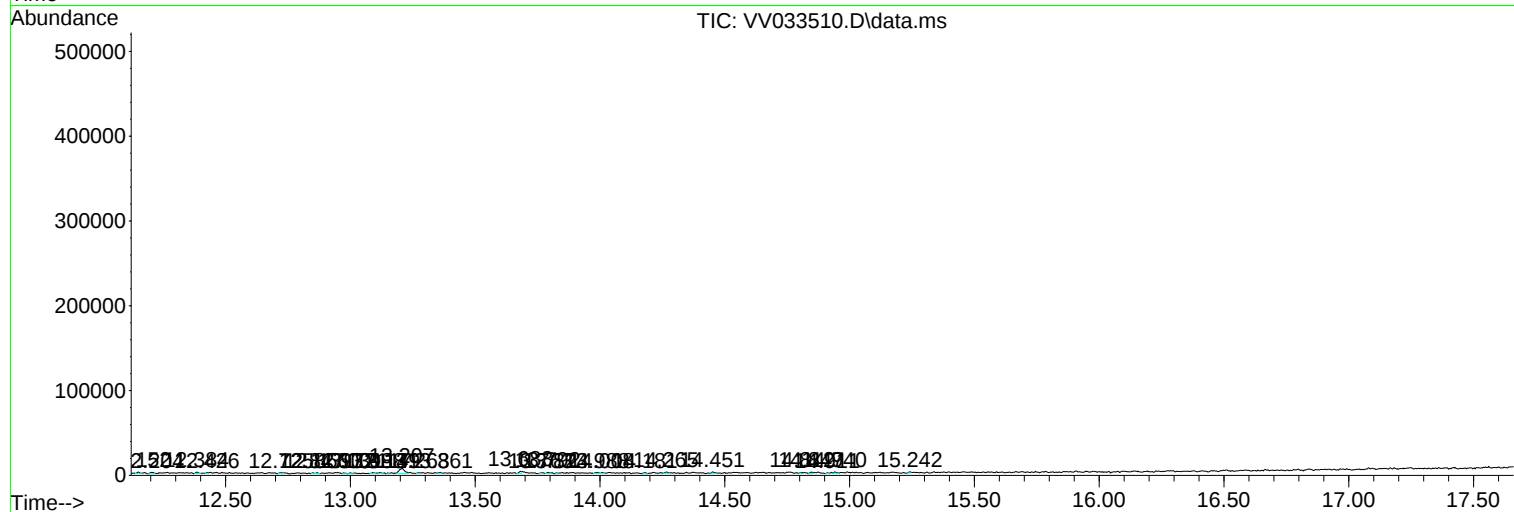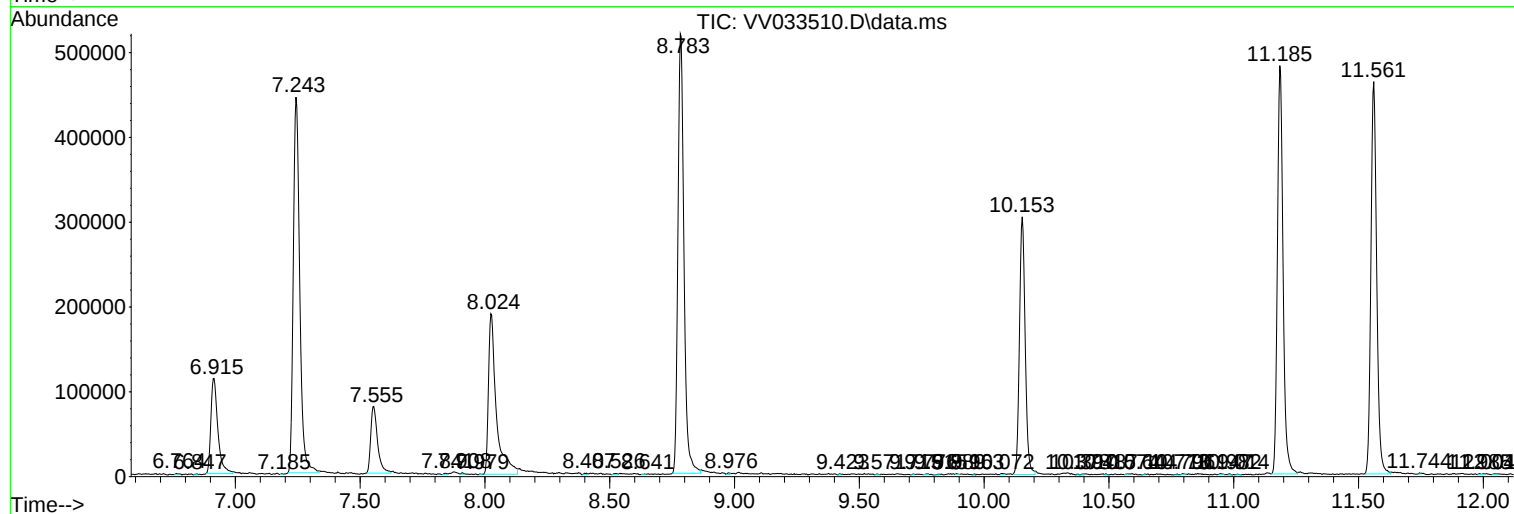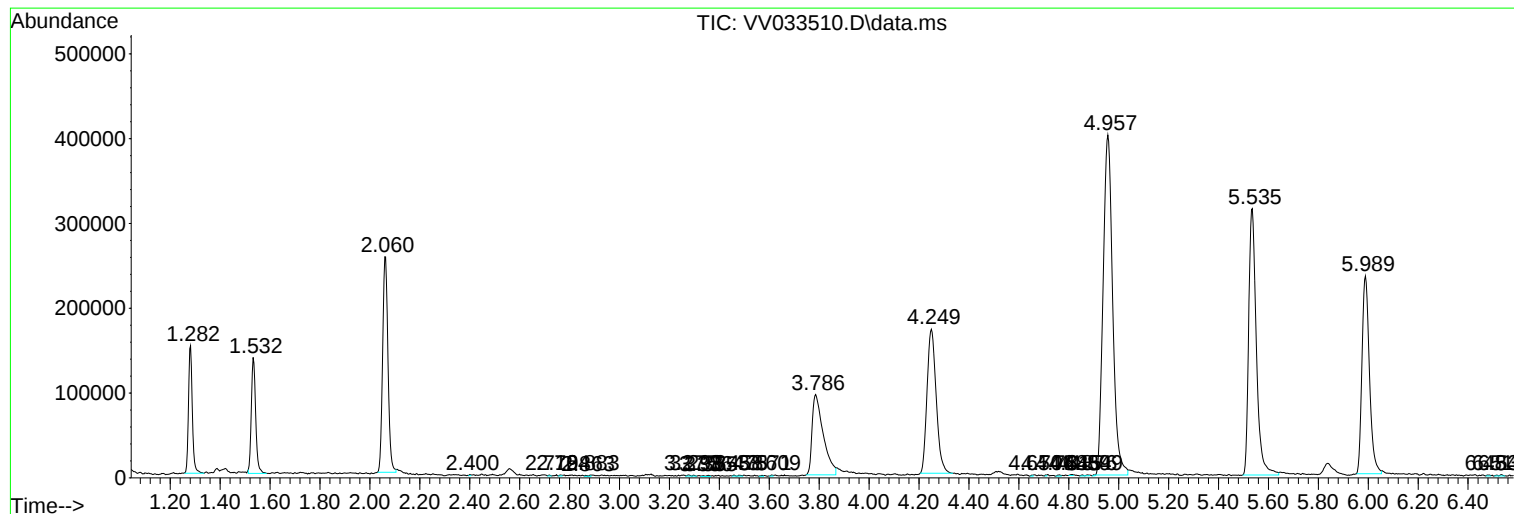

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033510.D
Acq On : 20 Dec 2023 14:33
Operator : SY/MD
Sample : 05927-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033510.D
Acq On : 20 Dec 2023 14:33
Operator : SY/MD
Sample : 05927-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------