

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033511.D
 Acq On : 20 Dec 2023 14:56
 Operator : SY/MD
 Sample : 05927-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	156814	162825	15.25%	1.995%
2	1.532	146	153	166	rVB	138691	162179	15.19%	1.987%
3	2.059	308	317	334	rBV	257596	378301	35.42%	4.634%
4	2.561	459	473	484	rBV	10484	24145	2.26%	0.296%
5	2.664	504	505	509	rVB5	1051	579	0.05%	0.007%
6	2.690	509	513	515	rBV4	1477	1055	0.10%	0.013%
7	2.767	534	537	539	rBV2	979	467	0.04%	0.006%
8	2.796	543	546	548	rBV3	1271	722	0.07%	0.009%
9	2.809	548	550	555	rVB5	1237	675	0.06%	0.008%
10	2.838	557	559	562	rVB4	1095	467	0.04%	0.006%
11	2.854	562	564	565	rBV2	940	539	0.05%	0.007%
12	2.960	593	597	599	rBV4	994	765	0.07%	0.009%
13	2.982	602	604	607	rBV3	1403	768	0.07%	0.009%
14	3.053	619	626	631	rVB8	1897	2670	0.25%	0.033%
15	3.088	631	637	639	rBV6	1930	1540	0.14%	0.019%
16	3.175	662	664	669	rVB4	1147	612	0.06%	0.007%
17	3.204	669	673	677	rBV5	1272	986	0.09%	0.012%
18	3.307	702	705	708	rVB5	1215	886	0.08%	0.011%
19	3.336	711	714	717	rBV4	885	632	0.06%	0.008%
20	3.407	732	736	738	rBV4	1306	796	0.07%	0.010%
21	3.471	753	756	759	rBV3	698	637	0.06%	0.008%
22	3.522	769	772	773	rBV2	959	429	0.04%	0.005%
23	3.558	781	783	785	rVB3	1239	477	0.04%	0.006%
24	3.590	789	793	795	rBV3	993	679	0.06%	0.008%
25	3.696	824	826	828	rBV3	989	453	0.04%	0.006%
26	3.786	839	854	890	rBV3	104360	348510	32.63%	4.269%
27	4.249	984	998	1026	rVB	171372	435855	40.81%	5.339%
28	4.715	1141	1143	1144	rBV2	1145	468	0.04%	0.006%
29	4.773	1158	1161	1166	rBV5	1280	1164	0.11%	0.014%
30	4.956	1202	1218	1244	rBV3	399899	1067965	100.00%	13.082%
31	5.362	1342	1344	1347	rBV4	1324	687	0.06%	0.008%
32	5.535	1386	1398	1423	rBV	310271	650555	60.92%	7.969%
33	5.989	1527	1539	1559	rBV	232958	486014	45.51%	5.954%
34	6.497	1693	1697	1700	rBV4	1912	2024	0.19%	0.025%
35	6.702	1759	1761	1765	rBV5	887	511	0.05%	0.006%
36	6.776	1782	1784	1790	rBV6	731	589	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033511.D
 Acq On : 20 Dec 2023 14:56
 Operator : SY/MD
 Sample : 05927-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.847	1804	1806	1809	rVV4	863	644	0.06%	0.008%
38	6.915	1817	1827	1851	rBV	110928	216018	20.23%	2.646%
39	7.243	1918	1929	1952	rBV	446728	790794	74.05%	9.687%
40	7.554	2015	2026	2040	rBV	81675	150291	14.07%	1.841%
41	8.024	2163	2172	2203	rBV	185790	400057	37.46%	4.901%
42	8.410	2290	2292	2295	rBV4	1443	760	0.07%	0.009%
43	8.587	2344	2347	2350	rBV5	1308	970	0.09%	0.012%
44	8.786	2398	2409	2429	rBV	513949	849061	79.50%	10.401%
45	9.358	2585	2587	2589	rBV2	1136	416	0.04%	0.005%
46	9.397	2597	2599	2602	rBV3	1241	700	0.07%	0.009%
47	9.435	2609	2611	2615	rBV4	1270	860	0.08%	0.011%
48	9.455	2615	2617	2620	rVV3	861	431	0.04%	0.005%
49	9.738	2703	2705	2711	rVB5	1050	646	0.06%	0.008%
50	9.812	2725	2728	2730	rBV3	617	520	0.05%	0.006%
51	9.873	2746	2747	2751	rVB3	1188	497	0.05%	0.006%
52	10.005	2785	2788	2790	rBV3	1371	760	0.07%	0.009%
53	10.075	2808	2810	2813	rVB3	1471	766	0.07%	0.009%
54	10.095	2813	2816	2819	rBV3	1159	902	0.08%	0.011%
55	10.152	2823	2834	2856	rVB	302583	482938	45.22%	5.916%
56	10.509	2942	2945	2950	rBV8	1275	1056	0.10%	0.013%
57	10.529	2950	2951	2954	rVB2	1157	433	0.04%	0.005%
58	10.654	2987	2990	2993	rBV5	1157	950	0.09%	0.012%
59	10.738	3014	3016	3019	rBV3	1335	733	0.07%	0.009%
60	10.754	3019	3021	3027	rVB6	656	489	0.05%	0.006%
61	10.876	3055	3059	3064	rBV7	1740	1685	0.16%	0.021%
62	10.908	3064	3069	3071	rBV5	1407	1026	0.10%	0.013%
63	10.982	3089	3092	3096	rVB4	968	781	0.07%	0.010%
64	11.021	3102	3104	3108	rBV4	1367	999	0.09%	0.012%
65	11.069	3117	3119	3122	rVB4	1462	728	0.07%	0.009%
66	11.091	3122	3126	3127	rBV3	791	495	0.05%	0.006%
67	11.120	3131	3135	3136	rBV3	1314	922	0.09%	0.011%
68	11.185	3144	3155	3174	rBV	476033	747481	69.99%	9.156%
69	11.490	3245	3250	3252	rBV5	1101	951	0.09%	0.012%
70	11.561	3259	3272	3290	rBV	460621	739913	69.28%	9.064%
71	12.066	3426	3429	3431	rBV3	1469	1019	0.10%	0.012%
72	12.114	3440	3444	3445	rBV3	784	565	0.05%	0.007%
73	12.188	3464	3467	3470	rVV4	1012	795	0.07%	0.010%
74	12.204	3470	3472	3475	rBV4	1357	680	0.06%	0.008%
75	12.268	3486	3492	3494	rBV6	1142	1399	0.13%	0.017%
76	12.307	3497	3504	3507	rVB9	1336	1543	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033511.D
 Acq On : 20 Dec 2023 14:56
 Operator : SY/MD
 Sample : 05927-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.326	3507	3510	3511	rBV3	1211	719	0.07%	0.009%
78	12.429	3540	3542	3545	rBV4	1625	645	0.06%	0.008%
79	12.516	3564	3569	3570	rBV3	751	686	0.06%	0.008%
80	12.548	3575	3579	3580	rBV5	947	637	0.06%	0.008%
81	12.680	3616	3620	3622	rBV5	1367	1185	0.11%	0.015%
82	12.728	3631	3635	3639	rVB6	1424	1281	0.12%	0.016%
83	12.750	3639	3642	3643	rBV2	949	450	0.04%	0.006%
84	13.136	3761	3762	3766	rBV2	1030	558	0.05%	0.007%
85	13.294	3809	3811	3814	rVB2	985	417	0.04%	0.005%
86	13.368	3830	3834	3835	rBV4	1028	758	0.07%	0.009%
87	13.493	3871	3873	3874	rBV2	951	485	0.05%	0.006%
88	13.538	3884	3887	3891	rBV6	1518	1045	0.10%	0.013%
89	13.943	4009	4013	4014	rBV2	1652	1068	0.10%	0.013%
90	14.040	4041	4043	4044	rBV	897	487	0.05%	0.006%
91	14.284	4115	4119	4122	rBV3	1032	885	0.08%	0.011%
92	14.426	4159	4163	4165	rBV4	1463	1121	0.10%	0.014%
93	14.477	4175	4179	4182	rBV5	1246	1176	0.11%	0.014%
94	14.503	4186	4187	4189	rBV2	1077	477	0.04%	0.006%
95	14.577	4209	4210	4212	rBV2	923	467	0.04%	0.006%
96	14.834	4288	4290	4292	rBV2	894	461	0.04%	0.006%
97	14.882	4303	4305	4307	rBV2	851	427	0.04%	0.005%
98	14.940	4320	4323	4325	rBV3	1273	669	0.06%	0.008%
99	15.030	4349	4351	4354	rBV4	859	614	0.06%	0.008%
100	15.297	4430	4434	4439	rBV	6235	5475	0.51%	0.067%




Sum of corrected areas: 8163493

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033511.D
Acq On : 20 Dec 2023 14:56
Operator : SY/MD
Sample : 05927-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

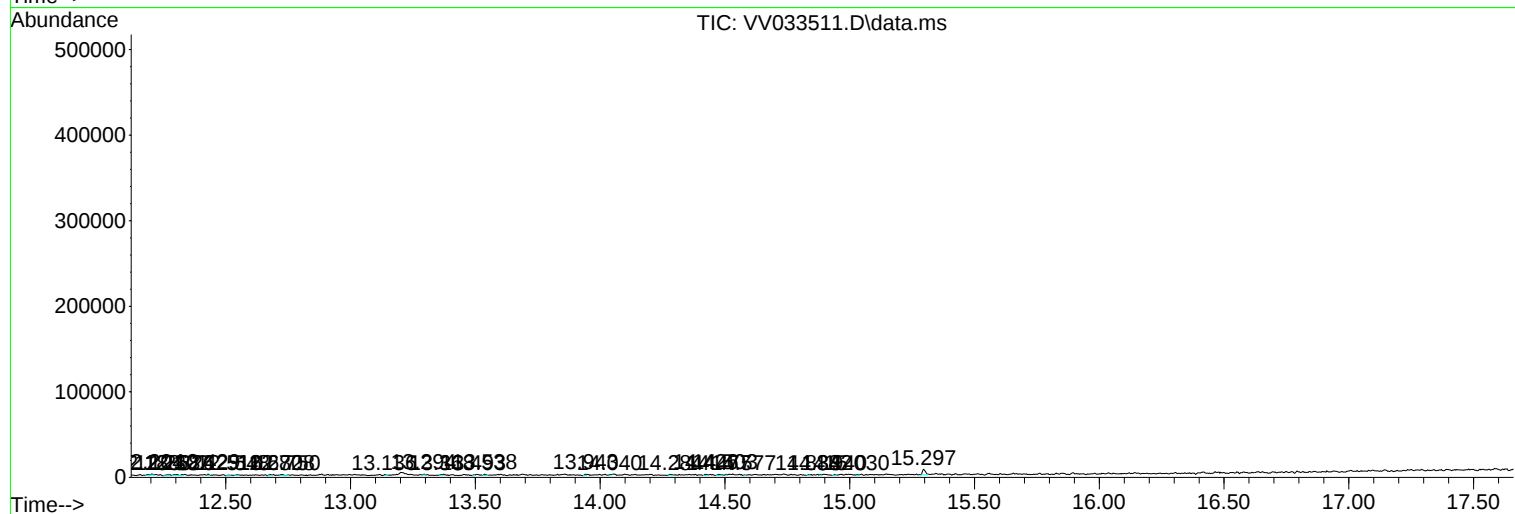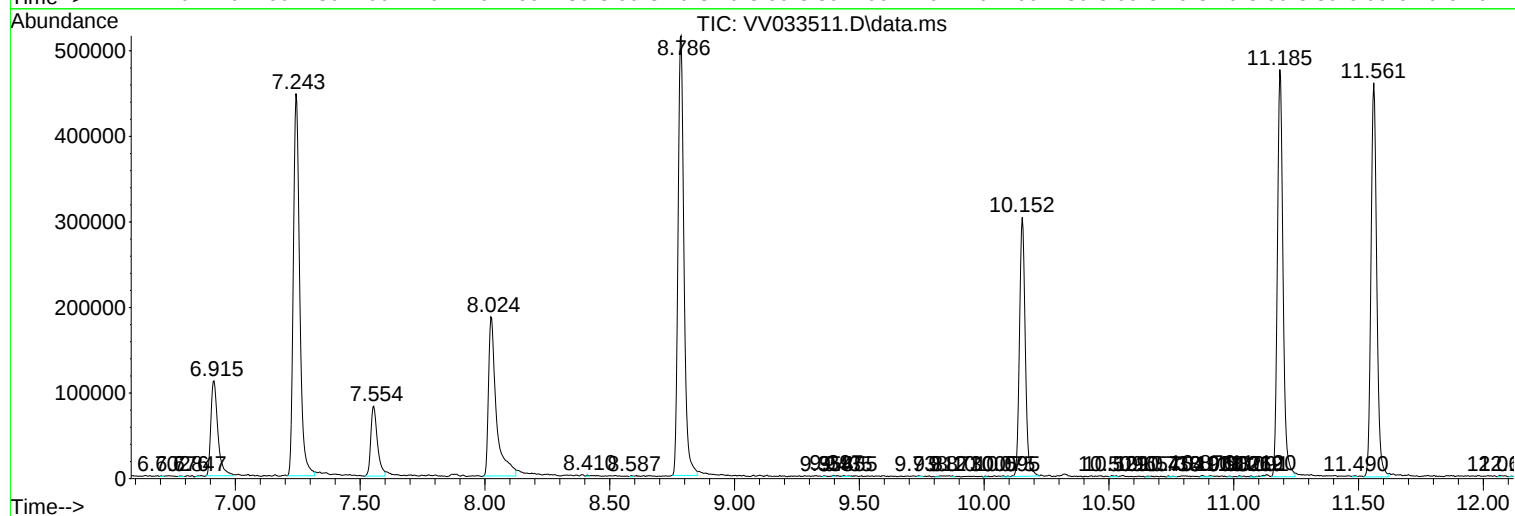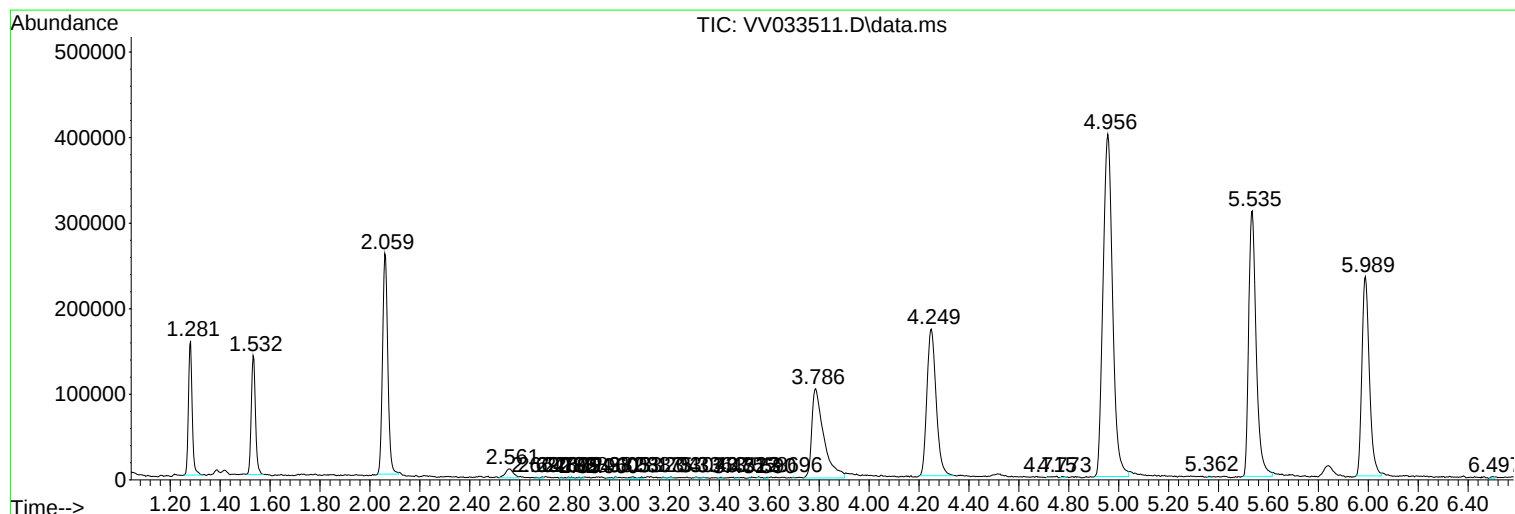

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033511.D
Acq On : 20 Dec 2023 14:56
Operator : SY/MD
Sample : 05927-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033511.D
Acq On : 20 Dec 2023 14:56
Operator : SY/MD
Sample : 05927-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------