

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033512.D
 Acq On : 20 Dec 2023 15:19
 Operator : SY/MD
 Sample : 05927-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	150302	160556	14.77%	1.969%
2	1.532	147	153	167	rVB	137840	162670	14.96%	1.995%
3	2.060	309	317	332	rVB	255863	370323	34.06%	4.541%
4	2.372	412	414	417	rBV3	850	322	0.03%	0.004%
5	2.391	417	420	424	rBV5	1306	1003	0.09%	0.012%
6	2.667	504	506	509	rBV4	887	554	0.05%	0.007%
7	2.709	516	519	523	rBV5	1545	1133	0.10%	0.014%
8	2.783	540	542	544	rVB3	1181	371	0.03%	0.005%
9	2.802	544	548	550	rBV5	1055	828	0.08%	0.010%
10	3.015	612	614	616	rBV2	1307	646	0.06%	0.008%
11	3.188	664	668	670	rBV4	780	481	0.04%	0.006%
12	3.343	710	716	719	rBV8	1996	1630	0.15%	0.020%
13	3.391	730	731	736	rBV4	714	663	0.06%	0.008%
14	3.494	761	763	765	rBV3	1491	762	0.07%	0.009%
15	3.597	792	795	800	rBV5	1704	1459	0.13%	0.018%
16	3.793	842	856	894	rBV4	89082	365891	33.66%	4.487%
17	4.249	985	998	1024	rVB	172556	439862	40.46%	5.394%
18	4.593	1102	1105	1108	rBV5	1730	872	0.08%	0.011%
19	4.834	1177	1180	1182	rBV4	1551	752	0.07%	0.009%
20	4.957	1199	1218	1244	rBV2	402917	1087174	100.00%	13.333%
21	5.535	1387	1398	1421	rBV	314798	651957	59.97%	7.995%
22	5.989	1526	1539	1562	rBV	240371	502185	46.19%	6.159%
23	6.584	1723	1724	1727	rVB2	906	445	0.04%	0.005%
24	6.603	1727	1730	1732	rBV4	833	627	0.06%	0.008%
25	6.728	1767	1769	1770	rBV2	846	294	0.03%	0.004%
26	6.773	1781	1783	1784	rBV2	1238	492	0.05%	0.006%
27	6.844	1803	1805	1807	rBV4	916	413	0.04%	0.005%
28	6.915	1817	1827	1845	rBV2	112437	213508	19.64%	2.618%
29	7.243	1919	1929	1952	rBV	447311	788550	72.53%	9.670%
30	7.555	2017	2026	2044	rBV2	83095	155676	14.32%	1.909%
31	7.805	2102	2104	2109	rVB5	2344	1275	0.12%	0.016%
32	8.024	2163	2172	2203	rBV	175640	384244	35.34%	4.712%
33	8.477	2307	2313	2316	rBV7	1799	2184	0.20%	0.027%
34	8.783	2398	2408	2430	rBV	506734	854834	78.63%	10.483%
35	9.214	2540	2542	2550	rVB7	1218	1083	0.10%	0.013%
36	9.297	2565	2568	2571	rVB3	1362	750	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033512.D
 Acq On : 20 Dec 2023 15:19
 Operator : SY/MD
 Sample : 05927-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	9.313	2571	2573	2574	rBV2	1307	620	0.06%	0.008%
38	9.461	2617	2619	2620	rBV2	1487	730	0.07%	0.009%
39	9.516	2634	2636	2637	rBV2	914	306	0.03%	0.004%
40	9.538	2641	2643	2645	rVB3	888	335	0.03%	0.004%
41	9.551	2645	2647	2650	rBV5	1328	960	0.09%	0.012%
42	9.706	2689	2695	2701	rBV8	1619	1930	0.18%	0.024%
43	9.799	2722	2724	2725	rBV2	1190	563	0.05%	0.007%
44	9.866	2743	2745	2747	rBV3	751	317	0.03%	0.004%
45	9.892	2750	2753	2755	rBV4	1614	1009	0.09%	0.012%
46	10.011	2788	2790	2794	rBV5	996	680	0.06%	0.008%
47	10.072	2806	2809	2810	rBV3	999	640	0.06%	0.008%
48	10.153	2824	2834	2858	rVB	301888	473117	43.52%	5.802%
49	10.384	2903	2906	2908	rBV4	1286	827	0.08%	0.010%
50	10.435	2918	2922	2928	rBV7	1049	1332	0.12%	0.016%
51	10.464	2928	2931	2935	rVV6	1786	1127	0.10%	0.014%
52	10.481	2935	2936	2940	rVB4	844	516	0.05%	0.006%
53	10.526	2946	2950	2953	rBV3	1201	916	0.08%	0.011%
54	10.574	2963	2965	2967	rBV3	1093	483	0.04%	0.006%
55	10.677	2994	2997	2998	rBV2	897	387	0.04%	0.005%
56	10.709	3003	3007	3010	rBV6	1523	1123	0.10%	0.014%
57	10.735	3014	3015	3019	rVB3	620	272	0.03%	0.003%
58	10.754	3019	3021	3023	rBV	924	522	0.05%	0.006%
59	10.767	3023	3025	3029	rVB6	1772	912	0.08%	0.011%
60	10.808	3037	3038	3042	rVB3	843	345	0.03%	0.004%
61	10.889	3059	3063	3064	rBV4	943	623	0.06%	0.008%
62	10.937	3076	3078	3079	rBV2	674	267	0.02%	0.003%
63	10.963	3083	3086	3088	rVB4	627	290	0.03%	0.004%
64	11.091	3122	3126	3128	rVV4	1213	887	0.08%	0.011%
65	11.185	3144	3155	3175	rBV	468079	744308	68.46%	9.128%
66	11.426	3226	3230	3231	rBV4	866	545	0.05%	0.007%
67	11.561	3261	3272	3293	rBV	456093	733296	67.45%	8.993%
68	11.731	3323	3325	3326	rBV2	1114	566	0.05%	0.007%
69	11.850	3360	3362	3367	rBV5	1169	773	0.07%	0.009%
70	11.905	3377	3379	3380	rBV2	636	289	0.03%	0.004%
71	12.114	3442	3444	3446	rBV3	817	433	0.04%	0.005%
72	12.197	3468	3470	3471	rBV2	1198	623	0.06%	0.008%
73	12.490	3559	3561	3564	rBV2	853	568	0.05%	0.007%
74	12.506	3564	3566	3569	rVV3	979	610	0.06%	0.007%
75	12.689	3618	3623	3624	rBV4	891	825	0.08%	0.010%
76	12.712	3629	3630	3633	rBV3	721	392	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033512.D
 Acq On : 20 Dec 2023 15:19
 Operator : SY/MD
 Sample : 05927-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.857	3672	3675	3676	rBV2	861	429	0.04%	0.005%
78	12.889	3683	3685	3686	rBV2	758	308	0.03%	0.004%
79	12.911	3691	3692	3700	rVV7	947	882	0.08%	0.011%
80	12.988	3714	3716	3722	rBV5	1820	1600	0.15%	0.020%
81	13.066	3736	3740	3744	rBV4	1211	1254	0.12%	0.015%
82	13.085	3744	3746	3749	rVV4	1380	806	0.07%	0.010%
83	13.111	3752	3754	3756	rVV3	889	444	0.04%	0.005%
84	13.127	3756	3759	3763	rVB5	1307	1099	0.10%	0.013%
85	13.259	3798	3800	3803	rBV4	818	413	0.04%	0.005%
86	13.297	3808	3812	3814	rBV5	982	589	0.05%	0.007%
87	13.361	3827	3832	3835	rBV7	1519	1473	0.14%	0.018%
88	13.416	3847	3849	3850	rBV2	1498	593	0.05%	0.007%
89	13.689	3927	3934	3937	rBV8	2106	2219	0.20%	0.027%
90	13.754	3950	3954	3956	rBV5	1183	909	0.08%	0.011%
91	13.911	4001	4003	4004	rBV	970	470	0.04%	0.006%
92	13.934	4008	4010	4011	rBV	772	411	0.04%	0.005%
93	14.030	4036	4040	4045	rVB5	1806	1668	0.15%	0.020%
94	14.062	4045	4050	4053	rBV5	1203	1459	0.13%	0.018%
95	14.098	4058	4061	4066	rVV5	1479	1171	0.11%	0.014%
96	14.294	4120	4122	4125	rBV3	977	438	0.04%	0.005%
97	14.432	4160	4165	4167	rBV6	2069	1328	0.12%	0.016%
98	14.451	4168	4171	4175	rVB4	1513	1209	0.11%	0.015%
99	14.988	4335	4338	4341	rVB5	1334	762	0.07%	0.009%
100	15.156	4387	4390	4391	rBV	1113	551	0.05%	0.007%




Sum of corrected areas: 8154218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033512.D
Acq On : 20 Dec 2023 15:19
Operator : SY/MD
Sample : 05927-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

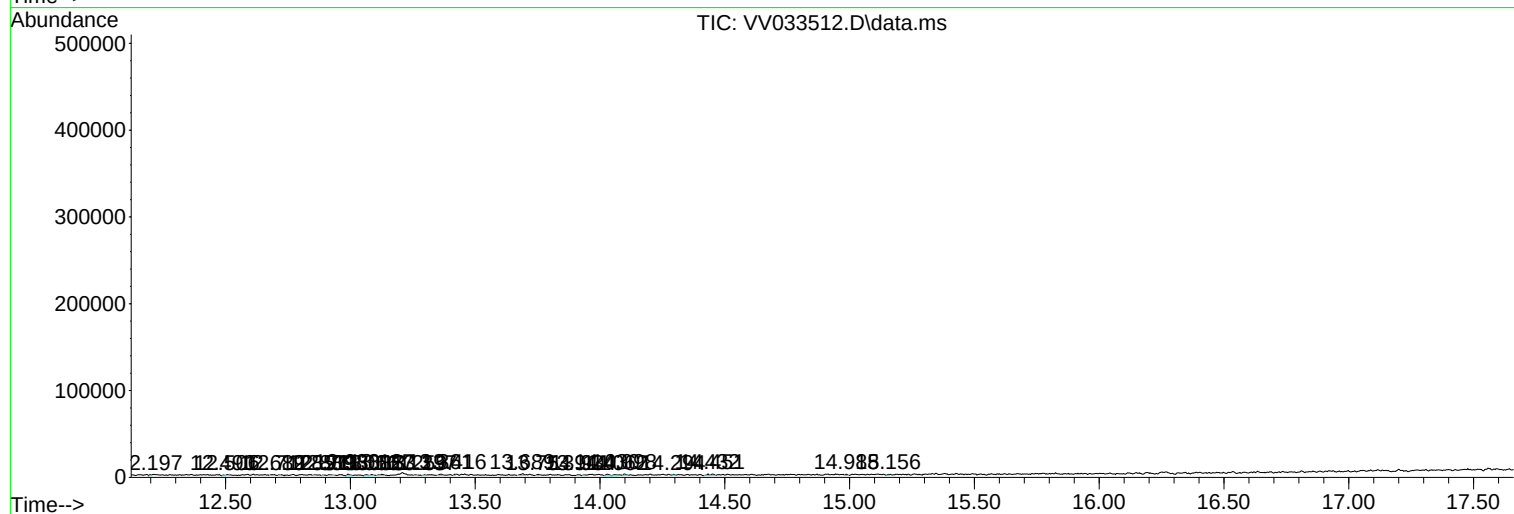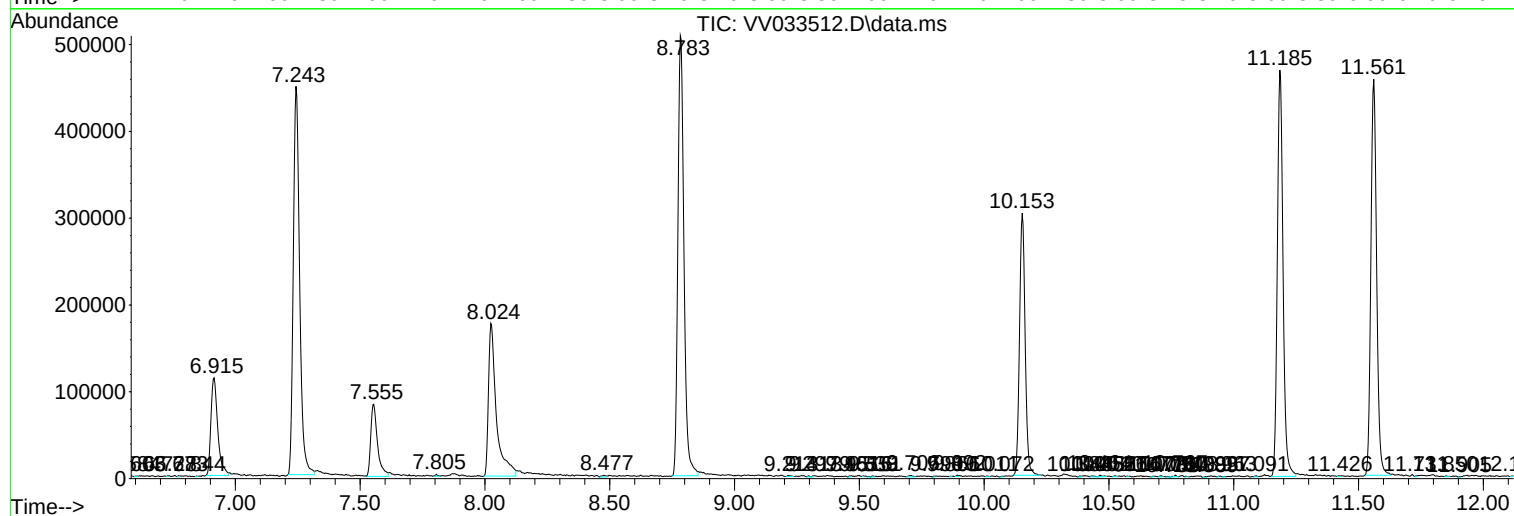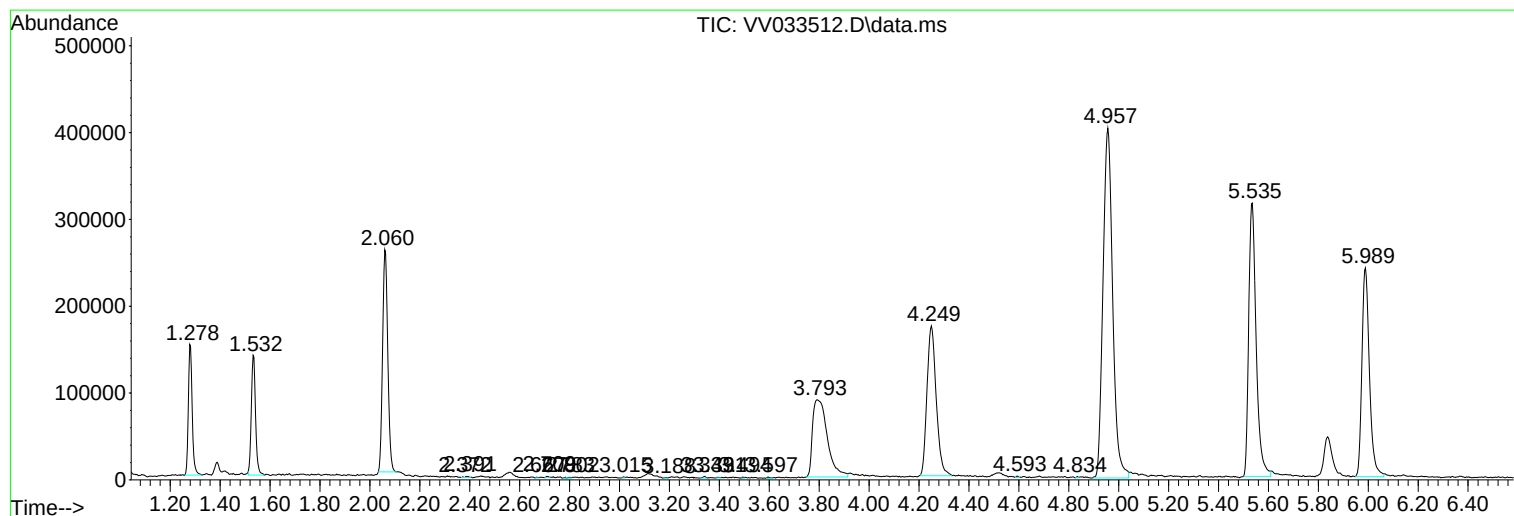

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033512.D
Acq On : 20 Dec 2023 15:19
Operator : SY/MD
Sample : 05927-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033512.D
Acq On : 20 Dec 2023 15:19
Operator : SY/MD
Sample : 05927-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------