

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033513.D
 Acq On : 20 Dec 2023 15:42
 Operator : SY/MD
 Sample : 05927-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rBV	156637	162395	14.83%	1.967%
2	1.532	147	153	170	rVB	139584	165430	15.11%	2.003%
3	2.060	309	317	342	rVB	265798	401038	36.62%	4.857%
4	2.529	458	463	464	rBV3	1123	1043	0.10%	0.013%
5	2.790	539	544	545	rBV4	1216	1102	0.10%	0.013%
6	2.822	552	554	557	rBV4	911	683	0.06%	0.008%
7	2.928	585	587	590	rBV4	1383	752	0.07%	0.009%
8	3.021	611	616	617	rBV5	1467	1016	0.09%	0.012%
9	3.114	637	645	646	rBV7	5558	5967	0.54%	0.072%
10	3.394	729	732	734	rBV4	813	570	0.05%	0.007%
11	3.513	767	769	772	rBV3	1096	739	0.07%	0.009%
12	3.542	775	778	781	rBV3	1451	712	0.07%	0.009%
13	3.571	781	787	789	rVV4	1045	967	0.09%	0.012%
14	3.699	823	827	829	rBV6	1170	810	0.07%	0.010%
15	3.722	832	834	837	rVB3	1289	547	0.05%	0.007%
16	3.789	844	855	858	rBV	67058	118077	10.78%	1.430%
17	4.249	982	998	1023	rBV2	174815	454897	41.54%	5.509%
18	4.465	1063	1065	1067	rVB2	1447	594	0.05%	0.007%
19	4.593	1103	1105	1106	rBV2	1090	557	0.05%	0.007%
20	4.728	1145	1147	1149	rBV3	1090	550	0.05%	0.007%
21	4.838	1177	1181	1187	rVB8	1109	1159	0.11%	0.014%
22	4.879	1189	1194	1195	rBV5	974	748	0.07%	0.009%
23	4.957	1201	1218	1247	rBV2	411064	1094992	100.00%	13.261%
24	5.249	1307	1309	1313	rBV5	1269	785	0.07%	0.010%
25	5.535	1386	1398	1419	rBV	313802	653065	59.64%	7.909%
26	5.838	1481	1492	1511	rBV3	80623	173159	15.81%	2.097%
27	5.989	1527	1539	1557	rBV	241662	493681	45.09%	5.979%
28	6.567	1717	1719	1721	rBV3	961	545	0.05%	0.007%
29	6.664	1747	1749	1752	rVB3	1391	564	0.05%	0.007%
30	6.703	1756	1761	1764	rBV7	1221	1337	0.12%	0.016%
31	6.915	1817	1827	1851	rBV	114031	218922	19.99%	2.651%
32	7.243	1918	1929	1948	rBV	449157	798621	72.93%	9.672%
33	7.555	2017	2026	2047	rBV	81128	153447	14.01%	1.858%
34	8.024	2154	2172	2204	rBV	196348	427292	39.02%	5.175%
35	8.375	2279	2281	2284	rVB3	1573	739	0.07%	0.009%
36	8.506	2320	2322	2324	rBV3	1470	629	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033513.D
 Acq On : 20 Dec 2023 15:42
 Operator : SY/MD
 Sample : 05927-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.783	2397	2408	2429	rBV	509932	860853	78.62%	10.425%
38	9.191	2529	2535	2536	rBV5	1363	1369	0.13%	0.017%
39	9.288	2563	2565	2568	rBV5	986	627	0.06%	0.008%
40	9.616	2664	2667	2670	rBV4	956	739	0.07%	0.009%
41	9.664	2680	2682	2687	rVB5	869	726	0.07%	0.009%
42	9.690	2687	2690	2693	rBV3	1014	845	0.08%	0.010%
43	9.747	2705	2708	2712	rBV6	897	822	0.08%	0.010%
44	9.911	2756	2759	2761	rBV4	1295	576	0.05%	0.007%
45	10.030	2794	2796	2800	rBV5	1016	617	0.06%	0.007%
46	10.098	2815	2817	2820	rBV3	916	607	0.06%	0.007%
47	10.153	2821	2834	2855	rVV	314595	502048	45.85%	6.080%
48	10.391	2905	2908	2916	rVB7	1297	1443	0.13%	0.017%
49	10.423	2916	2918	2923	rBV6	1020	1064	0.10%	0.013%
50	10.468	2930	2932	2936	rBV5	874	589	0.05%	0.007%
51	10.593	2969	2971	2973	rBV4	1377	546	0.05%	0.007%
52	10.690	3000	3001	3006	rBV5	1076	820	0.07%	0.010%
53	10.786	3026	3031	3035	rBV7	1831	1892	0.17%	0.023%
54	10.805	3035	3037	3040	rBV4	911	621	0.06%	0.008%
55	10.847	3047	3050	3052	rBV4	1359	749	0.07%	0.009%
56	10.924	3071	3074	3077	rBV4	1145	765	0.07%	0.009%
57	10.940	3077	3079	3081	rBV3	1077	549	0.05%	0.007%
58	11.079	3117	3122	3124	rBV6	938	694	0.06%	0.008%
59	11.130	3132	3138	3142	rBV6	1917	1832	0.17%	0.022%
60	11.185	3143	3155	3176	rBV	480265	749925	68.49%	9.082%
61	11.561	3255	3272	3296	rBV	469127	755222	68.97%	9.146%
62	11.734	3323	3326	3329	rBV4	1769	967	0.09%	0.012%
63	11.960	3394	3396	3400	rBV5	1090	754	0.07%	0.009%
64	11.979	3400	3402	3407	rVV4	1231	740	0.07%	0.009%
65	12.207	3470	3473	3476	rBV4	1245	668	0.06%	0.008%
66	12.352	3516	3518	3521	rBV3	1284	739	0.07%	0.009%
67	12.368	3521	3523	3528	rVV6	1105	852	0.08%	0.010%
68	12.419	3537	3539	3541	rVV3	969	622	0.06%	0.008%
69	12.622	3599	3602	3605	rBV3	817	628	0.06%	0.008%
70	12.661	3610	3614	3616	rBV3	1093	847	0.08%	0.010%
71	12.738	3635	3638	3642	rBV6	910	891	0.08%	0.011%
72	12.818	3658	3663	3666	rBV6	1456	1181	0.11%	0.014%
73	13.053	3732	3736	3741	rBV6	1159	984	0.09%	0.012%
74	13.082	3741	3745	3748	rBV4	950	759	0.07%	0.009%
75	13.339	3823	3825	3830	rBV5	1001	1016	0.09%	0.012%
76	13.432	3851	3854	3857	rVB5	1602	985	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033513.D
 Acq On : 20 Dec 2023 15:42
 Operator : SY/MD
 Sample : 05927-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.455	3857	3861	3862	rBV4	1053	590	0.05%	0.007%
78	13.580	3897	3900	3902	rBV3	1107	754	0.07%	0.009%
79	13.638	3916	3918	3922	rBV4	1001	575	0.05%	0.007%
80	13.763	3952	3957	3961	rBV6	1222	1005	0.09%	0.012%
81	13.812	3968	3972	3973	rBV4	1655	1015	0.09%	0.012%
82	13.889	3990	3996	3997	rBV6	1250	1076	0.10%	0.013%
83	13.931	4006	4009	4011	rBV3	1733	1122	0.10%	0.014%
84	13.972	4017	4022	4026	rBV6	1441	1443	0.13%	0.017%
85	14.030	4037	4040	4041	rBV2	986	584	0.05%	0.007%
86	14.088	4055	4058	4061	rBV4	1012	559	0.05%	0.007%
87	14.117	4064	4067	4071	rBV5	880	874	0.08%	0.011%
88	14.178	4083	4086	4087	rBV3	957	601	0.05%	0.007%
89	14.204	4092	4094	4097	rBV4	1007	623	0.06%	0.008%
90	14.281	4113	4118	4122	rVV7	1621	1794	0.16%	0.022%
91	14.545	4198	4200	4204	rBV4	1494	886	0.08%	0.011%
92	14.564	4204	4206	4210	rVB3	1502	889	0.08%	0.011%
93	14.705	4247	4250	4252	rBV3	978	689	0.06%	0.008%
94	14.873	4300	4302	4305	rBV3	931	621	0.06%	0.008%
95	14.940	4320	4323	4325	rBV2	962	629	0.06%	0.008%
96	14.976	4333	4334	4337	rBV2	926	557	0.05%	0.007%
97	15.168	4391	4394	4396	rVB3	1240	648	0.06%	0.008%
98	15.284	4427	4430	4432	rBV3	1219	633	0.06%	0.008%
99	15.673	4549	4551	4554	rBV3	1221	1011	0.09%	0.012%
100	15.818	4594	4596	4600	rBV5	1344	746	0.07%	0.009%


Sum of corrected areas: 8257228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033513.D
Acq On : 20 Dec 2023 15:42
Operator : SY/MD
Sample : 05927-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

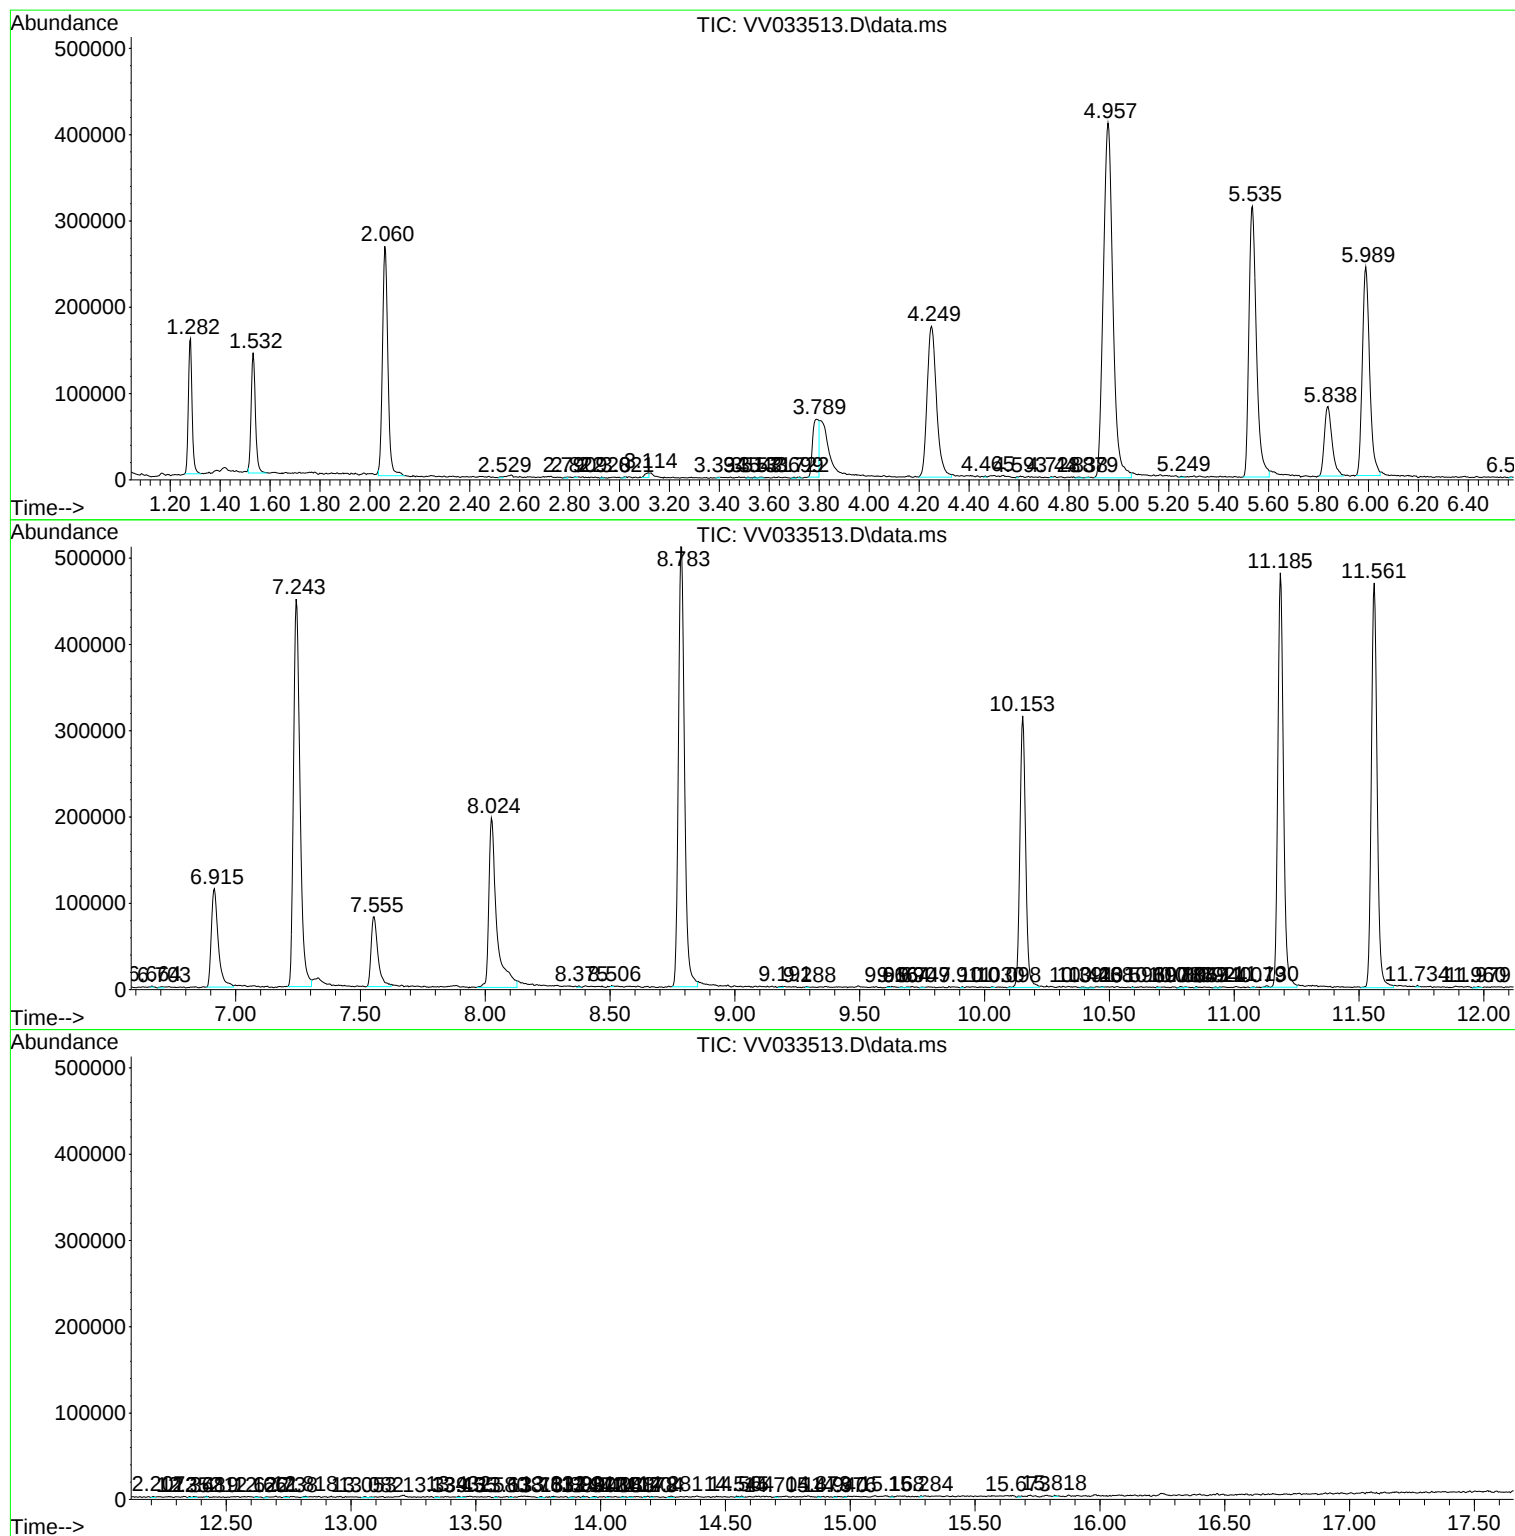

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033513.D
Acq On : 20 Dec 2023 15:42
Operator : SY/MD
Sample : 05927-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033513.D
Acq On : 20 Dec 2023 15:42
Operator : SY/MD
Sample : 05927-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------