

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033514.D
 Acq On : 20 Dec 2023 16:05
 Operator : SY/MD
 Sample : 05927-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rBV	148564	157183	14.75%	1.989%
2	1.532	147	153	165	rVB	132317	154291	14.47%	1.952%
3	2.059	309	317	330	rBV	250703	364395	34.18%	4.610%
4	2.410	423	426	429	rBV6	1506	1189	0.11%	0.015%
5	2.497	448	453	454	rBV5	1068	872	0.08%	0.011%
6	2.641	494	498	500	rBV4	1226	701	0.07%	0.009%
7	2.931	586	588	590	rBV3	1007	499	0.05%	0.006%
8	2.960	595	597	603	rVB6	1038	769	0.07%	0.010%
9	3.005	608	611	613	rBV5	871	621	0.06%	0.008%
10	3.204	671	673	675	rBV3	814	442	0.04%	0.006%
11	3.220	676	678	681	rVV3	990	479	0.04%	0.006%
12	3.252	687	688	693	rBV4	735	514	0.05%	0.007%
13	3.288	698	699	702	rBV3	1034	466	0.04%	0.006%
14	3.326	707	711	712	rBV3	1314	896	0.08%	0.011%
15	3.346	715	717	720	rVV4	1479	797	0.07%	0.010%
16	3.436	743	745	747	rVB3	1279	536	0.05%	0.007%
17	3.455	747	751	752	rBV2	1107	814	0.08%	0.010%
18	3.490	760	762	764	rBV2	963	457	0.04%	0.006%
19	3.600	794	796	800	rVB4	977	647	0.06%	0.008%
20	3.683	821	822	826	rVB3	1591	614	0.06%	0.008%
21	3.706	826	829	831	rBV3	1026	595	0.06%	0.008%
22	3.757	842	845	846	rBV3	951	505	0.05%	0.006%
23	3.783	846	853	882	rVV2	53837	157044	14.73%	1.987%
24	4.249	984	998	1023	rBV	170111	439477	41.23%	5.560%
25	4.693	1134	1136	1142	rVB5	1855	1439	0.13%	0.018%
26	4.956	1202	1218	1243	rBV2	397913	1065974	100.00%	13.486%
27	5.535	1387	1398	1422	rBV	304537	634686	59.54%	8.029%
28	5.841	1483	1493	1509	rBV	10419	25154	2.36%	0.318%
29	5.989	1526	1539	1566	rBV	235921	501367	47.03%	6.343%
30	6.333	1644	1646	1649	rVB4	1634	739	0.07%	0.009%
31	6.416	1670	1672	1674	rBV3	786	447	0.04%	0.006%
32	6.522	1703	1705	1706	rBV2	1175	446	0.04%	0.006%
33	6.622	1732	1736	1738	rBV5	621	491	0.05%	0.006%
34	6.677	1751	1753	1757	rBV3	1369	925	0.09%	0.012%
35	6.757	1773	1778	1782	rVB7	1578	1336	0.13%	0.017%
36	6.863	1806	1811	1814	rBV7	1376	1425	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033514.D
 Acq On : 20 Dec 2023 16:05
 Operator : SY/MD
 Sample : 05927-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.915	1817	1827	1850	rVV	110990	214186	20.09%	2.710%
38	7.243	1918	1929	1952	rBV	440484	791666	74.27%	10.015%
39	7.513	2011	2013	2015	rBV3	1010	509	0.05%	0.006%
40	7.554	2017	2026	2052	rVV	79958	150137	14.08%	1.899%
41	8.024	2164	2172	2205	rBV	180532	384842	36.10%	4.869%
42	8.783	2397	2408	2430	rBV	510282	846801	79.44%	10.713%
43	9.178	2528	2531	2536	rBV7	1393	1347	0.13%	0.017%
44	9.204	2536	2539	2542	rBV5	1278	982	0.09%	0.012%
45	9.326	2574	2577	2579	rBV3	1009	613	0.06%	0.008%
46	9.422	2604	2607	2610	rBV5	1283	1004	0.09%	0.013%
47	9.500	2627	2631	2633	rBV5	815	532	0.05%	0.007%
48	9.622	2667	2669	2672	rBV3	1260	816	0.08%	0.010%
49	9.728	2698	2702	2705	rVB5	1464	1194	0.11%	0.015%
50	9.789	2717	2721	2723	rVB4	1386	1041	0.10%	0.013%
51	9.847	2735	2739	2743	rBV6	1295	1339	0.13%	0.017%
52	9.905	2755	2757	2762	rVB4	1686	1130	0.11%	0.014%
53	9.937	2762	2767	2768	rBV4	1340	1005	0.09%	0.013%
54	10.011	2789	2790	2796	rVB4	1556	1002	0.09%	0.013%
55	10.037	2796	2798	2801	rBV4	1063	580	0.05%	0.007%
56	10.056	2801	2804	2806	rBV4	1152	705	0.07%	0.009%
57	10.082	2809	2812	2814	rBV3	730	572	0.05%	0.007%
58	10.152	2824	2834	2854	rVB	308642	482355	45.25%	6.102%
59	10.368	2899	2901	2903	rBV3	1004	495	0.05%	0.006%
60	10.718	3006	3010	3013	rBV5	1550	1136	0.11%	0.014%
61	10.770	3021	3026	3028	rBV5	733	748	0.07%	0.009%
62	10.873	3056	3058	3063	rVB4	1604	1163	0.11%	0.015%
63	10.902	3063	3067	3069	rBV5	1289	1004	0.09%	0.013%
64	11.004	3097	3099	3102	rBV4	1083	668	0.06%	0.008%
65	11.107	3126	3131	3133	rBV5	1360	1199	0.11%	0.015%
66	11.184	3145	3155	3178	rBV	468314	735557	69.00%	9.306%
67	11.442	3232	3235	3237	rBV4	1088	628	0.06%	0.008%
68	11.561	3260	3272	3292	rBV	456705	734006	68.86%	9.286%
69	11.731	3323	3325	3328	rBV3	1251	552	0.05%	0.007%
70	11.799	3343	3346	3349	rBV5	1560	1525	0.14%	0.019%
71	11.924	3382	3385	3387	rBV3	1400	872	0.08%	0.011%
72	12.017	3410	3414	3416	rBV4	1107	605	0.06%	0.008%
73	12.082	3432	3434	3438	rBV5	1070	786	0.07%	0.010%
74	12.255	3486	3488	3491	rVV3	1357	738	0.07%	0.009%
75	12.274	3491	3494	3497	rVV6	875	630	0.06%	0.008%
76	12.355	3516	3519	3522	rBV3	761	451	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033514.D
 Acq On : 20 Dec 2023 16:05
 Operator : SY/MD
 Sample : 05927-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.368	3522	3523	3528	rVB4	966	514	0.05%	0.007%
78	12.400	3528	3533	3536	rBV7	1615	1688	0.16%	0.021%
79	12.612	3597	3599	3602	rBV4	854	516	0.05%	0.007%
80	12.647	3607	3610	3614	rVB5	1278	759	0.07%	0.010%
81	12.709	3625	3629	3630	rBV4	984	570	0.05%	0.007%
82	12.850	3669	3673	3674	rBV4	742	535	0.05%	0.007%
83	13.178	3772	3775	3777	rBV3	916	725	0.07%	0.009%
84	13.204	3781	3783	3787	rVV4	1276	861	0.08%	0.011%
85	13.271	3801	3804	3808	rVB5	1419	924	0.09%	0.012%
86	13.426	3850	3852	3855	rBV3	829	441	0.04%	0.006%
87	13.451	3858	3860	3863	rBV4	1230	784	0.07%	0.010%
88	13.577	3895	3899	3901	rBV6	1443	1112	0.10%	0.014%
89	13.602	3905	3907	3909	rVB3	1236	464	0.04%	0.006%
90	13.763	3955	3957	3959	rVV3	939	509	0.05%	0.006%
91	13.827	3974	3977	3980	rVV4	1026	576	0.05%	0.007%
92	13.985	4022	4026	4027	rBV4	1487	937	0.09%	0.012%
93	14.107	4061	4064	4065	rBV4	767	452	0.04%	0.006%
94	14.274	4113	4116	4120	rBV6	1306	1219	0.11%	0.015%
95	14.307	4124	4126	4129	rVB4	1686	917	0.09%	0.012%
96	14.326	4129	4132	4134	rBV3	779	603	0.06%	0.008%
97	14.461	4172	4174	4177	rBV3	1260	971	0.09%	0.012%
98	14.602	4214	4218	4220	rBV4	1546	1031	0.10%	0.013%
99	15.329	4442	4444	4446	rBV3	873	469	0.04%	0.006%
100	15.361	4452	4454	4457	rBV4	891	502	0.05%	0.006%




Sum of corrected areas: 7904432

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033514.D
Acq On : 20 Dec 2023 16:05
Operator : SY/MD
Sample : 05927-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

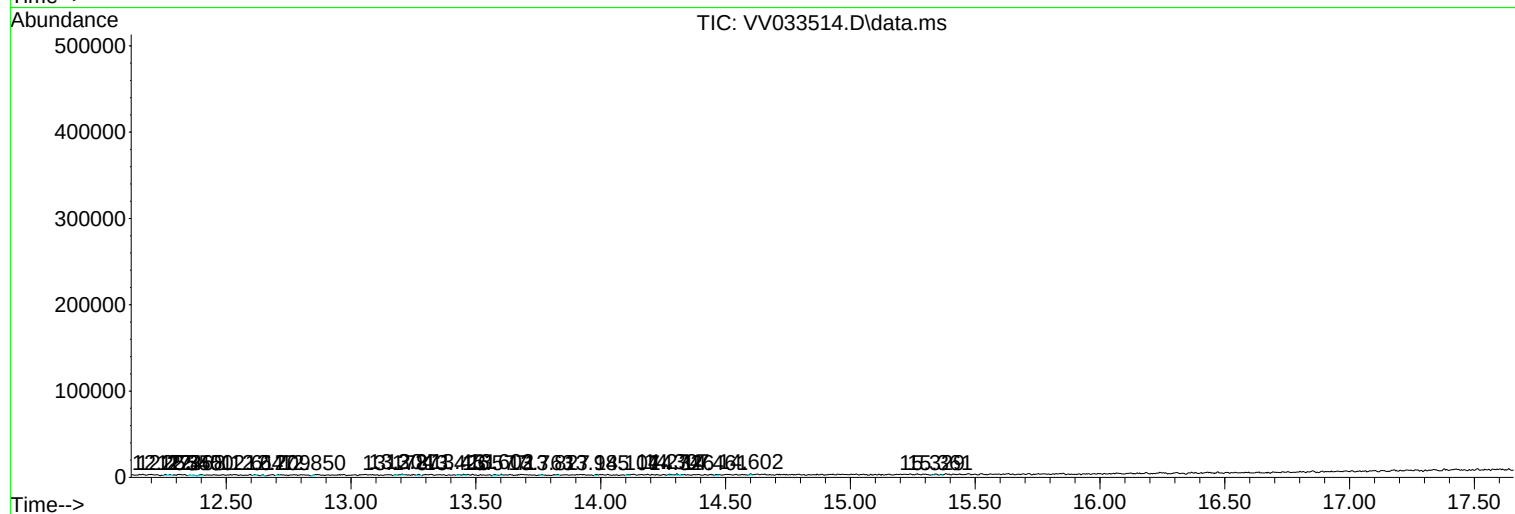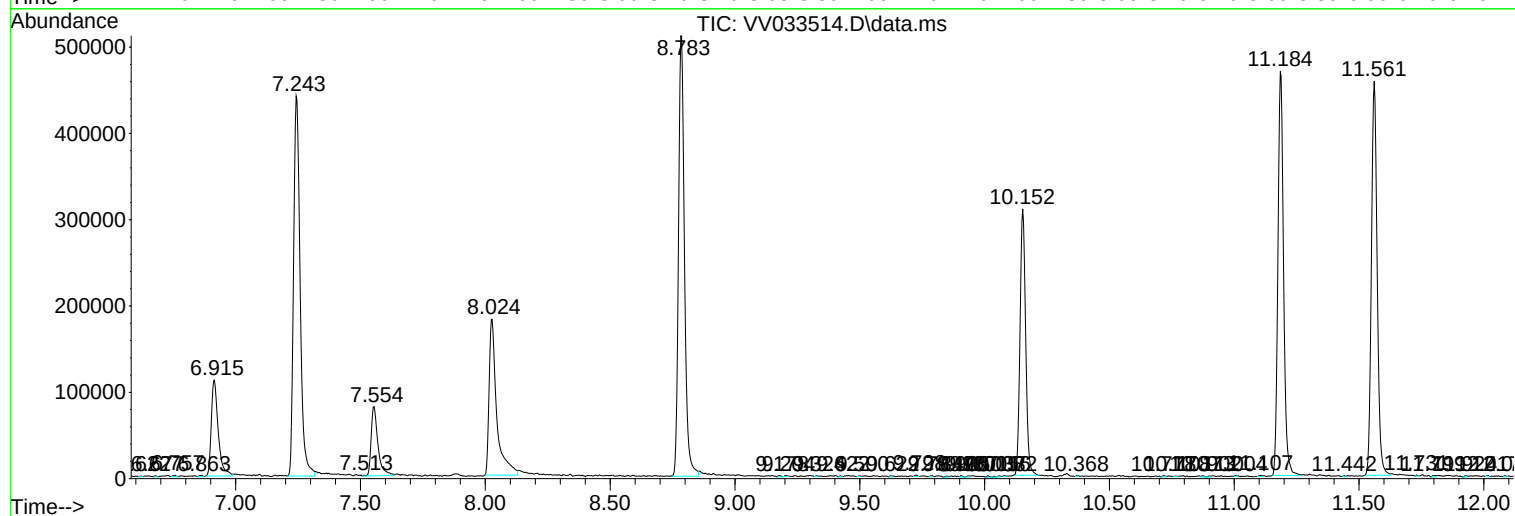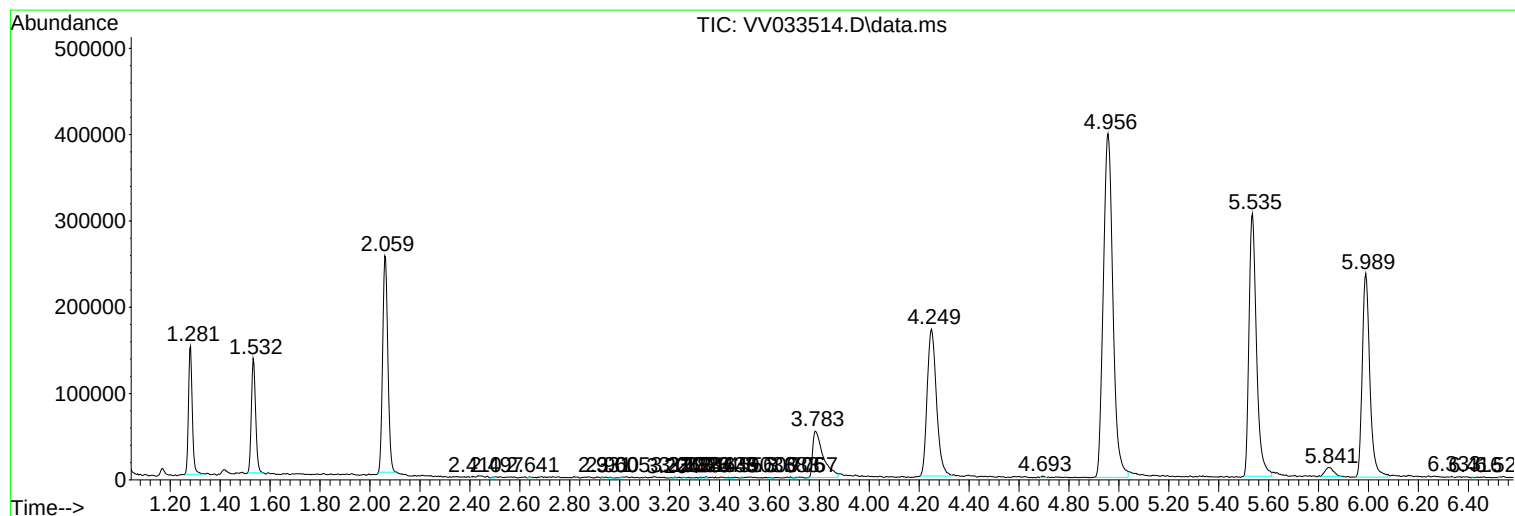

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033514.D
Acq On : 20 Dec 2023 16:05
Operator : SY/MD
Sample : 05927-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033514.D
Acq On : 20 Dec 2023 16:05
Operator : SY/MD
Sample : 05927-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------