

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033515.D
 Acq On : 20 Dec 2023 16:28
 Operator : SY/MD
 Sample : 05927-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	148169	157264	14.23%	1.904%
2	1.532	147	153	171	rVB	140565	167321	15.14%	2.026%
3	2.060	308	317	341	rVB	266054	404615	36.61%	4.900%
4	2.841	556	560	565	rBV7	1653	1567	0.14%	0.019%
5	2.912	580	582	583	rBV2	1252	475	0.04%	0.006%
6	2.999	606	609	613	rBV6	1354	1124	0.10%	0.014%
7	3.050	623	625	627	rVB3	799	315	0.03%	0.004%
8	3.072	627	632	634	rBV4	1193	977	0.09%	0.012%
9	3.092	634	638	640	rBV4	1594	1333	0.12%	0.016%
10	3.108	640	643	644	rBV3	2160	1198	0.11%	0.015%
11	3.188	665	668	673	rVB5	1651	933	0.08%	0.011%
12	3.211	673	675	677	rVB3	822	279	0.03%	0.003%
13	3.220	677	678	681	rBV3	840	513	0.05%	0.006%
14	3.272	692	694	695	rBV2	1135	478	0.04%	0.006%
15	3.362	720	722	724	rVB3	1512	599	0.05%	0.007%
16	3.375	724	726	728	rBV3	722	392	0.04%	0.005%
17	3.523	769	772	775	rBV3	1038	613	0.06%	0.007%
18	3.606	795	798	804	rBV6	1157	1210	0.11%	0.015%
19	3.709	829	830	831	rBV	996	354	0.03%	0.004%
20	3.786	845	854	855	rBV	57742	66162	5.99%	0.801%
21	4.249	985	998	1027	rVB	175571	448895	40.62%	5.436%
22	4.838	1179	1181	1184	rBV2	1009	552	0.05%	0.007%
23	4.957	1201	1218	1240	rBV2	410866	1105067	100.00%	13.382%
24	5.535	1387	1398	1432	rBV	304505	637729	57.71%	7.723%
25	5.834	1481	1491	1516	rVB	151460	309978	28.05%	3.754%
26	5.989	1528	1539	1558	rBV	244843	497731	45.04%	6.027%
27	6.571	1718	1720	1723	rVB4	1318	538	0.05%	0.007%
28	6.863	1805	1811	1815	rBV8	1233	1352	0.12%	0.016%
29	6.915	1816	1827	1845	rBV	116230	223849	20.26%	2.711%
30	7.166	1902	1905	1908	rBV5	1408	1067	0.10%	0.013%
31	7.182	1908	1910	1915	rVB5	1571	1001	0.09%	0.012%
32	7.243	1918	1929	1948	rBV	459764	814901	73.74%	9.868%
33	7.477	1999	2002	2003	rBV3	1647	1009	0.09%	0.012%
34	7.522	2013	2016	2017	rBV3	1733	1089	0.10%	0.013%
35	7.551	2017	2025	2044	rVV2	82971	152663	13.81%	1.849%
36	7.854	2116	2119	2120	rBV2	2102	1234	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033515.D
 Acq On : 20 Dec 2023 16:28
 Operator : SY/MD
 Sample : 05927-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.973	2153	2156	2157	rBV2	1125	542	0.05%	0.007%
38	8.024	2163	2172	2208	rBV	179409	396635	35.89%	4.803%
39	8.783	2398	2408	2434	rBV	506574	839773	75.99%	10.169%
40	9.452	2613	2616	2620	rBV6	1372	1018	0.09%	0.012%
41	9.545	2643	2645	2647	rBV3	1049	551	0.05%	0.007%
42	9.638	2672	2674	2675	rBV2	860	390	0.04%	0.005%
43	9.767	2712	2714	2717	rBV3	690	486	0.04%	0.006%
44	9.841	2732	2737	2740	rBV6	1413	1170	0.11%	0.014%
45	9.854	2740	2741	2743	rBV2	790	280	0.03%	0.003%
46	9.911	2757	2759	2761	rBV3	928	530	0.05%	0.006%
47	10.018	2789	2792	2794	rBV3	1252	758	0.07%	0.009%
48	10.043	2796	2800	2801	rBV4	986	598	0.05%	0.007%
49	10.153	2823	2834	2847	rBV	316860	492861	44.60%	5.968%
50	10.313	2880	2884	2885	rBV4	1967	1415	0.13%	0.017%
51	10.365	2897	2900	2902	rBV4	1666	1285	0.12%	0.016%
52	10.407	2911	2913	2915	rBV2	874	402	0.04%	0.005%
53	10.423	2916	2918	2919	rBV	843	274	0.02%	0.003%
54	10.571	2960	2964	2970	rBV4	1749	1758	0.16%	0.021%
55	10.654	2988	2990	2993	rVB4	1592	858	0.08%	0.010%
56	10.677	2993	2997	3001	rBV7	1313	1589	0.14%	0.019%
57	10.718	3006	3010	3013	rBV5	962	900	0.08%	0.011%
58	10.767	3021	3025	3028	rBV6	1510	1466	0.13%	0.018%
59	10.892	3062	3064	3067	rBV3	1284	912	0.08%	0.011%
60	10.940	3077	3079	3083	rBV3	1319	743	0.07%	0.009%
61	10.969	3083	3088	3091	rBV6	1110	1122	0.10%	0.014%
62	11.072	3118	3120	3121	rBV2	754	255	0.02%	0.003%
63	11.185	3143	3155	3173	rBV	465199	735480	66.56%	8.906%
64	11.561	3262	3272	3293	rVB	476337	752971	68.14%	9.118%
65	11.879	3369	3371	3374	rBV4	992	597	0.05%	0.007%
66	12.223	3476	3478	3479	rBV2	1378	679	0.06%	0.008%
67	12.313	3503	3506	3508	rBV4	1024	768	0.07%	0.009%
68	12.452	3547	3549	3552	rVB4	1209	636	0.06%	0.008%
69	12.471	3552	3555	3556	rBV4	815	458	0.04%	0.006%
70	12.506	3564	3566	3571	rBV5	1291	1133	0.10%	0.014%
71	12.599	3592	3595	3597	rBV4	1289	795	0.07%	0.010%
72	12.612	3597	3599	3602	rVV3	816	498	0.05%	0.006%
73	12.947	3701	3703	3706	rVB4	1220	451	0.04%	0.005%
74	13.265	3797	3802	3805	rBV7	2088	2219	0.20%	0.027%
75	13.574	3896	3898	3901	rBV4	1261	990	0.09%	0.012%
76	13.796	3965	3967	3968	rBV2	666	200	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033515.D
Acq On : 20 Dec 2023 16:28
Operator : SY/MD
Sample : 05927-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

77	13.866	3987	3989	3990	rBV2	919	392	0.04%	0.005%
78	14.017	4035	4036	4038	rBV2	791	297	0.03%	0.004%
79	14.040	4040	4043	4044	rBV2	1298	719	0.07%	0.009%
80	14.117	4064	4067	4069	rBV4	909	661	0.06%	0.008%
81	14.146	4074	4076	4077	rBV2	790	369	0.03%	0.004%
82	14.156	4077	4079	4081	rBV3	1170	594	0.05%	0.007%
83	15.075	4362	4365	4368	rBV4	1232	948	0.09%	0.011%
84	15.152	4386	4389	4391	rBV3	2153	1161	0.11%	0.014%




Sum of corrected areas: 8257964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033515.D
Acq On : 20 Dec 2023 16:28
Operator : SY/MD
Sample : 05927-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

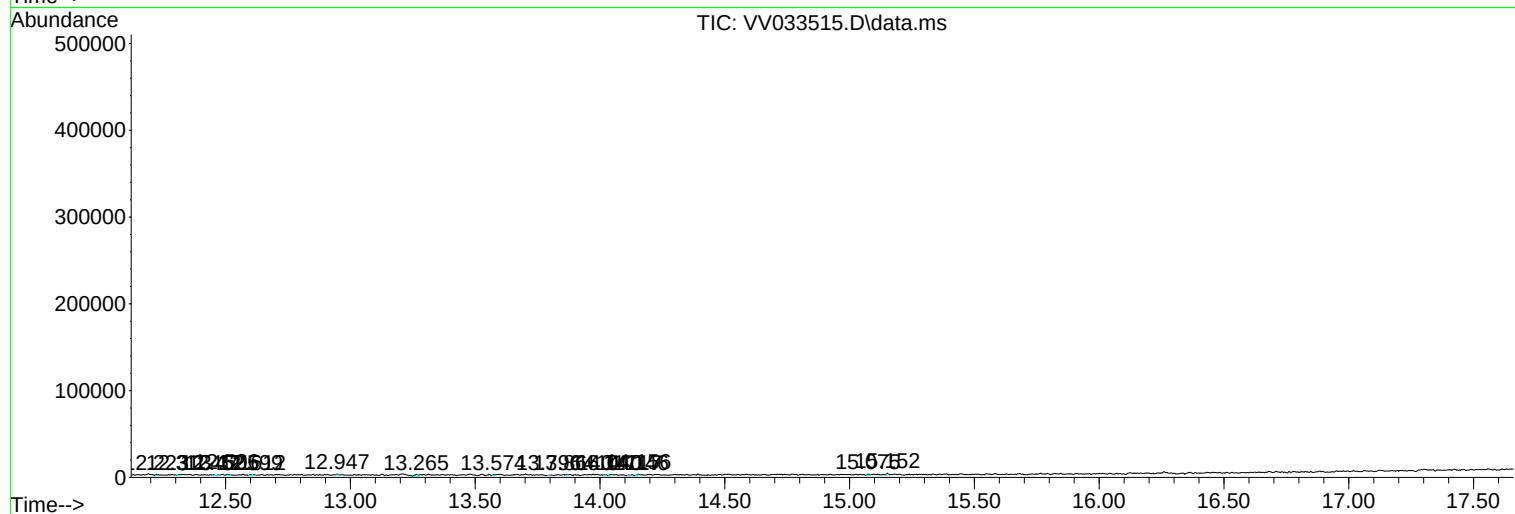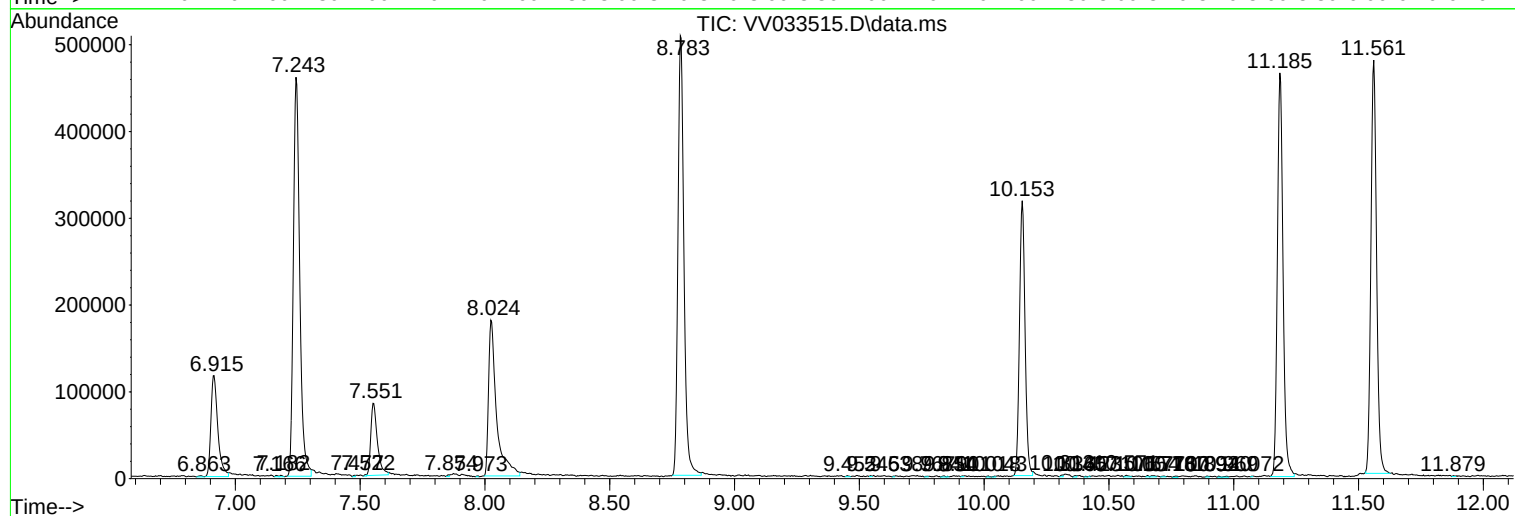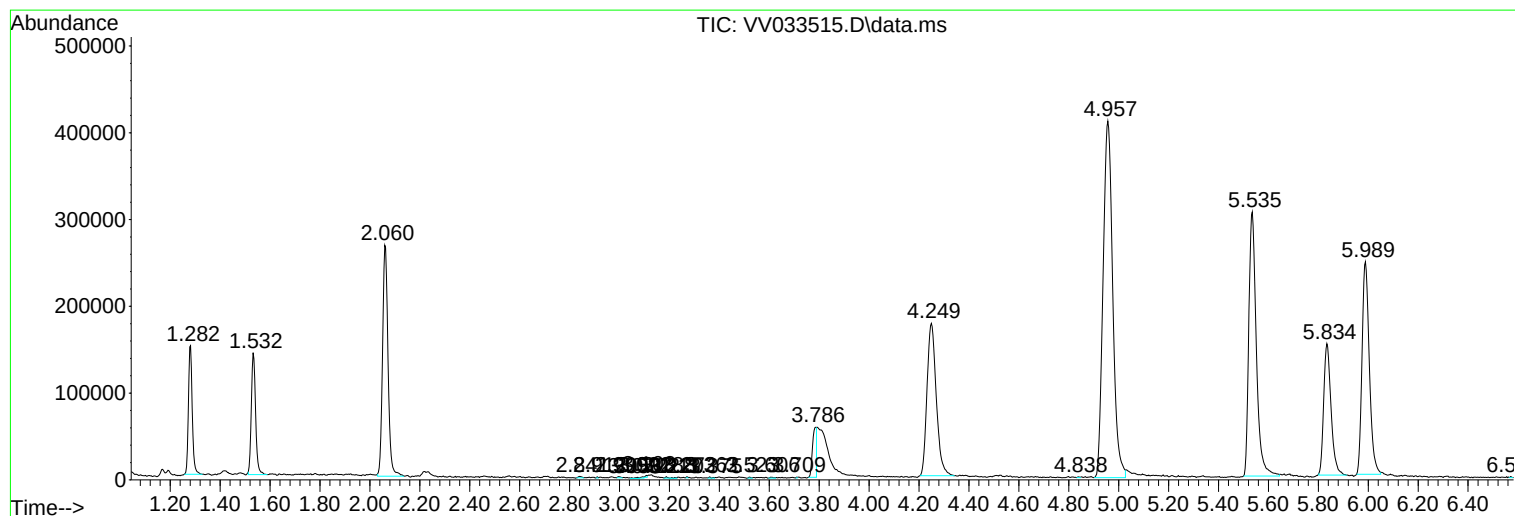

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033515.D
Acq On : 20 Dec 2023 16:28
Operator : SY/MD
Sample : 05927-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033515.D
Acq On : 20 Dec 2023 16:28
Operator : SY/MD
Sample : 05927-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------