

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033516.D
 Acq On : 20 Dec 2023 16:51
 Operator : SY/MD
 Sample : 05927-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	43	rBV	7753	7992	0.76%	0.103%
2	1.191	44	47	54	rVB	18853	17587	1.68%	0.226%
3	1.281	68	75	88	rVB	143307	151499	14.49%	1.943%
4	1.535	147	154	167	rVB	130705	156682	14.98%	2.010%
5	2.060	309	317	331	rVB	248005	360087	34.44%	4.619%
6	2.571	466	476	482	rBV	2024	4293	0.41%	0.055%
7	2.600	482	485	487	rBV3	1021	585	0.06%	0.008%
8	2.651	499	501	505	rBV4	1154	847	0.08%	0.011%
9	2.851	561	563	568	rVB5	1316	700	0.07%	0.009%
10	3.024	614	617	620	rVB5	1232	906	0.09%	0.012%
11	3.043	620	623	624	rBV3	1079	560	0.05%	0.007%
12	3.079	631	634	636	rVB2	1199	574	0.05%	0.007%
13	3.301	700	703	706	rBV4	1023	905	0.09%	0.012%
14	3.400	730	734	735	rBV4	896	527	0.05%	0.007%
15	3.490	759	762	763	rBV2	1086	606	0.06%	0.008%
16	3.571	786	787	790	rBV2	872	480	0.05%	0.006%
17	3.613	797	800	801	rBV3	1375	693	0.07%	0.009%
18	3.661	813	815	817	rBV3	756	505	0.05%	0.006%
19	3.677	818	820	826	rVB8	2157	1572	0.15%	0.020%
20	3.706	826	829	831	rBV4	835	675	0.06%	0.009%
21	3.789	845	855	856	rBV	59927	74011	7.08%	0.949%
22	4.249	984	998	1025	rBV	173628	447853	42.83%	5.745%
23	4.712	1140	1142	1146	rBV5	1161	746	0.07%	0.010%
24	4.821	1174	1176	1178	rBV3	1006	511	0.05%	0.007%
25	4.957	1203	1218	1243	rBV2	390659	1045672	100.00%	13.414%
26	5.535	1386	1398	1426	rBV	294354	615959	58.91%	7.901%
27	5.834	1480	1491	1514	rBV2	87034	190671	18.23%	2.446%
28	5.989	1528	1539	1563	rBV2	231636	474749	45.40%	6.090%
29	6.329	1642	1645	1646	rBV3	1049	580	0.06%	0.007%
30	6.436	1675	1678	1680	rBV2	1068	663	0.06%	0.009%
31	6.481	1689	1692	1694	rBV4	1079	614	0.06%	0.008%
32	6.529	1705	1707	1709	rBV3	1190	586	0.06%	0.008%
33	6.555	1712	1715	1716	rBV3	781	330	0.03%	0.004%
34	6.571	1718	1720	1723	rBV3	1224	788	0.08%	0.010%
35	6.638	1739	1741	1742	rBV2	952	351	0.03%	0.005%
36	6.696	1757	1759	1761	rBV3	1275	546	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033516.D
 Acq On : 20 Dec 2023 16:51
 Operator : SY/MD
 Sample : 05927-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.850	1804	1807	1813	rVB6	1714	1462	0.14%	0.019%
38	6.915	1817	1827	1853	rVV	108974	213580	20.43%	2.740%
39	7.243	1918	1929	1952	rBV	428927	768767	73.52%	9.861%
40	7.554	2017	2026	2045	rBV	77909	142482	13.63%	1.828%
41	7.863	2118	2122	2123	rBV5	2308	1623	0.16%	0.021%
42	7.905	2133	2135	2136	rBV2	918	347	0.03%	0.004%
43	7.963	2152	2153	2155	rBV	725	338	0.03%	0.004%
44	8.027	2163	2173	2205	rBV	170940	378561	36.20%	4.856%
45	8.641	2362	2364	2366	rBV3	1062	420	0.04%	0.005%
46	8.786	2398	2409	2437	rBV	485624	810577	77.52%	10.398%
47	9.197	2534	2537	2541	rBV5	1808	1556	0.15%	0.020%
48	9.255	2553	2555	2560	rVB6	827	543	0.05%	0.007%
49	9.278	2560	2562	2565	rBV3	1232	647	0.06%	0.008%
50	9.297	2565	2568	2569	rBV2	1432	698	0.07%	0.009%
51	9.381	2591	2594	2598	rBV5	1531	1001	0.10%	0.013%
52	9.500	2627	2631	2633	rBV5	1311	1089	0.10%	0.014%
53	9.554	2646	2648	2652	rBV3	963	651	0.06%	0.008%
54	9.587	2656	2658	2659	rBV2	1245	554	0.05%	0.007%
55	9.644	2674	2676	2678	rBV2	875	436	0.04%	0.006%
56	9.686	2686	2689	2693	rBV6	901	633	0.06%	0.008%
57	9.808	2724	2727	2729	rBV3	1253	582	0.06%	0.007%
58	9.927	2762	2764	2766	rBV3	1005	513	0.05%	0.007%
59	10.001	2782	2787	2788	rBV3	1495	1101	0.11%	0.014%
60	10.046	2799	2801	2804	rBV4	1239	717	0.07%	0.009%
61	10.152	2823	2834	2853	rBV	298949	475061	45.43%	6.094%
62	10.320	2880	2886	2892	rBV9	3578	4897	0.47%	0.063%
63	10.474	2931	2934	2935	rBV2	877	528	0.05%	0.007%
64	10.564	2959	2962	2964	rBV3	1436	694	0.07%	0.009%
65	10.580	2964	2967	2968	rBV3	1538	860	0.08%	0.011%
66	10.712	3005	3008	3012	rVB4	930	784	0.07%	0.010%
67	10.757	3019	3022	3024	rBV3	1111	749	0.07%	0.010%
68	10.789	3027	3032	3034	rBV3	1328	1101	0.11%	0.014%
69	10.828	3040	3044	3046	rBV3	1170	862	0.08%	0.011%
70	10.969	3085	3088	3090	rVB3	1097	587	0.06%	0.008%
71	10.985	3090	3093	3096	rBV3	1392	935	0.09%	0.012%
72	11.053	3112	3114	3118	rVB4	1525	928	0.09%	0.012%
73	11.185	3145	3155	3177	rBV	443564	692602	66.24%	8.884%
74	11.561	3262	3272	3290	rBV	443921	704193	67.34%	9.033%
75	11.882	3370	3372	3375	rBV3	1727	1159	0.11%	0.015%
76	12.037	3418	3420	3421	rBV2	1068	354	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033516.D
 Acq On : 20 Dec 2023 16:51
 Operator : SY/MD
 Sample : 05927-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGWC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.230	3478	3480	3483	rBV4	966	739	0.07%	0.009%
78	12.368	3521	3523	3525	rBV2	780	339	0.03%	0.004%
79	12.387	3527	3529	3532	rVB4	1496	566	0.05%	0.007%
80	12.413	3532	3537	3539	rVB5	1163	950	0.09%	0.012%
81	12.426	3539	3541	3544	rBV3	818	450	0.04%	0.006%
82	12.532	3571	3574	3576	rBV3	1427	856	0.08%	0.011%
83	12.715	3629	3631	3632	rBV	1480	583	0.06%	0.007%
84	12.750	3640	3642	3645	rBB4	838	329	0.03%	0.004%
85	13.075	3741	3743	3745	rBV3	829	503	0.05%	0.006%
86	13.098	3748	3750	3753	rVB3	1556	813	0.08%	0.010%
87	13.114	3753	3755	3756	rBV	865	339	0.03%	0.004%
88	13.278	3804	3806	3809	rBV3	1222	539	0.05%	0.007%
89	13.429	3852	3853	3855	rBV3	764	330	0.03%	0.004%
90	13.541	3883	3888	3890	rBV6	1907	1595	0.15%	0.020%
91	13.676	3928	3930	3933	rBV4	1291	820	0.08%	0.011%
92	13.863	3984	3988	3989	rBV3	777	553	0.05%	0.007%
93	13.950	4010	4015	4017	rBV4	1522	1213	0.12%	0.016%
94	13.992	4024	4028	4031	rBV5	1086	1096	0.10%	0.014%
95	14.078	4053	4055	4058	rBV4	1183	739	0.07%	0.009%
96	14.114	4064	4066	4067	rBV2	1166	571	0.05%	0.007%
97	14.252	4106	4109	4111	rBV4	848	490	0.05%	0.006%
98	14.342	4134	4137	4140	rBV4	1655	1347	0.13%	0.017%
99	14.586	4211	4213	4215	rBV3	1641	749	0.07%	0.010%
100	14.696	4243	4247	4249	rBV4	1268	1058	0.10%	0.014%




Sum of corrected areas: 7795644

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033516.D
Acq On : 20 Dec 2023 16:51
Operator : SY/MD
Sample : 05927-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

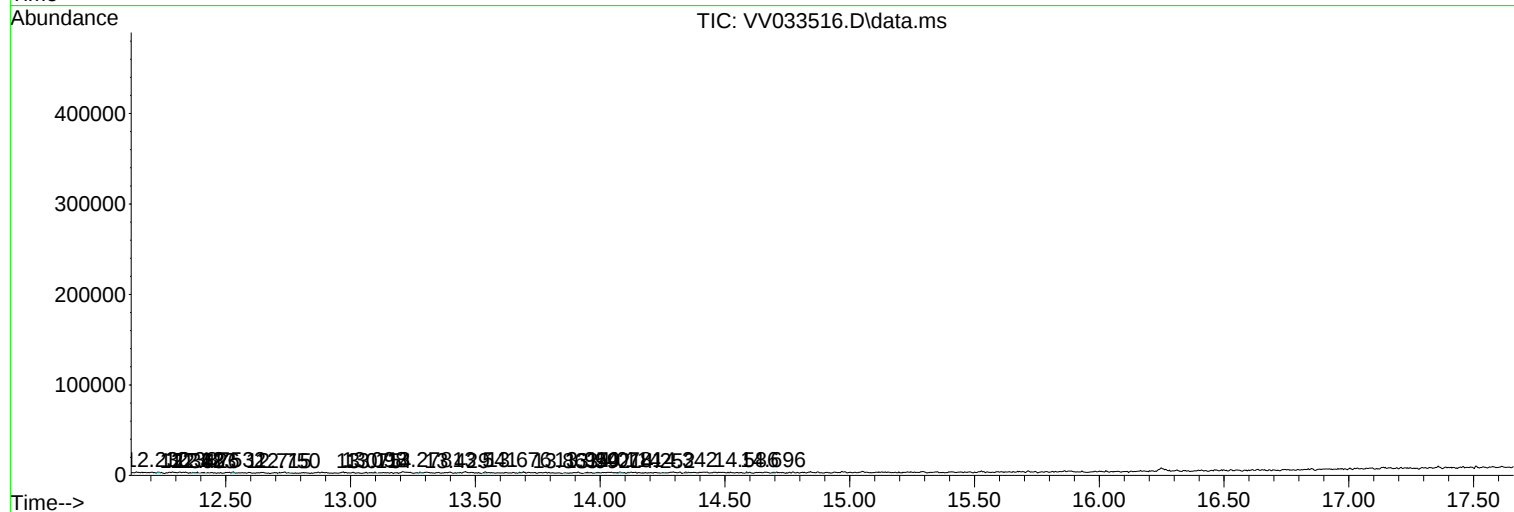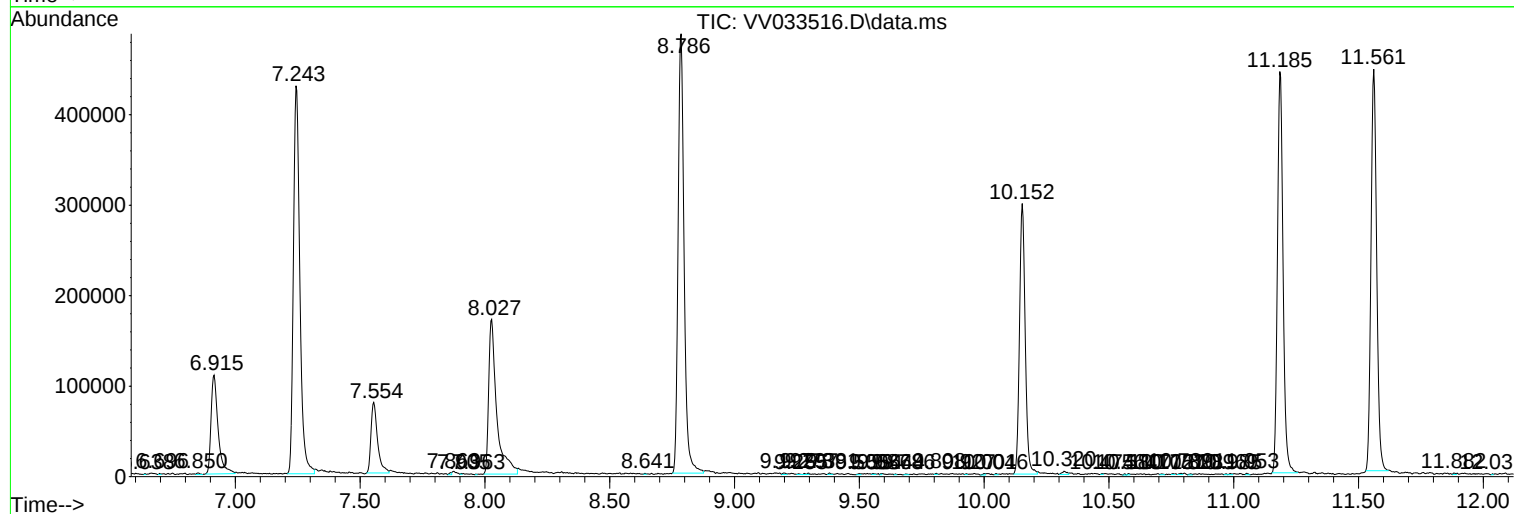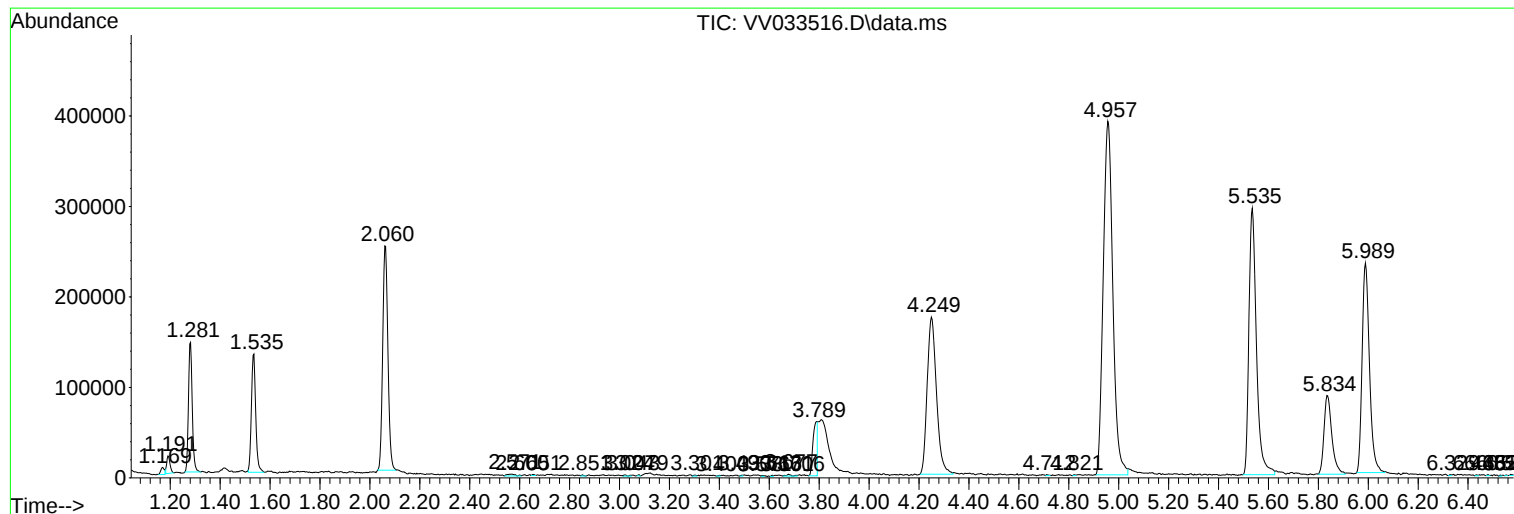

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033516.D
Acq On : 20 Dec 2023 16:51
Operator : SY/MD
Sample : 05927-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033516.D
Acq On : 20 Dec 2023 16:51
Operator : SY/MD
Sample : 05927-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGWC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------