

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033519.D
 Acq On : 20 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05927-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	45	rBV	10126	10856	1.05%	0.142%
2	1.278	68	74	89	rVB	147758	157717	15.22%	2.068%
3	1.532	146	153	167	rVB	136566	160358	15.48%	2.103%
4	2.060	308	317	334	rBV	257733	378916	36.57%	4.968%
5	2.548	463	469	471	rBV5	1869	1602	0.15%	0.021%
6	2.616	488	490	492	rBV2	1274	556	0.05%	0.007%
7	2.683	509	511	513	rBV2	1242	715	0.07%	0.009%
8	2.757	530	534	538	rBV6	2134	1899	0.18%	0.025%
9	2.822	551	554	557	rBV5	1017	585	0.06%	0.008%
10	2.838	557	559	562	rBV4	733	455	0.04%	0.006%
11	2.883	567	573	579	rBV9	1704	2313	0.22%	0.030%
12	2.963	596	598	601	rBV4	1099	808	0.08%	0.011%
13	3.063	627	629	631	rBV3	1026	527	0.05%	0.007%
14	3.085	634	636	638	rBV3	1122	471	0.05%	0.006%
15	3.166	659	661	665	rBV3	1222	1069	0.10%	0.014%
16	3.217	675	677	680	rVB2	889	599	0.06%	0.008%
17	3.236	680	683	684	rBV4	1041	478	0.05%	0.006%
18	3.304	701	704	707	rBV4	1028	670	0.06%	0.009%
19	3.420	736	740	741	rBV4	940	744	0.07%	0.010%
20	3.500	761	765	769	rBV6	1055	932	0.09%	0.012%
21	3.548	777	780	783	rBV4	1191	908	0.09%	0.012%
22	3.568	783	786	787	rVV2	878	413	0.04%	0.005%
23	3.603	793	797	801	rBV6	1394	938	0.09%	0.012%
24	3.703	825	828	830	rVB5	947	470	0.05%	0.006%
25	3.731	835	837	841	rBV5	1183	976	0.09%	0.013%
26	3.786	843	854	879	rBV	52989	160378	15.48%	2.103%
27	4.246	984	997	1023	rBV	170673	432323	41.72%	5.668%
28	4.420	1049	1051	1054	rBV3	1584	908	0.09%	0.012%
29	4.651	1121	1123	1126	rBV4	1458	1071	0.10%	0.014%
30	4.690	1133	1135	1139	rVB4	1525	978	0.09%	0.013%
31	4.722	1142	1145	1147	rBV3	1357	889	0.09%	0.012%
32	4.767	1157	1159	1160	rBV2	1043	450	0.04%	0.006%
33	4.866	1187	1190	1191	rBV4	1958	864	0.08%	0.011%
34	4.895	1196	1199	1200	rBV3	838	533	0.05%	0.007%
35	4.957	1202	1218	1248	rVV2	383634	1036150	100.00%	13.585%
36	5.535	1386	1398	1422	rBV	285516	605468	58.43%	7.938%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033519.D
 Acq On : 20 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05927-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	5.934	1519	1522	1524	rBV4	1359	941	0.09%	0.012%
38	5.985	1527	1538	1566	rVV	228121	483723	46.68%	6.342%
39	6.182	1598	1599	1604	rBV5	1521	1042	0.10%	0.014%
40	6.445	1678	1681	1684	rBV4	1435	1176	0.11%	0.015%
41	6.481	1690	1692	1693	rBV3	992	408	0.04%	0.005%
42	6.600	1727	1729	1733	rBV3	1054	678	0.07%	0.009%
43	6.915	1816	1827	1846	rBV	104139	203059	19.60%	2.662%
44	7.243	1918	1929	1952	rBV	417654	749975	72.38%	9.833%
45	7.551	2017	2025	2048	rBV	76292	141379	13.64%	1.854%
46	7.879	2123	2127	2132	rVB7	1922	2205	0.21%	0.029%
47	7.915	2136	2138	2140	rBV2	1163	538	0.05%	0.007%
48	7.966	2152	2154	2157	rBV4	784	512	0.05%	0.007%
49	7.979	2157	2158	2162	rBV4	1224	868	0.08%	0.011%
50	8.024	2163	2172	2205	rBV	172607	377624	36.44%	4.951%
51	8.718	2386	2388	2391	rBV3	1071	512	0.05%	0.007%
52	8.786	2395	2409	2431	rBV	489152	818544	79.00%	10.732%
53	9.159	2523	2525	2530	rVB5	1830	1064	0.10%	0.014%
54	9.233	2545	2548	2554	rBV4	1537	1267	0.12%	0.017%
55	9.490	2622	2628	2630	rBV5	1748	1721	0.17%	0.023%
56	9.628	2668	2671	2675	rVB5	1592	1477	0.14%	0.019%
57	9.648	2675	2677	2678	rBV	942	392	0.04%	0.005%
58	9.683	2686	2688	2694	rVB4	1580	1106	0.11%	0.015%
59	9.712	2694	2697	2701	rBV5	1249	1055	0.10%	0.014%
60	9.731	2701	2703	2705	rVV3	1065	508	0.05%	0.007%
61	9.860	2740	2743	2747	rVB5	1504	1283	0.12%	0.017%
62	9.876	2747	2748	2751	rBV3	1207	800	0.08%	0.010%
63	10.078	2808	2811	2812	rBV2	1231	561	0.05%	0.007%
64	10.152	2821	2834	2858	rBV	298399	484735	46.78%	6.356%
65	10.387	2901	2907	2909	rBV7	1036	1005	0.10%	0.013%
66	10.484	2934	2937	2939	rBV4	1213	548	0.05%	0.007%
67	10.522	2946	2949	2950	rBV3	974	482	0.05%	0.006%
68	10.622	2978	2980	2982	rVB3	1659	484	0.05%	0.006%
69	10.638	2982	2985	2987	rBV4	1165	820	0.08%	0.011%
70	10.677	2994	2997	3000	rVB5	1247	901	0.09%	0.012%
71	10.702	3002	3005	3007	rBV4	1361	701	0.07%	0.009%
72	10.718	3008	3010	3012	rBV3	883	439	0.04%	0.006%
73	10.773	3024	3027	3028	rBV3	782	408	0.04%	0.005%
74	10.831	3042	3045	3047	rBV3	984	551	0.05%	0.007%
75	10.902	3064	3067	3068	rBV2	1067	563	0.05%	0.007%
76	10.914	3068	3071	3074	rVV4	1240	1019	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033519.D
 Acq On : 20 Dec 2023 18:04
 Operator : SY/MD
 Sample : 05927-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	10.947	3078	3081	3083	rBV4	953	632	0.06%	0.008%
78	10.998	3095	3097	3100	rBV2	1183	758	0.07%	0.010%
79	11.104	3128	3130	3134	rVB5	957	519	0.05%	0.007%
80	11.185	3144	3155	3179	rBV	431704	678637	65.50%	8.898%
81	11.406	3222	3224	3225	rBV	914	388	0.04%	0.005%
82	11.561	3262	3272	3290	rVB	439986	677847	65.42%	8.887%
83	11.956	3393	3395	3399	rBV4	859	587	0.06%	0.008%
84	12.030	3415	3418	3421	rBV4	1219	840	0.08%	0.011%
85	12.242	3482	3484	3487	rBV4	1316	940	0.09%	0.012%
86	12.278	3493	3495	3497	rBV3	735	434	0.04%	0.006%
87	12.403	3532	3534	3538	rBV5	1446	892	0.09%	0.012%
88	12.525	3570	3572	3574	rBV3	1238	532	0.05%	0.007%
89	12.622	3600	3602	3607	rBV5	1141	1165	0.11%	0.015%
90	12.840	3666	3670	3673	rVV5	1106	937	0.09%	0.012%
91	12.966	3707	3709	3712	rBV3	935	618	0.06%	0.008%
92	13.201	3778	3782	3783	rBV4	877	578	0.06%	0.008%
93	13.673	3924	3929	3932	rBV4	1762	1685	0.16%	0.022%
94	14.570	4206	4208	4211	rBV3	1283	896	0.09%	0.012%
95	14.705	4248	4250	4255	rBV6	1382	1125	0.11%	0.015%
96	15.072	4362	4364	4366	rBV	941	462	0.04%	0.006%
97	15.168	4391	4394	4400	rBV6	1299	1140	0.11%	0.015%
98	15.319	4438	4441	4444	rBV4	1232	1173	0.11%	0.015%
99	15.480	4488	4491	4492	rBV2	1012	612	0.06%	0.008%
100	15.689	4554	4556	4557	rBV2	1450	539	0.05%	0.007%


Sum of corrected areas: 7626997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033519.D
Acq On : 20 Dec 2023 18:04
Operator : SY/MD
Sample : 05927-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

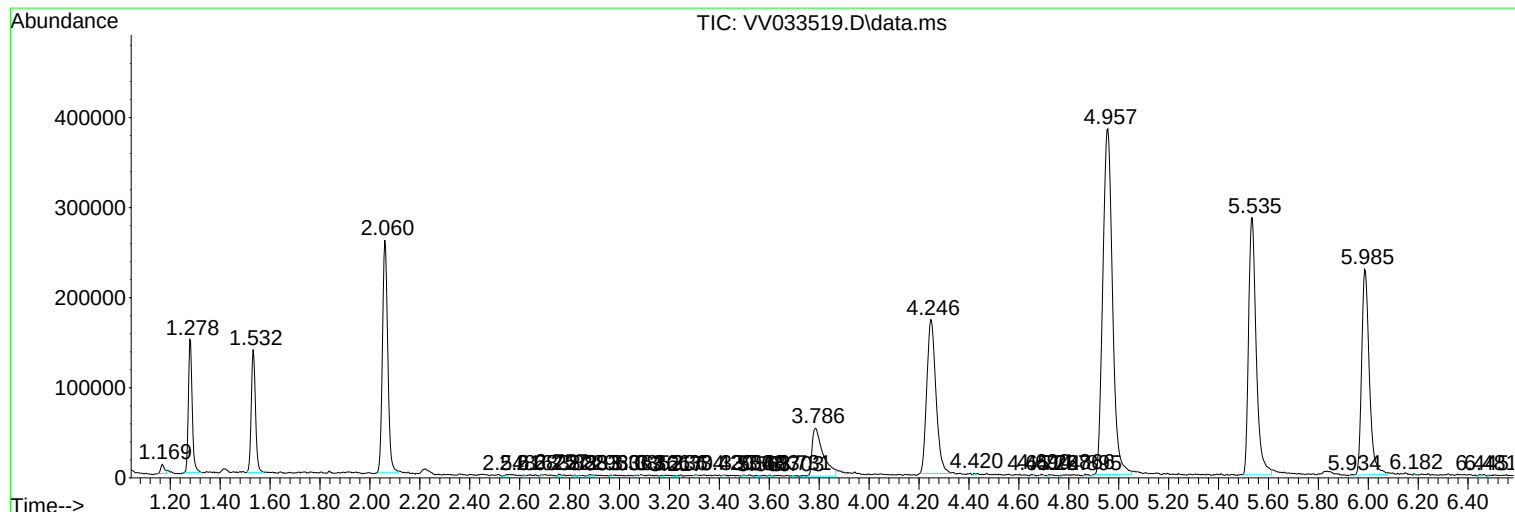

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033519.D
Acq On : 20 Dec 2023 18:04
Operator : SY/MD
Sample : 05927-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033519.D
Acq On : 20 Dec 2023 18:04
Operator : SY/MD
Sample : 05927-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc