

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033520.D
 Acq On : 20 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05927-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	151697	159117	15.40%	2.099%
2	1.532	146	153	166	rVB	133381	160024	15.49%	2.111%
3	2.060	308	317	334	rBV	256436	371679	35.98%	4.903%
4	2.298	389	391	395	rBV3	1168	763	0.07%	0.010%
5	2.716	517	521	525	rBV6	990	1081	0.10%	0.014%
6	2.847	560	562	568	rVB5	1261	904	0.09%	0.012%
7	2.960	594	597	599	rBV4	867	497	0.05%	0.007%
8	3.063	625	629	632	rBV6	623	524	0.05%	0.007%
9	3.130	646	650	652	rVB5	908	701	0.07%	0.009%
10	3.169	661	662	665	rBV3	1218	684	0.07%	0.009%
11	3.201	670	672	674	rVB3	1252	574	0.06%	0.008%
12	3.307	703	705	709	rVB5	1136	783	0.08%	0.010%
13	3.339	713	715	717	rBV3	1424	721	0.07%	0.010%
14	3.455	748	751	752	rBV2	1169	520	0.05%	0.007%
15	3.474	752	757	758	rBV4	1032	685	0.07%	0.009%
16	3.539	774	777	779	rBV4	1107	701	0.07%	0.009%
17	3.680	817	821	824	rBV6	1006	1065	0.10%	0.014%
18	3.703	824	828	830	rBV3	1231	848	0.08%	0.011%
19	3.741	837	840	843	rBV4	1224	939	0.09%	0.012%
20	3.786	843	854	883	rBV	56121	172192	16.67%	2.272%
21	4.076	942	944	947	rBV3	1142	609	0.06%	0.008%
22	4.159	966	970	975	rBV8	1220	1457	0.14%	0.019%
23	4.249	981	998	1020	rBV	169061	439515	42.54%	5.798%
24	4.728	1145	1147	1150	rVB4	1226	719	0.07%	0.009%
25	4.751	1150	1154	1156	rBV5	1249	764	0.07%	0.010%
26	4.957	1202	1218	1247	rBV2	381365	1033135	100.00%	13.629%
27	5.532	1387	1397	1424	rBV	278593	590639	57.17%	7.792%
28	5.815	1480	1485	1487	rBV5	3026	2897	0.28%	0.038%
29	5.989	1526	1539	1563	rBV	233196	485757	47.02%	6.408%
30	6.259	1620	1623	1627	rBV5	794	698	0.07%	0.009%
31	6.371	1656	1658	1662	rVB4	1193	689	0.07%	0.009%
32	6.397	1662	1666	1667	rBV3	1122	825	0.08%	0.011%
33	6.481	1689	1692	1693	rBV3	1109	567	0.05%	0.007%
34	6.516	1699	1703	1706	rBV4	1290	1120	0.11%	0.015%
35	6.651	1741	1745	1751	rVB7	1312	1423	0.14%	0.019%
36	6.683	1751	1755	1757	rBV4	833	714	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033520.D
 Acq On : 20 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05927-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.725	1766	1768	1773	rVB6	1311	619	0.06%	0.008%
38	6.764	1777	1780	1782	rBV3	1395	861	0.08%	0.011%
39	6.818	1794	1797	1798	rBV3	1137	581	0.06%	0.008%
40	6.841	1802	1804	1808	rBV5	971	734	0.07%	0.010%
41	6.915	1817	1827	1846	rBV	104900	202193	19.57%	2.667%
42	7.243	1919	1929	1953	rBV	419138	748966	72.49%	9.880%
43	7.555	2017	2026	2041	rBV	78425	140451	13.59%	1.853%
44	7.838	2113	2114	2117	rBV3	973	620	0.06%	0.008%
45	7.957	2149	2151	2154	rBV4	1016	590	0.06%	0.008%
46	7.982	2154	2159	2160	rBV4	1225	1106	0.11%	0.015%
47	8.024	2163	2172	2212	rBV	175332	393360	38.07%	5.189%
48	8.442	2300	2302	2304	rBV2	996	527	0.05%	0.007%
49	8.706	2382	2384	2390	rBV6	1022	1039	0.10%	0.014%
50	8.783	2398	2408	2431	rBV	465482	789732	76.44%	10.418%
51	8.995	2471	2474	2479	rBV7	1249	942	0.09%	0.012%
52	9.284	2560	2564	2568	rVB7	1038	708	0.07%	0.009%
53	9.497	2626	2630	2634	rVB6	1522	1025	0.10%	0.014%
54	9.542	2639	2644	2650	rBV7	1567	1705	0.17%	0.022%
55	9.567	2650	2652	2655	rVB3	1386	734	0.07%	0.010%
56	9.818	2728	2730	2733	rBV4	922	511	0.05%	0.007%
57	10.040	2796	2799	2802	rVB4	820	639	0.06%	0.008%
58	10.056	2802	2804	2809	rVB4	889	546	0.05%	0.007%
59	10.153	2822	2834	2858	rBV	299079	476008	46.07%	6.279%
60	10.413	2913	2915	2918	rBV4	1064	701	0.07%	0.009%
61	10.477	2932	2935	2937	rBV3	1419	932	0.09%	0.012%
62	10.738	3013	3016	3018	rBV4	1050	625	0.06%	0.008%
63	10.818	3039	3041	3044	rBV3	1201	772	0.07%	0.010%
64	10.834	3044	3046	3050	rVV3	934	710	0.07%	0.009%
65	10.854	3050	3052	3056	rVV5	1419	890	0.09%	0.012%
66	10.882	3056	3061	3064	rVB5	1141	936	0.09%	0.012%
67	10.902	3064	3067	3072	rBV6	1253	963	0.09%	0.013%
68	10.992	3092	3095	3097	rVB3	948	552	0.05%	0.007%
69	11.082	3121	3123	3129	rVB5	1186	878	0.08%	0.012%
70	11.120	3132	3135	3141	rVB7	1159	920	0.09%	0.012%
71	11.185	3144	3155	3178	rBV	421875	661628	64.04%	8.728%
72	11.378	3213	3215	3217	rVB3	1294	492	0.05%	0.006%
73	11.413	3224	3226	3228	rBV3	1118	613	0.06%	0.008%
74	11.561	3261	3272	3297	rBV	427334	684424	66.25%	9.029%
75	11.812	3346	3350	3351	rBV4	990	608	0.06%	0.008%
76	12.030	3413	3418	3420	rBV4	1873	1381	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033520.D
 Acq On : 20 Dec 2023 18:27
 Operator : SY/MD
 Sample : 05927-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.181	3462	3465	3469	rVB6	1438	1153	0.11%	0.015%
78	12.207	3469	3473	3474	rBV3	1391	881	0.09%	0.012%
79	12.262	3486	3490	3493	rBV3	1455	1353	0.13%	0.018%
80	12.477	3555	3557	3562	rVB5	1008	670	0.06%	0.009%
81	12.503	3562	3565	3567	rBV3	875	485	0.05%	0.006%
82	12.664	3612	3615	3619	rBV2	1022	949	0.09%	0.013%
83	12.693	3619	3624	3628	rBV7	1011	1153	0.11%	0.015%
84	12.821	3661	3664	3667	rBV5	820	536	0.05%	0.007%
85	12.857	3670	3675	3678	rBV4	1417	1216	0.12%	0.016%
86	12.934	3698	3699	3702	rVB3	1359	545	0.05%	0.007%
87	12.950	3702	3704	3706	rBV2	1408	499	0.05%	0.007%
88	12.966	3707	3709	3714	rVB3	1182	940	0.09%	0.012%
89	12.998	3714	3719	3720	rBV3	1243	796	0.08%	0.011%
90	13.056	3735	3737	3742	rBV5	1361	866	0.08%	0.011%
91	13.091	3745	3748	3750	rBV3	967	680	0.07%	0.009%
92	13.204	3780	3783	3784	rBV3	1789	824	0.08%	0.011%
93	13.374	3833	3836	3838	rBV3	887	643	0.06%	0.008%
94	14.149	4075	4077	4081	rVB4	1141	903	0.09%	0.012%
95	14.175	4083	4085	4086	rBV2	1185	503	0.05%	0.007%
96	14.426	4158	4163	4164	rBV5	1483	1030	0.10%	0.014%
97	14.808	4280	4282	4286	rBV3	1399	1220	0.12%	0.016%
98	15.078	4363	4366	4368	rBV4	1718	1200	0.12%	0.016%
99	15.320	4437	4441	4444	rBV4	1639	1249	0.12%	0.016%
100	15.342	4444	4448	4450	rBV5	1710	1494	0.14%	0.020%


Sum of corrected areas: 7580540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033520.D
Acq On : 20 Dec 2023 18:27
Operator : SY/MD
Sample : 05927-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

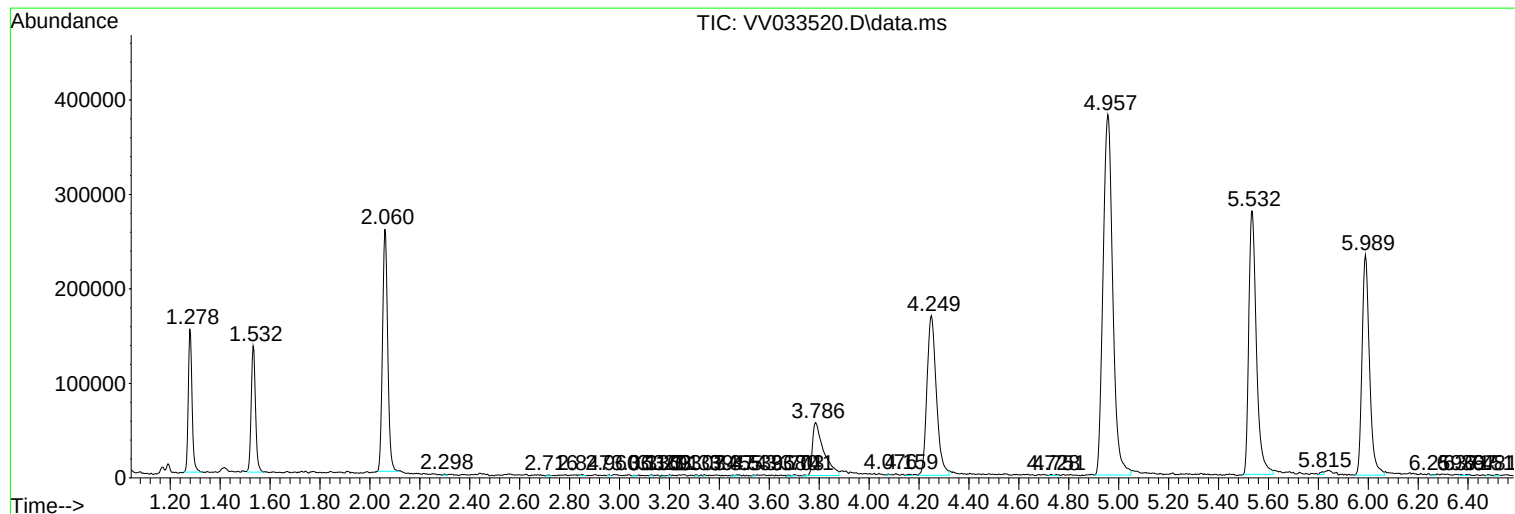

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033520.D
Acq On : 20 Dec 2023 18:27
Operator : SY/MD
Sample : 05927-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033520.D
Acq On : 20 Dec 2023 18:27
Operator : SY/MD
Sample : 05927-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc