

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033521.D
 Acq On : 20 Dec 2023 18:50
 Operator : SY/MD
 Sample : 05850-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VW033521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rVB	150798	157181	11.75%	1.820%
2	1.532	146	153	168	rVB	132859	158930	11.88%	1.840%
3	2.059	308	317	330	rBV	248446	365300	27.30%	4.230%
4	2.805	544	549	552	rBV7	1853	1446	0.11%	0.017%
5	2.883	571	573	575	rVB	641	273	0.02%	0.003%
6	2.899	575	578	581	rVB4	1469	884	0.07%	0.010%
7	2.912	581	582	585	rBV3	1001	551	0.04%	0.006%
8	3.002	608	610	614	rBV5	853	636	0.05%	0.007%
9	3.034	618	620	624	rVV5	1091	546	0.04%	0.006%
10	3.050	624	625	629	rVB4	1755	946	0.07%	0.011%
11	3.075	629	633	634	rBV2	1370	876	0.07%	0.010%
12	3.127	646	649	654	rBV7	1699	1806	0.13%	0.021%
13	3.391	729	731	732	rBV2	1043	414	0.03%	0.005%
14	3.432	740	744	747	rBV4	1113	899	0.07%	0.010%
15	3.481	757	759	762	rVB3	909	432	0.03%	0.005%
16	3.510	767	768	771	rVB2	897	409	0.03%	0.005%
17	3.529	771	774	777	rBV3	585	396	0.03%	0.005%
18	3.555	777	782	783	rBV5	1340	1020	0.08%	0.012%
19	3.667	815	817	820	rBV3	708	615	0.05%	0.007%
20	3.706	826	829	830	rBV3	1041	603	0.05%	0.007%
21	3.735	834	838	842	rBV7	1288	1229	0.09%	0.014%
22	3.786	845	854	881	rBV	55269	155346	11.61%	1.799%
23	4.249	985	998	1024	rVB2	160743	408243	30.51%	4.727%
24	4.493	1072	1074	1077	rBV4	1987	1066	0.08%	0.012%
25	4.593	1103	1105	1110	rVB5	1386	1003	0.07%	0.012%
26	4.844	1181	1183	1185	rVB3	1216	497	0.04%	0.006%
27	4.863	1185	1189	1193	rBV5	1764	1096	0.08%	0.013%
28	4.956	1202	1218	1246	rBV2	376538	1019100	76.17%	11.800%
29	5.358	1339	1343	1345	rBV3	1671	1136	0.08%	0.013%
30	5.403	1353	1357	1359	rBV5	944	834	0.06%	0.010%
31	5.474	1377	1379	1381	rVB3	1183	456	0.03%	0.005%
32	5.490	1381	1384	1387	rBV5	1422	712	0.05%	0.008%
33	5.535	1387	1398	1423	rBV	287000	608293	45.47%	7.044%
34	5.931	1519	1521	1525	rVB3	1653	794	0.06%	0.009%
35	5.989	1525	1539	1564	rBV	225365	477161	35.66%	5.525%
36	6.442	1677	1680	1681	rBV3	1130	467	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033521.D
 Acq On : 20 Dec 2023 18:50
 Operator : SY/MD
 Sample : 05850-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.458	1681	1685	1686	rBV5	985	727	0.05%	0.008%
38	6.538	1704	1710	1713	rBV7	1171	1553	0.12%	0.018%
39	6.596	1725	1728	1729	rBV2	967	496	0.04%	0.006%
40	6.677	1751	1753	1756	rBV4	517	324	0.02%	0.004%
41	6.915	1816	1827	1845	rBV	104929	200447	14.98%	2.321%
42	7.246	1918	1930	1953	rBV	408625	734407	54.89%	8.504%
43	7.554	2016	2026	2045	rBV	77445	142398	10.64%	1.649%
44	7.947	2146	2148	2151	rBV4	853	562	0.04%	0.007%
45	8.027	2164	2173	2209	rBV	165470	362506	27.09%	4.198%
46	8.628	2358	2360	2361	rBV2	1284	546	0.04%	0.006%
47	8.786	2395	2409	2439	rBV	498537	938516	70.15%	10.867%
48	9.181	2529	2532	2534	rVB4	1230	630	0.05%	0.007%
49	9.249	2550	2553	2554	rBV3	934	544	0.04%	0.006%
50	9.284	2562	2564	2566	rBV3	1062	460	0.03%	0.005%
51	9.349	2580	2584	2586	rBV5	1302	951	0.07%	0.011%
52	9.513	2633	2635	2637	rVB3	1886	705	0.05%	0.008%
53	9.529	2637	2640	2641	rBV3	1398	617	0.05%	0.007%
54	9.718	2696	2699	2700	rBV2	1404	610	0.05%	0.007%
55	9.750	2706	2709	2712	rVB4	1109	675	0.05%	0.008%
56	9.767	2712	2714	2715	rBV2	877	307	0.02%	0.004%
57	9.924	2758	2763	2764	rBV4	1068	738	0.06%	0.009%
58	9.972	2776	2778	2779	rBV2	698	361	0.03%	0.004%
59	10.040	2797	2799	2802	rVB4	1066	605	0.05%	0.007%
60	10.075	2805	2810	2812	rBV5	1918	1605	0.12%	0.019%
61	10.107	2816	2820	2822	rVV5	1163	932	0.07%	0.011%
62	10.152	2823	2834	2861	rVB	295336	472246	35.30%	5.468%
63	10.496	2940	2941	2945	rVB4	844	386	0.03%	0.004%
64	10.628	2975	2982	2985	rBV5	1073	1251	0.09%	0.014%
65	10.718	3008	3010	3015	rBV5	894	778	0.06%	0.009%
66	10.783	3027	3030	3031	rBV2	904	490	0.04%	0.006%
67	10.821	3040	3042	3045	rBV3	1126	687	0.05%	0.008%
68	10.953	3081	3083	3085	rBV3	977	374	0.03%	0.004%
69	11.017	3101	3103	3106	rVB3	848	454	0.03%	0.005%
70	11.046	3109	3112	3118	rBV7	1629	1600	0.12%	0.019%
71	11.123	3126	3136	3144	rBV2	16311	26320	1.97%	0.305%
72	11.184	3146	3155	3180	rVB	454295	783617	58.57%	9.074%
73	11.371	3210	3213	3215	rBV2	1778	1109	0.08%	0.013%
74	11.567	3261	3274	3292	rBV2	568526	1337929	100.00%	15.492%
75	11.808	3346	3349	3355	rBV7	1220	1331	0.10%	0.015%
76	11.831	3355	3356	3359	rBV2	1310	751	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033521.D
 Acq On : 20 Dec 2023 18:50
 Operator : SY/MD
 Sample : 05850-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QL7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

77	12.111	3441	3443	3445	rBV3	1214	626	0.05%	0.007%
78	12.175	3458	3463	3464	rBV4	1375	918	0.07%	0.011%
79	12.229	3475	3480	3485	rBV6	1354	1551	0.12%	0.018%
80	12.297	3498	3501	3504	rBV6	921	680	0.05%	0.008%
81	12.368	3521	3523	3525	rBV3	1071	609	0.05%	0.007%
82	12.844	3666	3671	3672	rBV3	1464	1085	0.08%	0.013%
83	12.873	3676	3680	3681	rBV4	1091	774	0.06%	0.009%
84	12.937	3697	3700	3704	rBV6	1052	843	0.06%	0.010%
85	13.056	3735	3737	3739	rBV3	805	423	0.03%	0.005%
86	13.078	3742	3744	3745	rBV2	1056	474	0.04%	0.005%
87	13.200	3771	3782	3800	rBV	88044	146209	10.93%	1.693%
88	13.387	3833	3840	3842	rBV6	1782	2037	0.15%	0.024%
89	13.455	3859	3861	3864	rBV3	1208	749	0.06%	0.009%
90	13.570	3895	3897	3899	rBV3	991	323	0.02%	0.004%
91	13.641	3917	3919	3921	rBV3	1233	600	0.04%	0.007%
92	13.683	3921	3932	3948	rVB	48280	79645	5.95%	0.922%
93	13.940	4008	4012	4014	rBV4	1139	741	0.06%	0.009%
94	14.065	4049	4051	4055	rBV4	835	549	0.04%	0.006%
95	14.249	4106	4108	4110	rBV3	855	518	0.04%	0.006%
96	14.287	4117	4120	4121	rBV3	1740	872	0.07%	0.010%
97	14.419	4158	4161	4164	rBV5	985	629	0.05%	0.007%
98	14.506	4183	4188	4190	rBV5	1498	1155	0.09%	0.013%
99	14.635	4226	4228	4230	rBV3	898	469	0.04%	0.005%
100	14.673	4238	4240	4242	rBV3	1268	547	0.04%	0.006%




Sum of corrected areas: 8636167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033521.D
Acq On : 20 Dec 2023 18:50
Operator : SY/MD
Sample : 05850-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

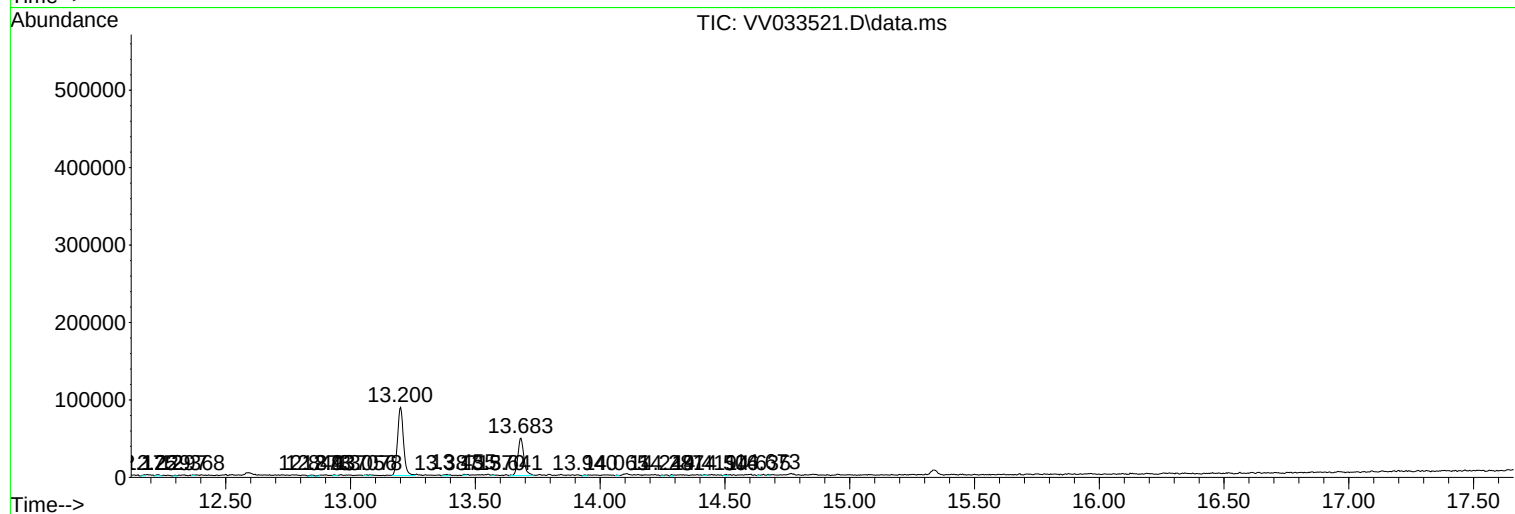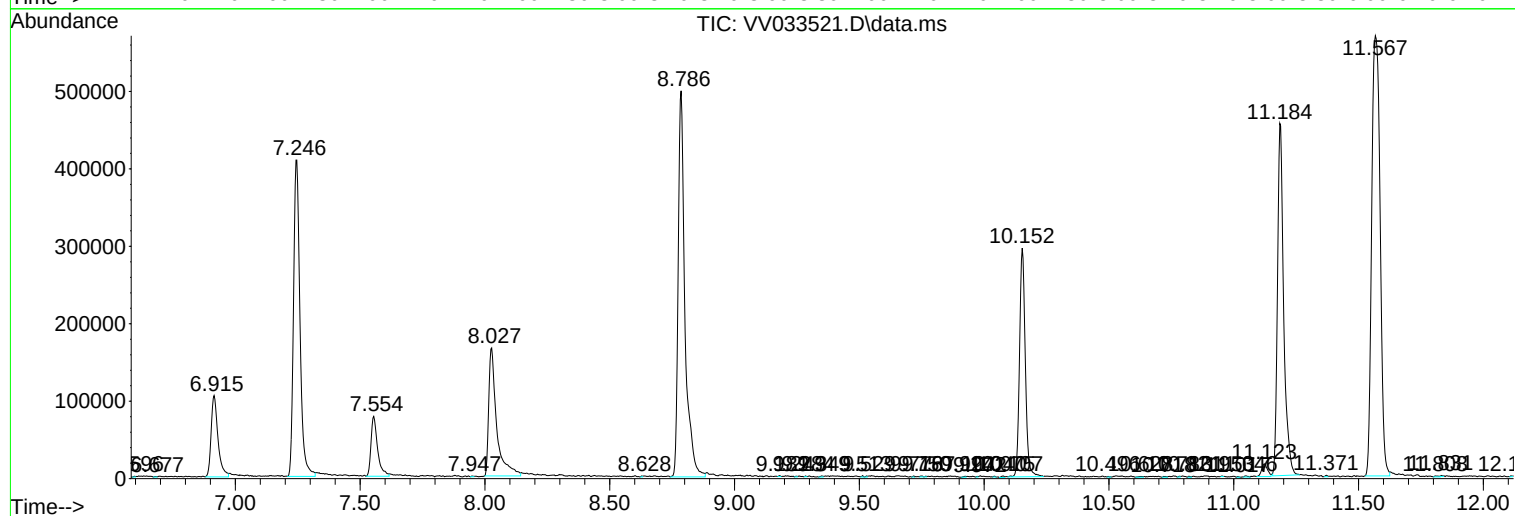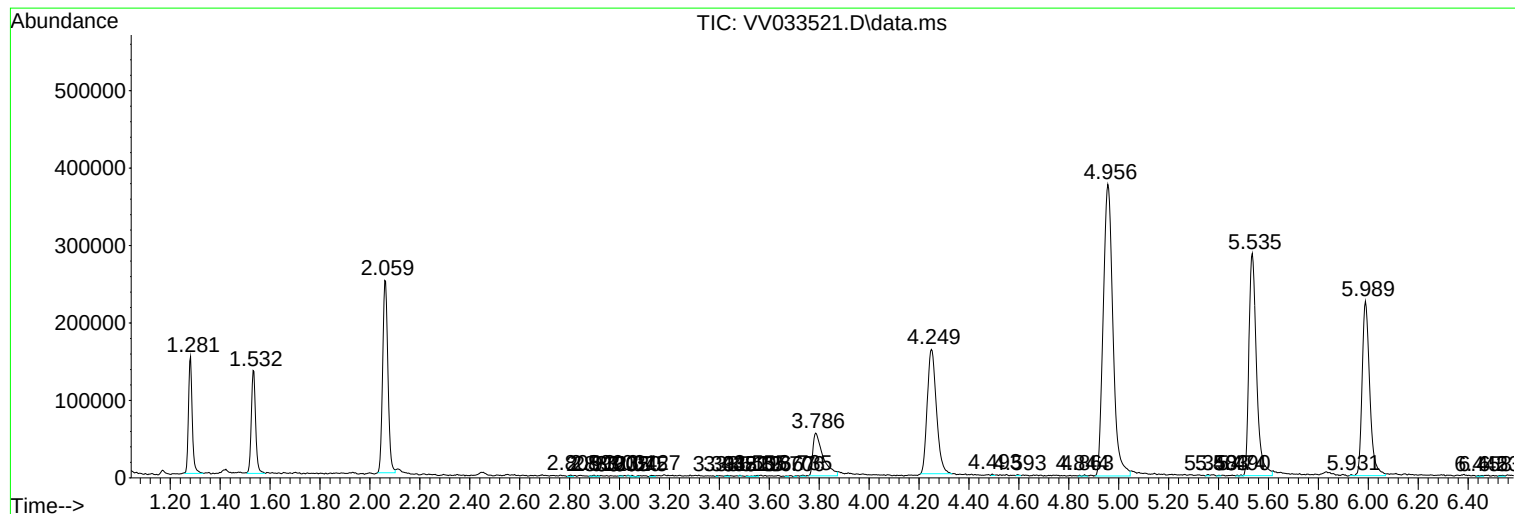

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033521.D
Acq On : 20 Dec 2023 18:50
Operator : SY/MD
Sample : 05850-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033521.D
Acq On : 20 Dec 2023 18:50
Operator : SY/MD
Sample : 05850-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QL7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------