

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033522.D
 Acq On : 20 Dec 2023 19:13
 Operator : SY/MD
 Sample : 05850-05DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rVB	155672	161610	10.14%	1.843%
2	1.532	146	153	169	rVB	136054	160101	10.04%	1.826%
3	2.060	308	317	334	rBV	260227	379181	23.78%	4.325%
4	2.413	425	427	428	rBV2	1128	348	0.02%	0.004%
5	2.799	542	547	549	rBV2	804	549	0.03%	0.006%
6	2.828	554	556	557	rBV2	1134	492	0.03%	0.006%
7	2.870	566	569	572	rBV3	1236	808	0.05%	0.009%
8	2.928	584	587	589	rVB4	1174	628	0.04%	0.007%
9	3.005	609	611	612	rBV	775	236	0.01%	0.003%
10	3.153	652	657	659	rBV6	1688	1624	0.10%	0.019%
11	3.326	708	711	713	rBV3	772	464	0.03%	0.005%
12	3.420	739	740	741	rBV3	651	136	0.01%	0.002%
13	3.433	741	744	745	rBV3	888	553	0.03%	0.006%
14	3.523	769	772	774	rBV4	990	909	0.06%	0.010%
15	3.600	794	796	799	rBV3	580	347	0.02%	0.004%
16	3.622	799	803	805	rBV5	968	869	0.05%	0.010%
17	3.677	818	820	824	rBV4	1236	746	0.05%	0.009%
18	3.751	842	843	844	rVB	729	141	0.01%	0.002%
19	3.786	844	854	877	rBV2	55346	157875	9.90%	1.801%
20	4.249	985	998	1023	rBV	168577	421652	26.45%	4.809%
21	4.857	1185	1187	1189	rBV3	1185	400	0.03%	0.005%
22	4.892	1196	1198	1201	rBV4	928	563	0.04%	0.006%
23	4.957	1201	1218	1231	rBV2	394671	1054992	66.17%	12.033%
24	5.535	1386	1398	1419	rBV	295810	623180	39.09%	7.108%
25	5.989	1528	1539	1559	rBV	230940	469664	29.46%	5.357%
26	6.477	1689	1691	1694	rBV4	1208	812	0.05%	0.009%
27	6.651	1741	1745	1748	rBV5	1978	1602	0.10%	0.018%
28	6.767	1777	1781	1783	rBV5	964	619	0.04%	0.007%
29	6.915	1816	1827	1843	rBV	107983	205593	12.90%	2.345%
30	7.243	1919	1929	1952	rBV	432855	762400	47.82%	8.696%
31	7.555	2017	2026	2045	rBV	77829	143073	8.97%	1.632%
32	7.873	2124	2125	2129	rBV4	1052	931	0.06%	0.011%
33	8.024	2164	2172	2196	rBV	183281	373774	23.44%	4.263%
34	8.362	2275	2277	2280	rBV3	1331	772	0.05%	0.009%
35	8.423	2291	2296	2300	rBV5	1810	2057	0.13%	0.023%
36	8.715	2385	2387	2389	rBV3	1171	650	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122023\
 Data File : VW033522.D
 Acq On : 20 Dec 2023 19:13
 Operator : SY/MD
 Sample : 05850-05DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.744	2395	2396	2397	rBV	1080	331	0.02%	0.004%
38	8.786	2398	2409	2411	rBV	555401	698100	43.79%	7.962%
39	9.313	2570	2573	2575	rBV4	1539	745	0.05%	0.008%
40	9.400	2598	2600	2602	rBV3	906	332	0.02%	0.004%
41	9.477	2620	2624	2627	rBV4	1012	937	0.06%	0.011%
42	9.554	2644	2648	2650	rBV3	2233	1400	0.09%	0.016%
43	9.590	2658	2659	2660	rVB	738	142	0.01%	0.002%
44	9.603	2660	2663	2665	rBV4	819	532	0.03%	0.006%
45	9.747	2706	2708	2712	rVB3	1324	631	0.04%	0.007%
46	9.853	2739	2741	2745	rVB5	1699	1061	0.07%	0.012%
47	9.876	2745	2748	2749	rBV2	1074	510	0.03%	0.006%
48	10.005	2785	2788	2790	rBV4	971	651	0.04%	0.007%
49	10.024	2790	2794	2796	rVB3	1043	705	0.04%	0.008%
50	10.046	2799	2801	2802	rBV2	899	253	0.02%	0.003%
51	10.085	2812	2813	2815	rBV2	513	171	0.01%	0.002%
52	10.153	2822	2834	2849	rBV	303942	480879	30.16%	5.485%
53	10.300	2877	2880	2882	rBV2	1898	1081	0.07%	0.012%
54	10.419	2916	2917	2919	rVB	857	293	0.02%	0.003%
55	10.432	2919	2921	2923	rBV3	1182	815	0.05%	0.009%
56	10.461	2928	2930	2932	rVV3	935	463	0.03%	0.005%
57	10.667	2992	2994	2998	rBV3	1808	1042	0.07%	0.012%
58	10.683	2998	2999	3001	rBV2	898	490	0.03%	0.006%
59	10.789	3030	3032	3034	rBV3	1119	548	0.03%	0.006%
60	10.834	3042	3046	3048	rBV4	1515	1297	0.08%	0.015%
61	10.870	3052	3057	3059	rBV6	1748	1423	0.09%	0.016%
62	10.918	3070	3072	3075	rBV3	1115	562	0.04%	0.006%
63	10.960	3083	3085	3088	rVB3	620	228	0.01%	0.003%
64	10.976	3088	3090	3091	rBV2	860	316	0.02%	0.004%
65	11.005	3094	3099	3103	rBV5	1004	969	0.06%	0.011%
66	11.021	3103	3104	3107	rVV2	940	421	0.03%	0.005%
67	11.120	3126	3135	3145	rBV3	40841	66735	4.19%	0.761%
68	11.188	3145	3156	3160	rBV	512417	825404	51.77%	9.414%
69	11.468	3240	3243	3245	rBV4	1092	746	0.05%	0.009%
70	11.519	3253	3259	3260	rBV6	1311	1299	0.08%	0.015%
71	11.574	3261	3276	3299	rVV2	680734	1594328	100.00%	18.184%
72	12.033	3416	3419	3424	rBV6	1165	1096	0.07%	0.013%
73	12.165	3457	3460	3462	rBV3	1208	741	0.05%	0.008%
74	12.233	3479	3481	3483	rBV2	1255	602	0.04%	0.007%
75	12.741	3636	3639	3640	rBV3	653	343	0.02%	0.004%
76	13.130	3758	3760	3762	rVB2	919	409	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
 Data File : VV033522.D
 Acq On : 20 Dec 2023 19:13
 Operator : SY/MD
 Sample : 05850-05DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0QM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	13.143	3762	3764	3766	rBV4	881	364	0.02%	0.004%
78	13.201	3772	3782	3798	rBV	68447	109544	6.87%	1.249%
79	13.426	3850	3852	3854	rBV3	958	422	0.03%	0.005%
80	13.493	3870	3873	3874	rBV3	770	433	0.03%	0.005%
81	13.577	3897	3899	3902	rBV3	1379	733	0.05%	0.008%
82	13.683	3924	3932	3943	rBV5	18418	27711	1.74%	0.316%
83	13.779	3960	3962	3964	rBV2	1470	936	0.06%	0.011%
84	13.876	3990	3992	3993	rBV2	806	351	0.02%	0.004%
85	13.940	4010	4012	4013	rBV2	938	329	0.02%	0.004%
86	13.969	4017	4021	4022	rBV2	1377	1026	0.06%	0.012%
87	14.033	4037	4041	4042	rBV4	953	604	0.04%	0.007%
88	14.082	4052	4056	4059	rBV5	1136	995	0.06%	0.011%
89	14.207	4089	4095	4097	rBV4	1410	1696	0.11%	0.019%
90	14.422	4160	4162	4164	rVB3	1103	353	0.02%	0.004%
91	14.590	4211	4214	4218	rBV3	1471	896	0.06%	0.010%
92	14.789	4274	4276	4277	rBV3	756	273	0.02%	0.003%
93	14.934	4318	4321	4323	rBV4	1197	847	0.05%	0.010%
94	14.972	4331	4333	4335	rBV2	1231	704	0.04%	0.008%




Sum of corrected areas: 8767599

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033522.D
Acq On : 20 Dec 2023 19:13
Operator : SY/MD
Sample : 05850-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

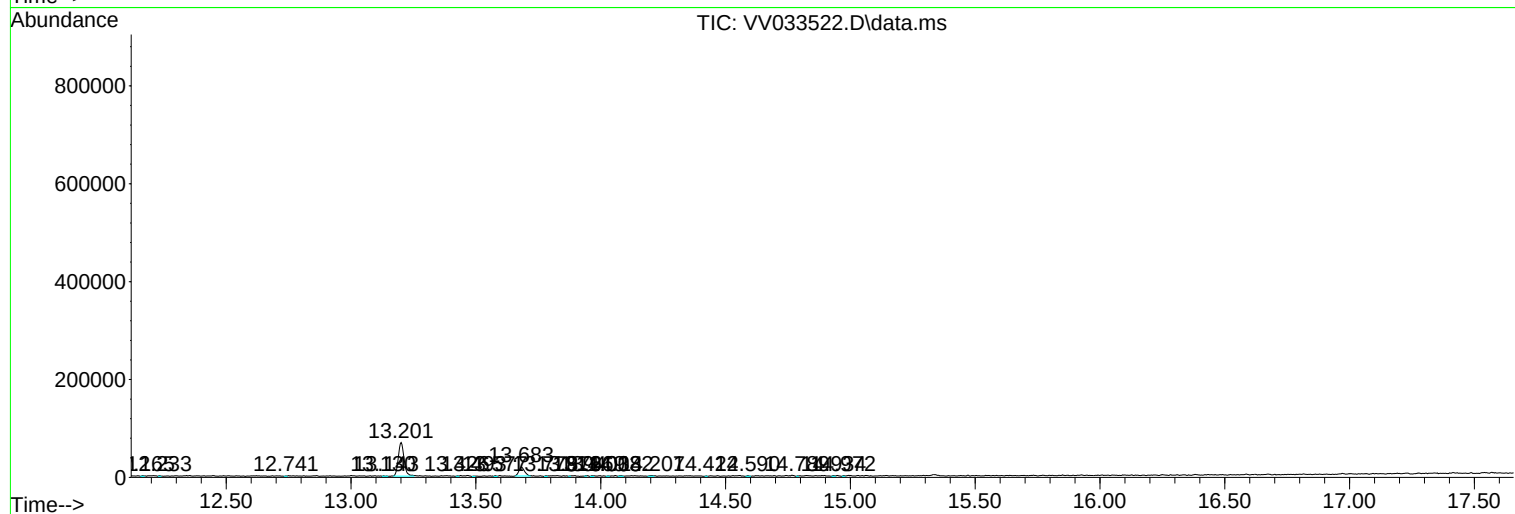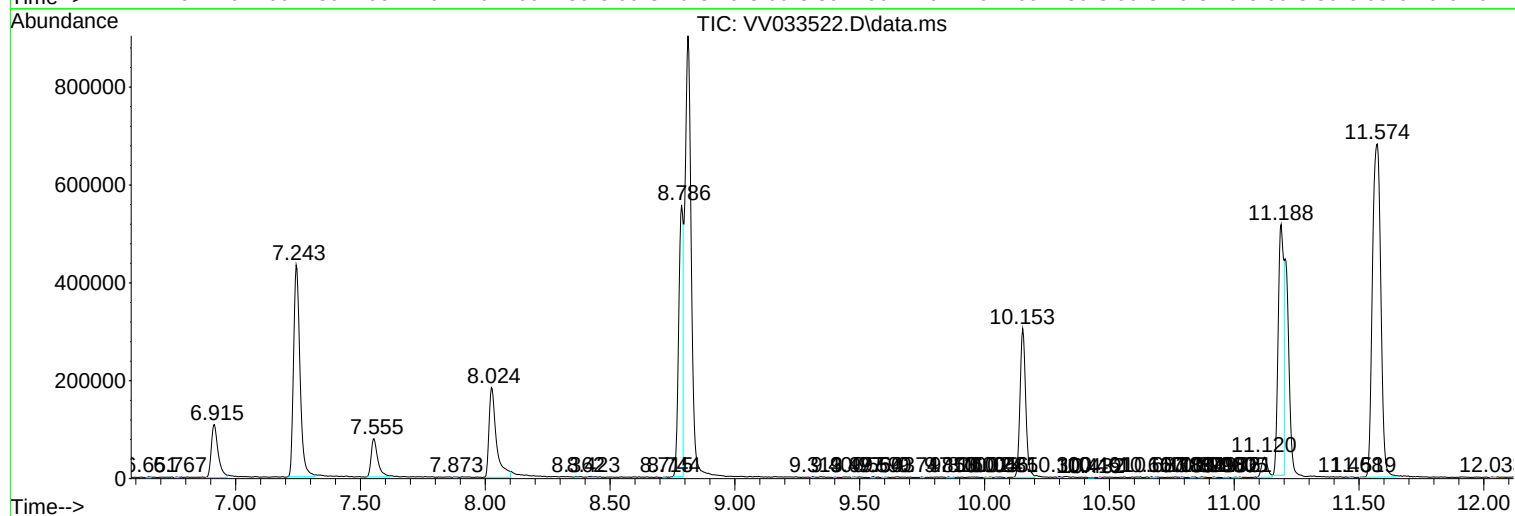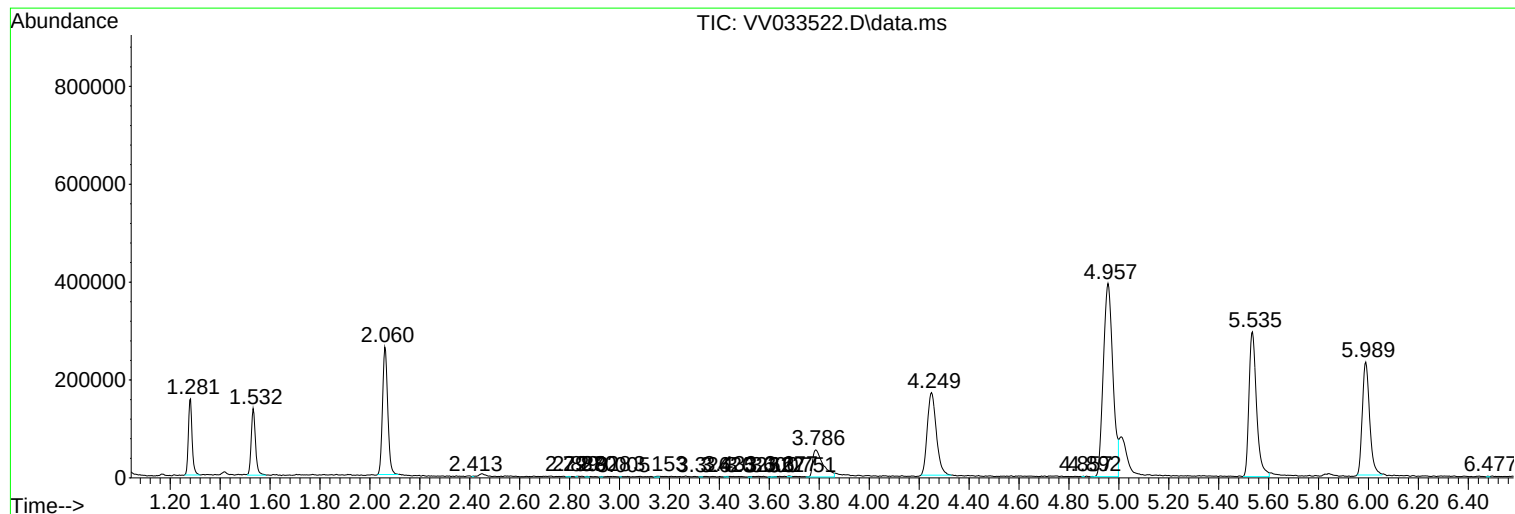

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033522.D
Acq On : 20 Dec 2023 19:13
Operator : SY/MD
Sample : 05850-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033522.D
Acq On : 20 Dec 2023 19:13
Operator : SY/MD
Sample : 05850-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0QM2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------