
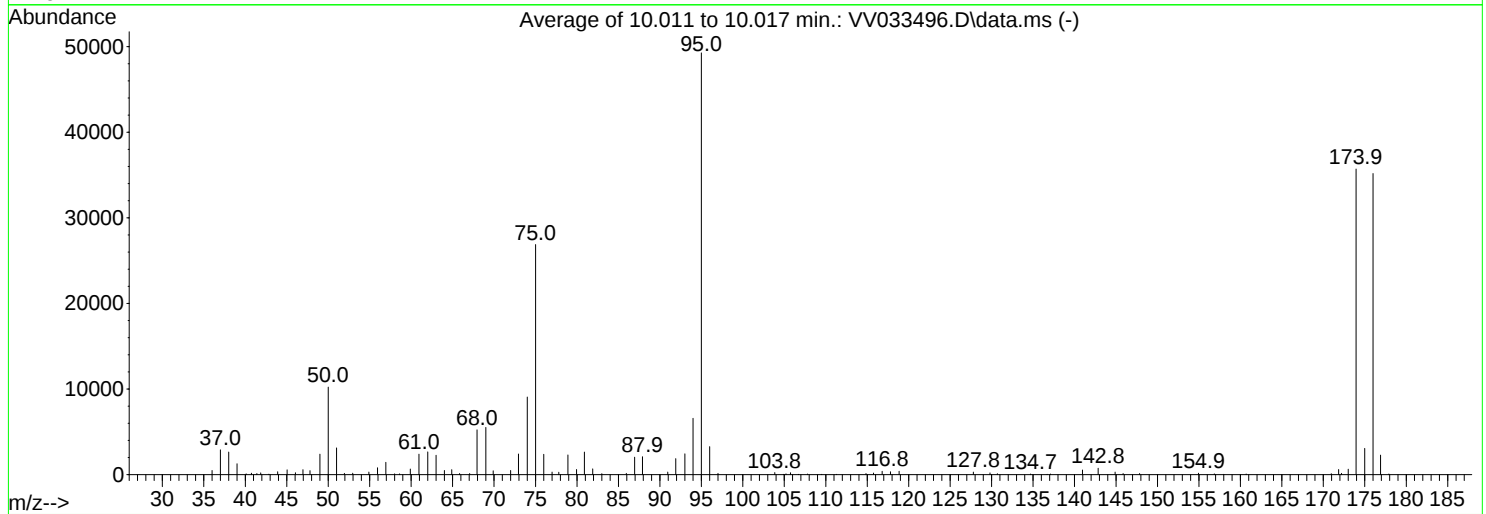


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122023\
Data File : VV033496.D
Acq On : 20 Dec 2023 08:29
Operator : SY/MD
Sample : BFB250
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB250

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis
Last Update : Thu Dec 21 01:43:54 2023

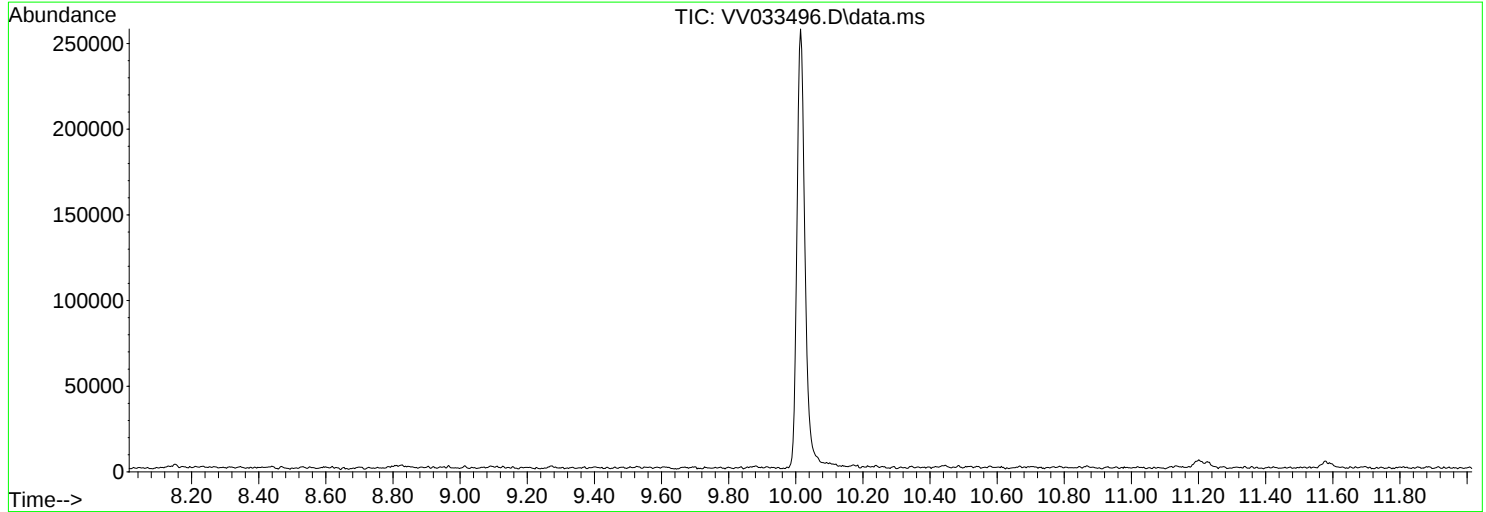

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10227	PASS
75	95	30	80	54.6	26885	PASS
95	95	100	100	100.0	49275	PASS
96	95	5	9	6.6	3275	PASS
173	174	0.00	2	1.8	631	PASS
174	95	50	120	72.5	35701	PASS
175	174	5	9	8.6	3066	PASS
176	174	95	105	98.5	35171	PASS
177	176	5	10	6.5	2287	PASS

m/z	Abundance
35.30	117.0
36.10	196.0
37.00	163.0
37.70	112.0
39.90	286.0
42.40	135.0
42.80	125.0
43.90	299.0
47.30	102.0
48.50	109.0
49.50	131.0
50.50	117.0
51.90	124.0
52.60	125.0
54.20	101.0
57.10	124.0
57.90	107.0
60.90	115.0
67.20	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	677.0
37.00	3012.0
38.00	2774.0
39.00	1373.0
39.80	335.0
40.70	122.0
41.40	183.0
41.80	174.0
43.00	143.0
43.90	676.0
45.10	572.0
46.00	236.0
46.90	642.0
47.80	484.0
49.00	2374.0
50.00	10102.0
51.00	3270.0
52.00	286.0
52.90	184.0
54.20	119.0
54.90	218.0
56.00	786.0
57.00	1505.0
58.10	194.0
59.90	681.0
61.00	2575.0
62.00	2540.0
63.00	2192.0
64.00	430.0
64.90	611.0
65.90	149.0
67.00	236.0
68.00	5145.0
69.00	5585.0
69.90	380.0
72.00	483.0
72.90	2237.0
74.00	8936.0
75.00	26264.0
76.00	2458.0
77.00	337.0
77.80	305.0
78.90	2256.0
79.90	581.0
80.90	2633.0
81.90	690.0
83.10	110.0
85.90	141.0
86.90	1988.0
87.90	2072.0
91.00	334.0
91.90	1986.0
93.00	2390.0
94.00	6517.0
95.00	48672.0
96.00	3400.0
97.00	128.0
103.80	237.0
104.90	112.0
105.70	238.0
109.50	101.0
114.80	122.0
115.80	192.0
116.80	385.0
117.80	299.0
118.80	398.0
127.80	262.0
129.80	195.0
130.70	110.0
137.10	133.0
141.00	551.0
142.80	743.0
144.90	315.0
145.90	106.0
147.80	131.0
154.90	176.0
171.80	519.0
172.20	426.0
173.00	542.0
173.90	34808.0
175.00	3093.0
176.00	33688.0
176.90	2256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	710.0
37.00	3155.0
38.00	2677.0
39.00	1291.0
39.80	320.0
40.80	150.0
41.40	192.0
41.80	224.0
43.00	190.0
43.90	663.0
45.10	594.0
46.10	222.0
46.90	596.0
47.80	484.0
49.00	2444.0
50.00	10554.0
51.00	3159.0
52.00	271.0
52.90	187.0
54.90	310.0
56.00	835.0
57.00	1594.0
58.10	206.0
58.60	141.0
59.90	668.0
61.00	2594.0
62.00	2746.0
63.00	2340.0
64.00	530.0
64.90	597.0
65.90	140.0
67.00	289.0
67.90	5388.0
69.00	5651.0
69.90	459.0
72.00	516.0
73.00	2514.0
74.00	9382.0
75.00	27704.0
76.00	2427.0
77.00	290.0
77.80	278.0
78.90	2379.0
80.00	611.0
80.90	2751.0
81.90	691.0
83.00	105.0
86.00	140.0
86.90	2153.0
87.90	2132.0
91.00	312.0
91.90	1952.0
93.00	2556.0
94.00	6803.0
95.00	50944.0
96.00	3402.0
97.00	166.0
103.80	231.0
105.20	135.0
105.70	230.0
107.80	104.0
114.90	147.0
115.80	200.0
116.80	416.0
117.80	356.0
118.90	402.0
127.80	312.0
129.80	199.0
130.70	119.0
134.70	102.0
137.10	112.0
141.00	544.0
142.80	789.0
144.90	315.0
145.80	126.0
147.90	147.0
155.00	191.0
156.90	142.0
158.00	101.0
160.70	107.0
171.00	137.0
171.80	640.0
173.00	633.0
174.00	36792.0
175.00	3175.0
176.00	36360.0
176.90	2335.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250

m/z	Abundance
36.00	680.0
37.00	3035.0
38.00	2457.0
39.00	1151.0
40.10	302.0
40.80	213.0
41.90	208.0
42.90	210.0
43.90	584.0
45.00	538.0
46.00	192.0
47.00	500.0
47.80	459.0
49.00	2370.0
50.00	10024.0
51.00	2914.0
52.00	258.0
53.00	145.0
54.90	352.0
55.90	799.0
56.90	1582.0
58.10	205.0
58.60	120.0
59.90	605.0
61.00	2337.0
62.00	2657.0
63.00	2268.0
64.00	516.0
64.90	513.0
65.80	131.0
67.00	268.0
67.90	5188.0
69.00	5314.0
69.90	513.0
72.00	463.0
73.00	2464.0
74.00	8866.0
75.00	26688.0
76.00	2262.0
77.00	286.0
77.80	280.0
78.90	2266.0
79.90	618.0
80.90	2511.0
81.90	638.0
82.90	114.0
86.00	160.0
87.00	1989.0
87.90	2072.0
90.90	257.0
91.90	1685.0
93.00	2363.0
94.00	6436.0
95.00	48208.0
96.00	3022.0
97.00	177.0
103.90	247.0
105.20	136.0
105.80	201.0
106.70	107.0
107.80	101.0
111.30	104.0
114.90	131.0
115.70	181.0
116.80	398.0
117.80	345.0
118.90	384.0
127.80	330.0
129.80	201.0
130.70	116.0
134.70	118.0
136.70	104.0
140.90	555.0
142.90	738.0
144.90	286.0
145.80	148.0
147.80	145.0
154.90	143.0
156.80	158.0
160.70	135.0
170.90	178.0
171.90	629.0
173.00	719.0
174.00	35504.0
175.00	2931.0
176.00	35464.0
176.90	2269.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB250