


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122121\
 Data File : VV024123.D
 Acq On : 21 Dec 2021 11:59
 Operator : SY/MD
 Sample : BFB208
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB208

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Dec 23 07:39:59 2021

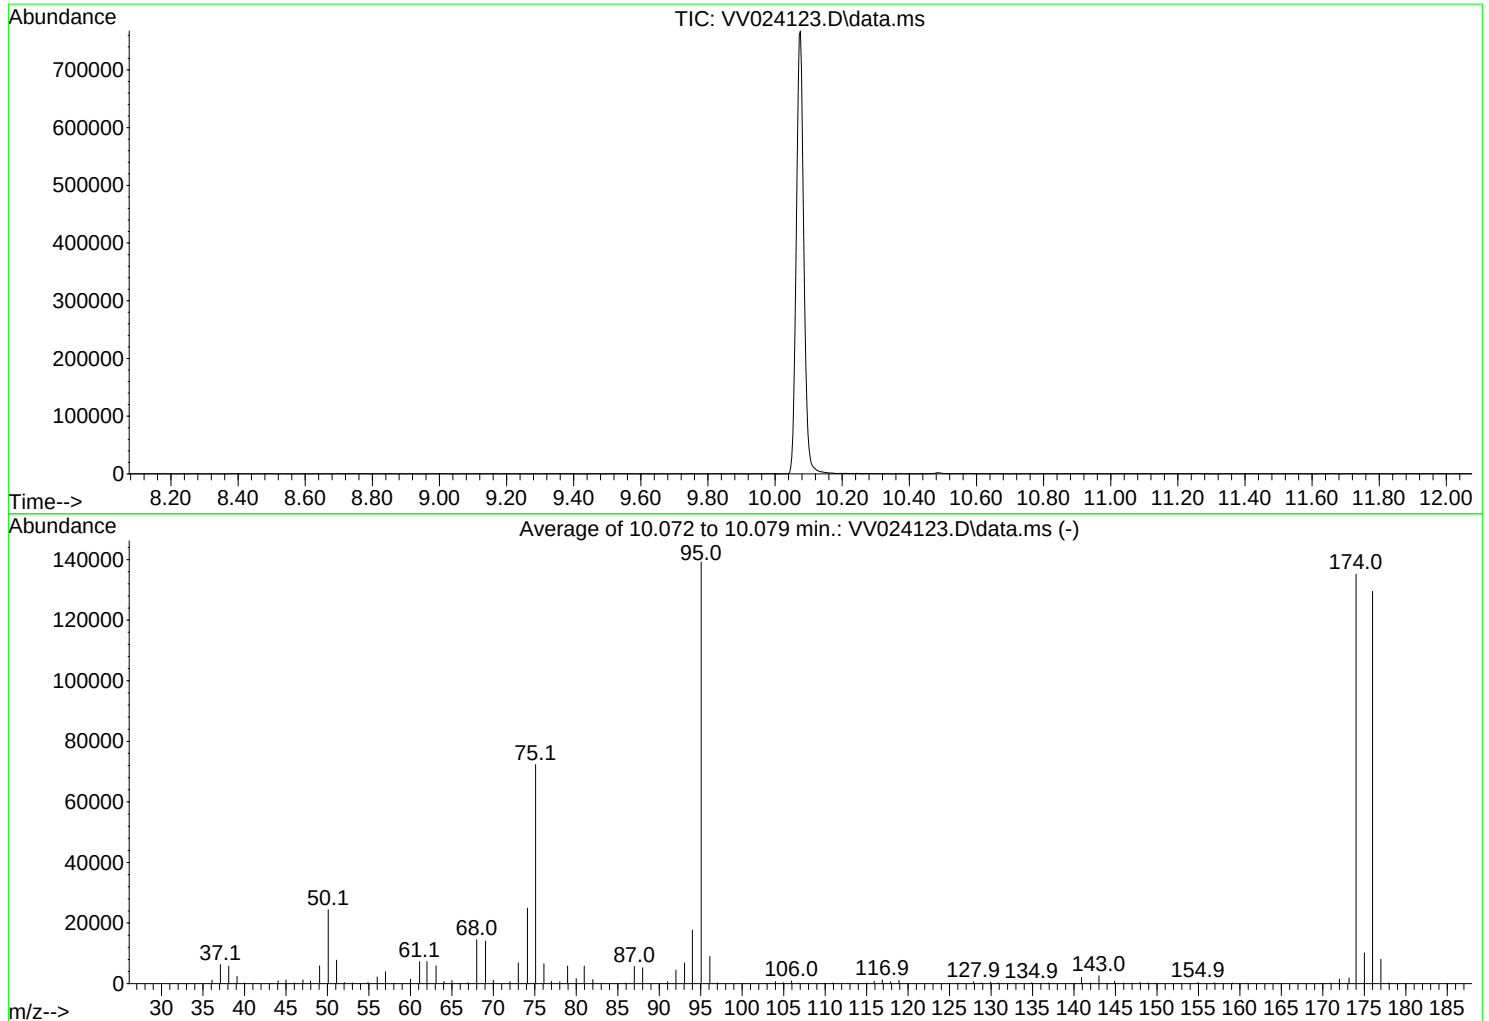

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	24395	PASS
75	95	30	80	51.9	72328	PASS
95	95	100	100	100.0	139256	PASS
96	95	5	9	6.5	9004	PASS
173	174	0.00	2	1.4	1929	PASS
174	95	50	120	97.1	135165	PASS
175	174	5	9	7.5	10153	PASS
176	174	95	101	95.8	129544	PASS
177	176	5	9	6.2	8008	PASS

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.10	1217.0
37.10	6567.0
38.10	6027.0
39.10	2489.0
40.00	205.0
43.10	101.0
44.10	1013.0
45.00	1310.0
46.00	233.0
47.00	1280.0
48.00	843.0
49.00	6170.0
50.10	25632.0
51.10	8058.0
52.10	401.0
53.00	228.0
54.90	510.0
56.00	2316.0
57.00	3966.0
58.10	150.0
60.00	1384.0
61.10	7213.0
62.00	7277.0
63.10	6266.0
64.00	847.0
65.00	1019.0
65.90	152.0
67.00	319.0
68.00	15141.0
69.00	14304.0
70.00	1151.0
71.90	678.0
73.00	7041.0
74.10	25712.0
75.10	74136.0
76.10	6850.0
77.00	724.0
78.00	571.0
79.00	6243.0
80.00	1694.0
80.90	6036.0
82.00	1341.0
83.10	206.0
85.90	249.0
87.00	5788.0
88.00	5578.0
91.00	673.0
92.00	4702.0
93.00	7225.0
94.00	18280.0
95.10	143360.0
96.10	9932.0
97.00	295.0
102.80	115.0
104.00	683.0
104.90	305.0
106.00	900.0
106.80	148.0
110.00	174.0
110.90	216.0
112.00	148.0
112.90	130.0
115.00	173.0
115.90	895.0
116.90	1360.0
117.90	607.0
118.90	1172.0
126.10	130.0
127.90	775.0
128.90	312.0
129.90	551.0
130.80	264.0
134.90	313.0
136.90	269.0
140.00	150.0
140.90	2047.0
142.10	295.0
143.00	2753.0
144.00	121.0
144.90	957.0
145.90	257.0
146.90	149.0
147.90	475.0
148.90	278.0
149.80	155.0
153.70	118.0
154.90	471.0
156.90	299.0
159.10	182.0
160.80	190.0
170.90	326.0
172.00	1456.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

173.10	1885.0
174.00	136832.0
175.00	10547.0
176.00	130768.0
177.00	8371.0
178.00	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.10	1189.0
37.10	6525.0
38.10	5988.0
39.10	2367.0
40.00	203.0
41.00	119.0
43.00	100.0
44.10	987.0
45.00	1236.0
46.00	263.0
47.10	1261.0
47.90	869.0
49.10	6052.0
50.10	25088.0
51.10	8014.0
52.10	367.0
53.00	227.0
54.90	459.0
56.00	2334.0
57.00	4091.0
58.00	177.0
60.00	1449.0
61.10	7495.0
62.00	7583.0
63.10	6114.0
64.10	736.0
65.00	1018.0
65.90	129.0
67.00	345.0
68.00	15098.0
69.10	14456.0
70.00	1133.0
72.00	652.0
73.00	7103.0
74.10	25808.0
75.10	74944.0
76.10	6826.0
77.00	782.0
78.00	591.0
79.00	6020.0
80.00	1697.0
80.90	6006.0
82.00	1359.0
83.00	196.0
85.90	239.0
87.00	5871.0
88.00	5397.0
91.00	655.0
92.00	4596.0
93.00	7162.0
94.00	18304.0
95.10	144256.0
96.10	9199.0
97.00	290.0
102.80	116.0
104.00	698.0
105.00	341.0
106.00	952.0
106.80	177.0
109.90	183.0
110.90	244.0
112.00	157.0
112.70	143.0
115.00	196.0
115.90	866.0
116.90	1272.0
117.90	676.0
118.90	1186.0
125.80	116.0
126.10	126.0
127.90	708.0
128.80	278.0
130.00	527.0
130.80	297.0
134.90	354.0
136.90	264.0
139.70	130.0
140.10	152.0
140.90	2084.0
142.00	272.0
143.00	2751.0
144.00	144.0
144.90	862.0
145.90	219.0
147.00	170.0
147.90	454.0
148.90	308.0
149.90	151.0
153.80	127.0
154.90	477.0
156.90	324.0
159.10	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

160.80	191.0
169.70	121.0
171.00	259.0
172.00	1603.0
173.10	1998.0
174.00	139904.0
175.00	10463.0
176.00	134208.0
177.00	8248.0
178.00	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.10	1099.0
37.10	5863.0
38.10	5283.0
39.10	2241.0
40.00	207.0
41.10	124.0
42.90	104.0
44.00	824.0
45.00	1067.0
46.00	247.0
47.10	1136.0
47.90	789.0
49.10	5440.0
50.10	22464.0
51.10	7179.0
52.00	289.0
53.00	182.0
54.90	380.0
56.00	2080.0
57.00	3749.0
58.00	165.0
60.00	1414.0
61.10	6981.0
62.00	6974.0
63.10	5285.0
64.00	631.0
65.00	937.0
65.90	113.0
66.90	352.0
68.00	13332.0
69.10	13404.0
70.00	1003.0
72.10	655.0
73.00	6532.0
74.10	23288.0
75.10	67904.0
76.10	6007.0
77.00	763.0
78.00	527.0
78.90	5240.0
80.00	1569.0
81.00	5396.0
82.00	1271.0
83.00	171.0
86.00	193.0
87.00	5381.0
88.00	4808.0
91.00	614.0
92.00	4160.0
93.10	6283.0
94.00	16488.0
95.00	130152.0
96.10	7880.0
97.00	249.0
104.00	675.0
105.00	293.0
105.90	835.0
106.80	189.0
109.90	165.0
110.90	216.0
112.00	153.0
112.70	142.0
115.00	210.0
115.90	692.0
116.90	1088.0
117.90	642.0
118.90	1067.0
125.80	120.0
127.90	565.0
128.70	248.0
129.90	440.0
130.90	304.0
134.90	358.0
137.00	266.0
140.20	138.0
140.90	1896.0
141.90	263.0
143.00	2330.0
144.00	154.0
144.90	653.0
146.00	203.0
147.00	163.0
148.00	423.0
148.90	232.0
149.90	145.0
152.80	112.0
153.90	144.0
155.00	389.0
156.30	102.0
156.90	292.0
159.10	206.0
160.80	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

169.70	133.0
172.00	1560.0
173.20	1905.0
174.00	128760.0
175.00	9449.0
176.00	123656.0
177.00	7404.0
177.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208