

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033526.D
 Acq On : 21 Dec 2023 11:56
 Operator : SY/MD
 Sample : VV1221WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	129574	136619	13.99%	1.833%
2	1.532	146	153	169	rVB	123970	147208	15.07%	1.975%
3	2.060	308	317	330	rBV	233181	336929	34.50%	4.519%
4	2.339	399	404	409	rBV6	1440	1963	0.20%	0.026%
5	2.362	409	411	414	rBV4	1051	684	0.07%	0.009%
6	2.526	457	462	465	rBV6	1223	989	0.10%	0.013%
7	2.571	474	476	480	rVB4	872	551	0.06%	0.007%
8	2.831	556	557	563	rVB5	1300	842	0.09%	0.011%
9	2.876	567	571	575	rBV6	1621	1483	0.15%	0.020%
10	3.002	607	610	612	rBV3	852	565	0.06%	0.008%
11	3.278	693	696	700	rBV8	810	764	0.08%	0.010%
12	3.327	708	711	715	rBV3	934	884	0.09%	0.012%
13	3.346	715	717	722	rVB5	1160	617	0.06%	0.008%
14	3.368	722	724	729	rBV6	988	896	0.09%	0.012%
15	3.394	729	732	733	rBV3	1122	540	0.06%	0.007%
16	3.539	774	777	781	rVB5	1110	943	0.10%	0.013%
17	3.587	787	792	793	rBV4	1234	831	0.09%	0.011%
18	3.642	807	809	812	rBV4	873	684	0.07%	0.009%
19	3.786	845	854	875	rBV	51837	146702	15.02%	1.968%
20	4.246	983	997	1020	rBV	158997	403339	41.30%	5.410%
21	4.523	1081	1083	1086	rBV3	1364	862	0.09%	0.012%
22	4.712	1139	1142	1146	rBV5	1713	1587	0.16%	0.021%
23	4.751	1151	1154	1155	rBV3	1028	551	0.06%	0.007%
24	4.793	1164	1167	1168	rBV2	1104	617	0.06%	0.008%
25	4.953	1200	1217	1248	rBV2	363715	976642	100.00%	13.100%
26	5.532	1385	1397	1422	rBV	286072	601941	61.63%	8.074%
27	5.986	1527	1538	1565	rBV	217125	450657	46.14%	6.045%
28	6.265	1622	1625	1627	rBV3	988	791	0.08%	0.011%
29	6.442	1675	1680	1681	rBV3	1148	717	0.07%	0.010%
30	6.481	1690	1692	1695	rVB3	1527	811	0.08%	0.011%
31	6.584	1721	1724	1726	rVB3	1080	550	0.06%	0.007%
32	6.805	1791	1793	1798	rBV6	1165	776	0.08%	0.010%
33	6.867	1809	1812	1816	rBV5	1008	938	0.10%	0.013%
34	6.912	1816	1826	1855	rVV	103481	200854	20.57%	2.694%
35	7.243	1918	1929	1956	rBV	393159	695618	71.23%	9.331%
36	7.551	2016	2025	2051	rBV	73905	136831	14.01%	1.835%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033526.D
 Acq On : 21 Dec 2023 11:56
 Operator : SY/MD
 Sample : VV1221WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	7.838	2109	2114	2116	rBV5	1627	1264	0.13%	0.017%
38	7.915	2135	2138	2139	rBV2	1581	840	0.09%	0.011%
39	7.957	2150	2151	2156	rVB5	1413	901	0.09%	0.012%
40	8.024	2163	2172	2204	rBV	176347	400077	40.96%	5.367%
41	8.635	2359	2362	2366	rBV4	1492	1237	0.13%	0.017%
42	8.719	2386	2388	2392	rBV5	1301	920	0.09%	0.012%
43	8.783	2397	2408	2434	rBV	484113	807487	82.68%	10.831%
44	9.092	2502	2504	2508	rBV4	1481	750	0.08%	0.010%
45	9.442	2611	2613	2617	rVB4	1028	686	0.07%	0.009%
46	9.471	2617	2622	2623	rBV5	1091	747	0.08%	0.010%
47	9.516	2634	2636	2638	rBV3	1200	622	0.06%	0.008%
48	9.625	2668	2670	2673	rBV4	983	543	0.06%	0.007%
49	9.709	2694	2696	2699	rVB4	1050	556	0.06%	0.007%
50	9.728	2700	2702	2705	rVB3	1481	646	0.07%	0.009%
51	9.818	2727	2730	2733	rBV4	1268	909	0.09%	0.012%
52	9.857	2737	2742	2745	rBV6	2556	2283	0.23%	0.031%
53	9.989	2780	2783	2787	rBV4	989	731	0.07%	0.010%
54	10.153	2823	2834	2849	rBV	285912	457950	46.89%	6.143%
55	10.272	2869	2871	2875	rVB4	1620	897	0.09%	0.012%
56	10.297	2876	2879	2881	rVV3	1745	964	0.10%	0.013%
57	10.452	2924	2927	2931	rVB4	1480	1023	0.10%	0.014%
58	10.471	2931	2933	2935	rBV3	1126	711	0.07%	0.010%
59	10.561	2958	2961	2963	rBV3	1118	820	0.08%	0.011%
60	10.609	2973	2976	2982	rBV7	990	728	0.07%	0.010%
61	10.641	2982	2986	2988	rBV5	1441	821	0.08%	0.011%
62	10.712	3005	3008	3013	rBV7	1303	1520	0.16%	0.020%
63	10.960	3078	3085	3088	rBV7	1064	879	0.09%	0.012%
64	10.995	3095	3096	3099	rBV3	829	566	0.06%	0.008%
65	11.069	3117	3119	3124	rVB6	1254	745	0.08%	0.010%
66	11.101	3124	3129	3130	rBV4	1201	895	0.09%	0.012%
67	11.185	3144	3155	3177	rBV	460076	702309	71.91%	9.421%
68	11.381	3213	3216	3222	rVB6	1759	1825	0.19%	0.024%
69	11.561	3258	3272	3293	rBV	432394	699961	71.67%	9.389%
70	11.905	3377	3379	3382	rVB3	1355	849	0.09%	0.011%
71	11.979	3397	3402	3405	rBV6	1005	1037	0.11%	0.014%
72	11.992	3405	3406	3411	rVV4	934	625	0.06%	0.008%
73	12.046	3420	3423	3426	rBV3	1053	822	0.08%	0.011%
74	12.162	3456	3459	3465	rBV5	1286	1159	0.12%	0.016%
75	12.268	3489	3492	3497	rVB7	1232	1185	0.12%	0.016%
76	12.323	3503	3509	3513	rBV8	1379	1578	0.16%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033526.D
 Acq On : 21 Dec 2023 11:56
 Operator : SY/MD
 Sample : VV1221WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK257

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.468	3553	3554	3559	rVB4	766	542	0.06%	0.007%
78	12.590	3585	3592	3605	rBV4	4696	8668	0.89%	0.116%
79	12.686	3619	3622	3625	rBV4	1516	1145	0.12%	0.015%
80	12.850	3671	3673	3676	rBV3	945	751	0.08%	0.010%
81	12.918	3690	3694	3699	rBV5	1261	1251	0.13%	0.017%
82	13.107	3751	3753	3757	rVB4	1334	704	0.07%	0.009%
83	13.207	3777	3784	3796	rVB9	8992	14936	1.53%	0.200%
84	13.255	3796	3799	3801	rBV3	1284	835	0.09%	0.011%
85	13.378	3833	3837	3838	rBV3	1334	879	0.09%	0.012%
86	13.442	3849	3857	3872	rVB	22892	39877	4.08%	0.535%
87	13.567	3891	3896	3901	rBV8	1629	1694	0.17%	0.023%
88	13.609	3906	3909	3914	rVV6	1310	1166	0.12%	0.016%
89	13.686	3926	3933	3941	rVB7	9824	14365	1.47%	0.193%
90	13.812	3970	3972	3974	rBV3	1071	588	0.06%	0.008%
91	13.860	3982	3987	3989	rBV3	962	778	0.08%	0.010%
92	13.895	3995	3998	4000	rBV4	1249	761	0.08%	0.010%
93	14.066	4048	4051	4054	rBV3	951	610	0.06%	0.008%
94	14.551	4196	4202	4206	rBV6	1312	1775	0.18%	0.024%
95	14.660	4233	4236	4242	rVB6	1470	1256	0.13%	0.017%
96	14.702	4245	4249	4250	rBV4	1501	998	0.10%	0.013%
97	15.037	4350	4353	4355	rBV3	1426	760	0.08%	0.010%
98	15.114	4374	4377	4379	rBV3	808	545	0.06%	0.007%
99	15.310	4436	4438	4440	rBV2	1173	719	0.07%	0.010%
100	15.866	4605	4611	4617	rBV10	2968	3574	0.37%	0.048%




Sum of corrected areas: 7455021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033526.D
Acq On : 21 Dec 2023 11:56
Operator : SY/MD
Sample : VV1221WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

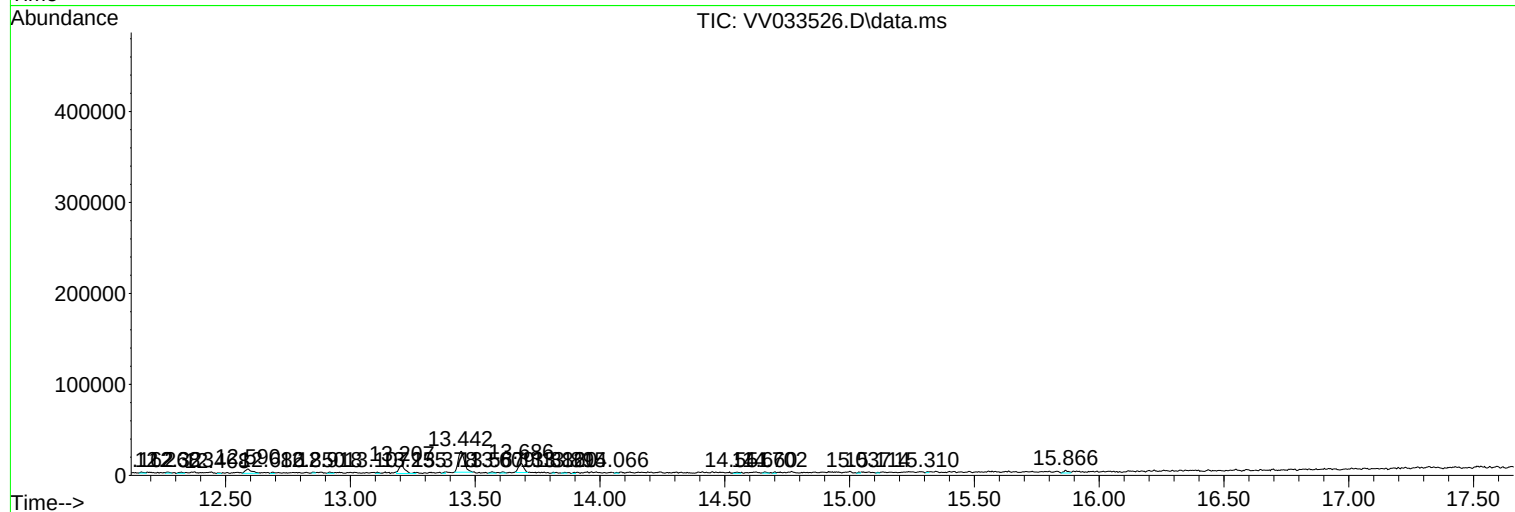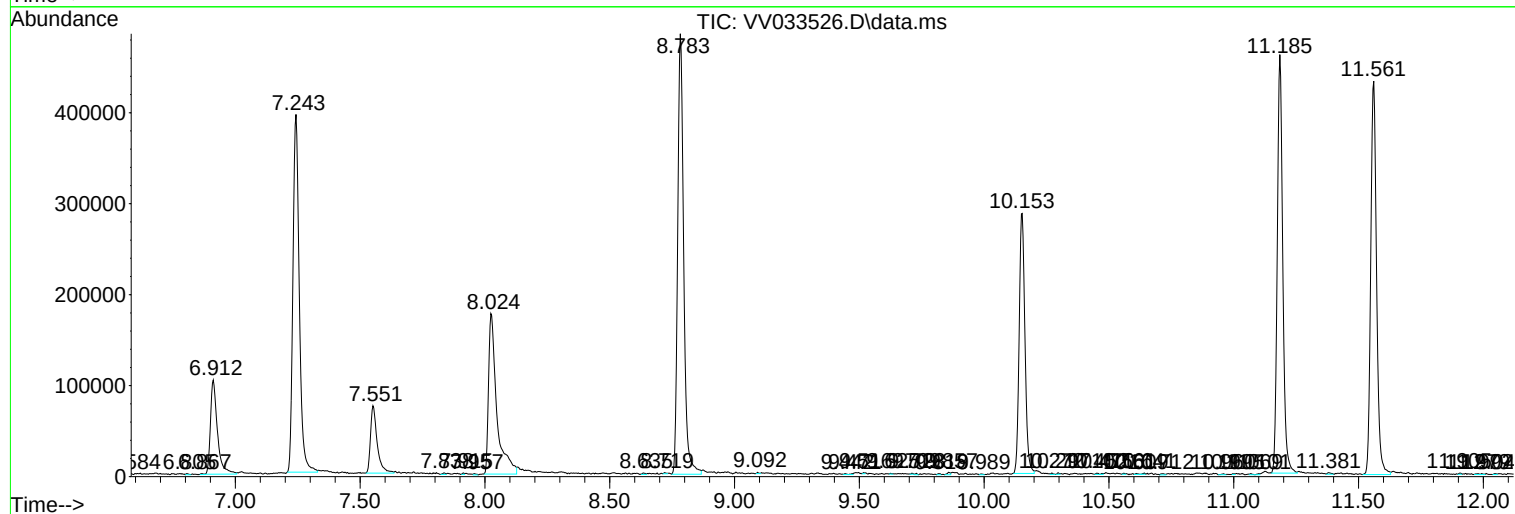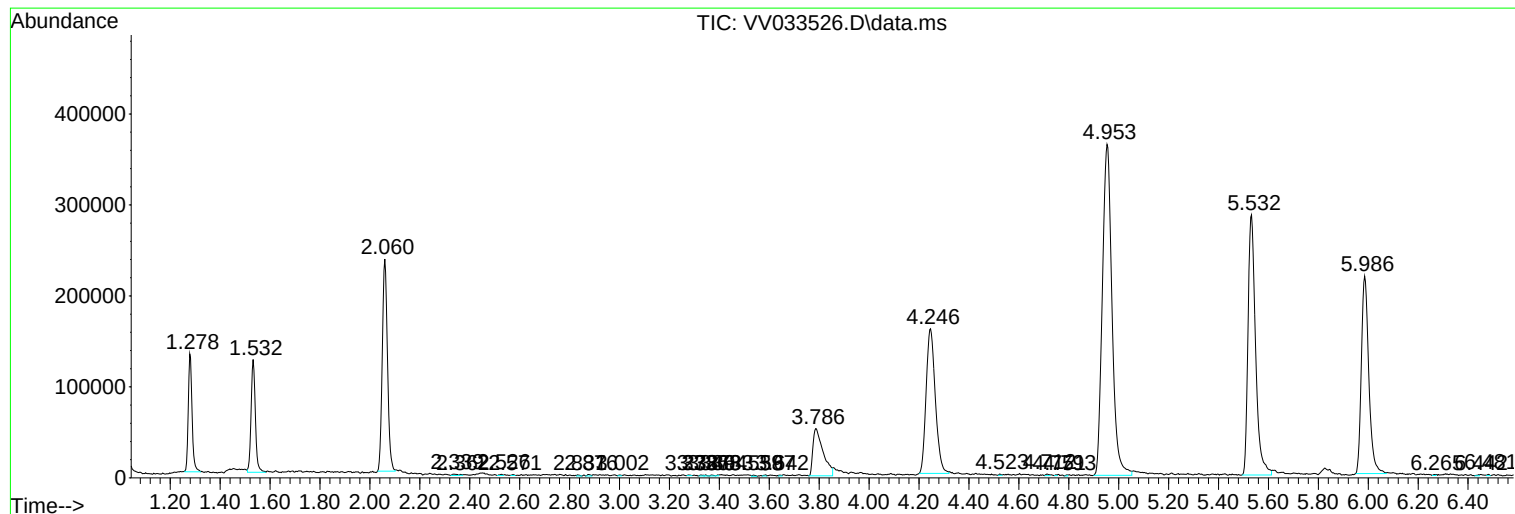

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033526.D
Acq On : 21 Dec 2023 11:56
Operator : SY/MD
Sample : VV1221WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033526.D
Acq On : 21 Dec 2023 11:56
Operator : SY/MD
Sample : VV1221WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK257

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc