

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033527.D
 Acq On : 21 Dec 2023 12:18
 Operator : SY/MD
 Sample : VV1221MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	127036	131978	13.90%	1.811%
2	1.532	147	153	166	rVB	119569	140628	14.81%	1.929%
3	2.060	309	317	336	rVB	220653	322271	33.95%	4.421%
4	2.381	415	417	420	rVB4	1567	633	0.07%	0.009%
5	2.812	549	551	553	rBV2	740	471	0.05%	0.006%
6	2.844	557	561	565	rBV7	1552	1362	0.14%	0.019%
7	2.925	584	586	589	rVB4	1103	484	0.05%	0.007%
8	2.944	589	592	594	rBV4	915	766	0.08%	0.011%
9	3.034	619	620	624	rBV3	998	583	0.06%	0.008%
10	3.076	629	633	635	rBV6	875	588	0.06%	0.008%
11	3.108	641	643	644	rBV2	915	219	0.02%	0.003%
12	3.117	644	646	648	rVB4	957	327	0.03%	0.004%
13	3.127	648	649	650	rBV	878	225	0.02%	0.003%
14	3.188	666	668	669	rBV2	855	347	0.04%	0.005%
15	3.224	676	679	684	rVB7	1275	1081	0.11%	0.015%
16	3.249	685	687	688	rBV2	709	163	0.02%	0.002%
17	3.298	700	702	707	rVB4	1263	944	0.10%	0.013%
18	3.529	772	774	776	rBV3	946	329	0.03%	0.005%
19	3.600	794	796	799	rBV4	573	343	0.04%	0.005%
20	3.616	799	801	803	rVV3	820	339	0.04%	0.005%
21	3.645	807	810	814	rBV5	769	611	0.06%	0.008%
22	3.789	847	855	880	rBV2	55619	157253	16.56%	2.157%
23	4.249	984	998	1023	rBV	156422	402812	42.43%	5.526%
24	4.670	1125	1129	1131	rBV4	1137	848	0.09%	0.012%
25	4.764	1156	1158	1161	rBV3	1198	747	0.08%	0.010%
26	4.809	1168	1172	1176	rBV7	938	1049	0.11%	0.014%
27	4.889	1196	1197	1200	rBV3	954	443	0.05%	0.006%
28	4.957	1203	1218	1245	rVV2	354622	949347	100.00%	13.024%
29	5.410	1357	1359	1360	rBV2	1355	631	0.07%	0.009%
30	5.535	1387	1398	1425	rBV	278384	587650	61.90%	8.062%
31	5.780	1472	1474	1477	rBV4	1582	1014	0.11%	0.014%
32	5.989	1528	1539	1560	rBV	216340	444663	46.84%	6.100%
33	6.580	1721	1723	1725	rBV3	1704	931	0.10%	0.013%
34	6.728	1765	1769	1774	rBV7	1624	1864	0.20%	0.026%
35	6.793	1788	1789	1794	rBV5	1160	698	0.07%	0.010%
36	6.831	1798	1801	1803	rVB3	920	529	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033527.D
 Acq On : 21 Dec 2023 12:18
 Operator : SY/MD
 Sample : VV1221MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.915	1817	1827	1847	rBV2	99709	193778	20.41%	2.658%
38	7.243	1919	1929	1957	rBV	382106	691064	72.79%	9.481%
39	7.555	2018	2026	2046	rBV	73450	129219	13.61%	1.773%
40	7.821	2108	2109	2112	rBV3	1404	614	0.06%	0.008%
41	7.902	2131	2134	2136	rBV3	570	352	0.04%	0.005%
42	7.915	2136	2138	2141	rBV3	1345	867	0.09%	0.012%
43	8.027	2164	2173	2206	rBV	185093	402100	42.36%	5.516%
44	8.519	2323	2326	2327	rBV2	928	562	0.06%	0.008%
45	8.632	2359	2361	2364	rBV4	702	463	0.05%	0.006%
46	8.786	2398	2409	2437	rBV	473773	793095	83.54%	10.881%
47	9.307	2568	2571	2572	rBV2	1081	584	0.06%	0.008%
48	9.529	2638	2640	2642	rBV2	713	212	0.02%	0.003%
49	9.603	2660	2663	2668	rBV6	1316	1185	0.12%	0.016%
50	9.686	2688	2689	2690	rBV	846	254	0.03%	0.003%
51	9.712	2694	2697	2699	rBV5	999	728	0.08%	0.010%
52	9.921	2757	2762	2767	rBV7	1517	1616	0.17%	0.022%
53	9.976	2777	2779	2780	rBV	548	286	0.03%	0.004%
54	10.153	2821	2834	2853	rBV	295765	475265	50.06%	6.520%
55	10.333	2883	2890	2893	rBV8	1587	1796	0.19%	0.025%
56	10.442	2920	2924	2929	rBV5	1599	1571	0.17%	0.022%
57	10.599	2971	2973	2975	rBV3	721	304	0.03%	0.004%
58	10.609	2975	2976	2979	rBV2	633	306	0.03%	0.004%
59	10.625	2979	2981	2982	rBV2	827	452	0.05%	0.006%
60	10.953	3082	3083	3087	rBV4	970	768	0.08%	0.011%
61	11.027	3104	3106	3112	rVB6	1800	1475	0.16%	0.020%
62	11.053	3112	3114	3116	rBV	1331	824	0.09%	0.011%
63	11.185	3144	3155	3174	rBV	438997	697571	73.48%	9.570%
64	11.452	3236	3238	3241	rVB4	1487	856	0.09%	0.012%
65	11.468	3241	3243	3244	rBV2	1360	509	0.05%	0.007%
66	11.561	3261	3272	3293	rBV	426690	681959	71.83%	9.356%
67	11.825	3352	3354	3357	rBV3	1044	495	0.05%	0.007%
68	11.866	3363	3367	3368	rBV4	1042	796	0.08%	0.011%
69	12.079	3429	3433	3439	rBV7	2094	2079	0.22%	0.029%
70	12.111	3439	3443	3447	rVV5	1876	1431	0.15%	0.020%
71	12.197	3465	3470	3471	rBV3	1298	844	0.09%	0.012%
72	12.239	3482	3483	3486	rBV3	472	284	0.03%	0.004%
73	12.255	3486	3488	3489	rBV	904	222	0.02%	0.003%
74	12.291	3498	3499	3500	rBV	638	190	0.02%	0.003%
75	12.455	3548	3550	3553	rBV4	1065	637	0.07%	0.009%
76	12.487	3559	3560	3561	rBV	831	288	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033527.D
 Acq On : 21 Dec 2023 12:18
 Operator : SY/MD
 Sample : VV1221MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.558	3580	3582	3586	rVB5	1459	799	0.08%	0.011%
78	12.580	3586	3589	3590	rBV3	1427	791	0.08%	0.011%
79	12.699	3621	3626	3632	rBV9	1740	2555	0.27%	0.035%
80	12.805	3658	3659	3660	rBV	590	160	0.02%	0.002%
81	12.834	3664	3668	3669	rBV3	1653	959	0.10%	0.013%
82	12.882	3681	3683	3685	rBV3	936	370	0.04%	0.005%
83	13.197	3778	3781	3787	rBV7	3558	4573	0.48%	0.063%
84	13.255	3797	3799	3801	rVB2	1368	623	0.07%	0.009%
85	13.275	3801	3805	3806	rBV3	750	420	0.04%	0.006%
86	13.329	3817	3822	3823	rBV4	1009	823	0.09%	0.011%
87	13.355	3828	3830	3833	rBV3	1009	554	0.06%	0.008%
88	13.448	3848	3859	3872	rBV	7940	17874	1.88%	0.245%
89	13.570	3895	3897	3898	rBV2	1193	539	0.06%	0.007%
90	13.638	3916	3918	3920	rBV4	896	336	0.04%	0.005%
91	13.686	3926	3933	3937	rBV7	4045	5305	0.56%	0.073%
92	13.799	3963	3968	3975	rBV8	1825	2055	0.22%	0.028%
93	13.927	4000	4008	4009	rBV5	1209	1654	0.17%	0.023%
94	14.242	4103	4106	4108	rBV2	1246	811	0.09%	0.011%
95	14.320	4127	4130	4131	rBV2	832	494	0.05%	0.007%
96	14.574	4202	4209	4211	rBV6	1636	1619	0.17%	0.022%
97	14.599	4215	4217	4219	rBV3	1205	569	0.06%	0.008%
98	14.725	4254	4256	4260	rBV4	1881	1105	0.12%	0.015%
99	14.847	4292	4294	4295	rBV2	1278	520	0.05%	0.007%
100	15.104	4371	4374	4375	rBV4	1145	536	0.06%	0.007%




Sum of corrected areas: 7289116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033527.D
Acq On : 21 Dec 2023 12:18
Operator : SY/MD
Sample : VV1221MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

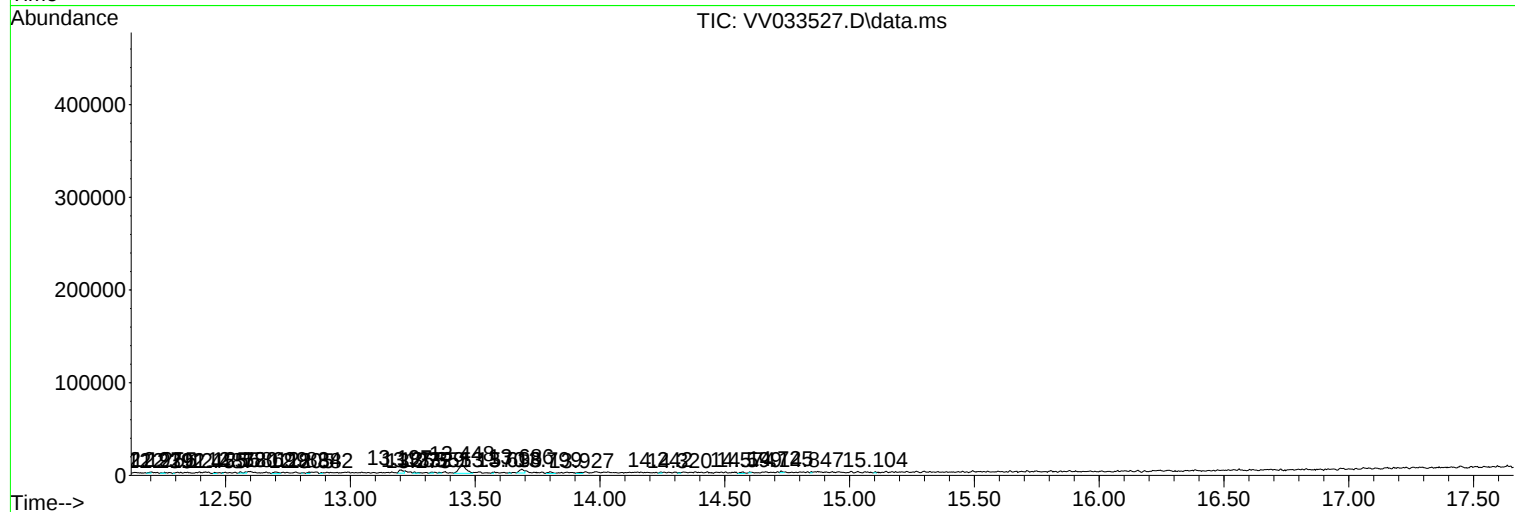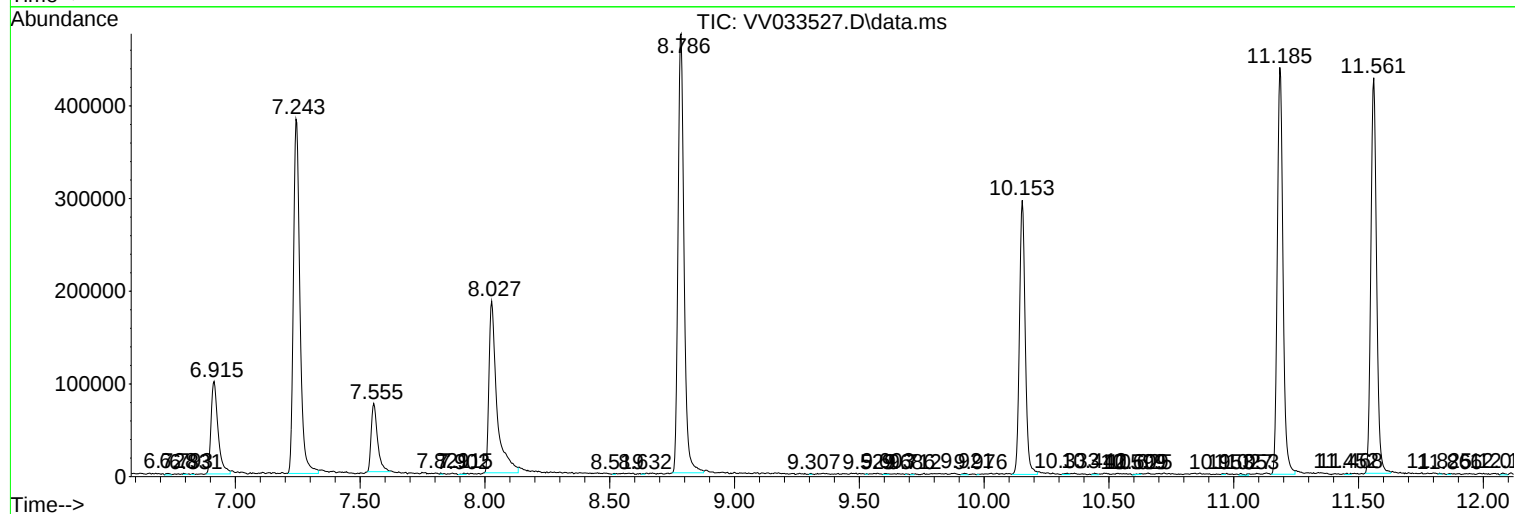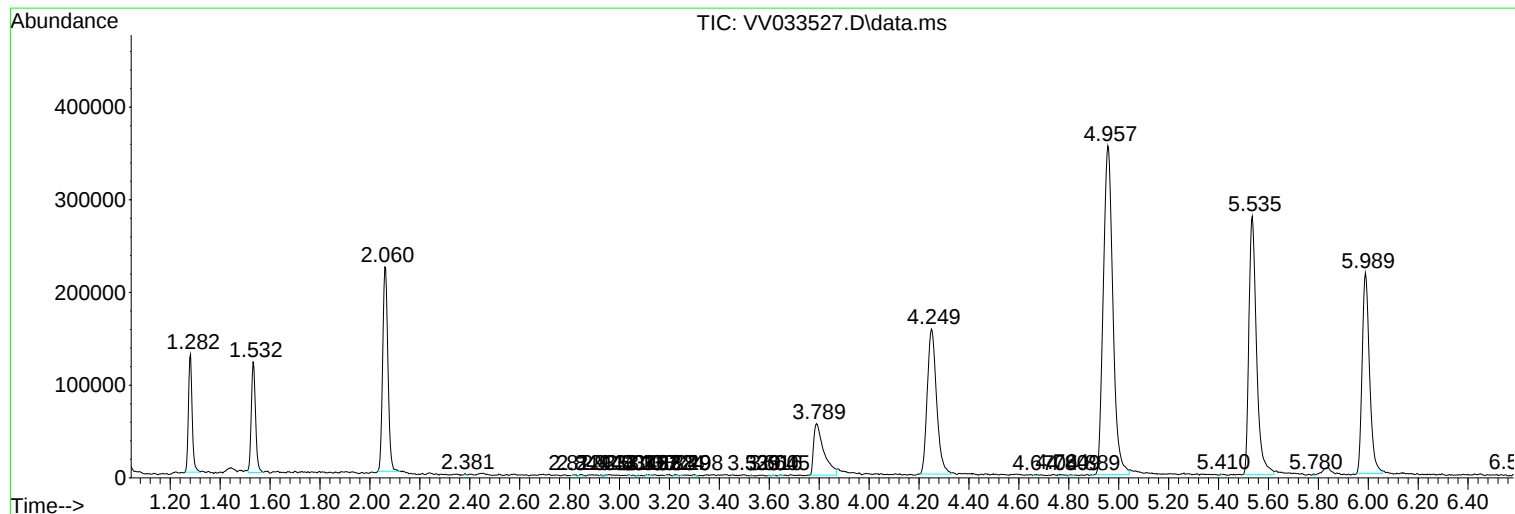

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033527.D
Acq On : 21 Dec 2023 12:18
Operator : SY/MD
Sample : VV1221MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033527.D
Acq On : 21 Dec 2023 12:18
Operator : SY/MD
Sample : VV1221MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
