

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033528.D
 Acq On : 21 Dec 2023 12:42
 Operator : SY/MD
 Sample : 05847-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M

Title : VOC Analysis

Signal : TIC: VV033528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	117286	125388	13.52%	1.783%
2	1.532	147	153	165	rVB	116035	134799	14.54%	1.917%
3	2.059	309	317	331	rBV	207743	301519	32.51%	4.287%
4	2.442	430	436	437	rBV5	2999	2212	0.24%	0.031%
5	2.523	457	461	464	rBV4	1381	1300	0.14%	0.018%
6	2.638	494	497	498	rBV3	1484	862	0.09%	0.012%
7	2.735	525	527	528	rBV2	1447	653	0.07%	0.009%
8	2.802	546	548	552	rVB3	809	680	0.07%	0.010%
9	2.828	552	556	560	rBV5	1296	1188	0.13%	0.017%
10	3.027	616	618	623	rBV6	1082	708	0.08%	0.010%
11	3.098	637	640	641	rBV3	1500	711	0.08%	0.010%
12	3.146	652	655	660	rBV6	1339	944	0.10%	0.013%
13	3.240	680	684	687	rBV6	1157	907	0.10%	0.013%
14	3.272	691	694	696	rBV3	1095	598	0.06%	0.009%
15	3.326	708	711	716	rVB7	860	825	0.09%	0.012%
16	3.381	726	728	734	rVB5	1710	1280	0.14%	0.018%
17	3.445	744	748	750	rBV4	1570	1057	0.11%	0.015%
18	3.481	755	759	761	rBV4	1169	1002	0.11%	0.014%
19	3.567	783	786	790	rBV5	845	584	0.06%	0.008%
20	3.658	808	814	816	rBV5	937	716	0.08%	0.010%
21	3.789	846	855	882	rBV	59659	169837	18.31%	2.415%
22	4.249	984	998	1022	rBV	152185	386093	41.63%	5.489%
23	4.542	1086	1089	1092	rBV5	1113	795	0.09%	0.011%
24	4.815	1172	1174	1176	rBV3	894	556	0.06%	0.008%
25	4.866	1188	1190	1194	rBV5	1367	665	0.07%	0.009%
26	4.957	1203	1218	1247	rBV2	340717	927396	100.00%	13.185%
27	5.355	1339	1342	1344	rBV4	1600	1072	0.12%	0.015%
28	5.407	1356	1358	1362	rBV5	1360	789	0.09%	0.011%
29	5.535	1387	1398	1426	rVV	264705	565082	60.93%	8.034%
30	5.989	1528	1539	1558	rBV	206392	428069	46.16%	6.086%
31	6.217	1609	1610	1614	rBV4	1120	691	0.07%	0.010%
32	6.310	1637	1639	1641	rVB2	1692	606	0.07%	0.009%
33	6.381	1658	1661	1663	rBV4	1529	816	0.09%	0.012%
34	6.558	1712	1716	1718	rBV4	862	790	0.09%	0.011%
35	6.619	1732	1735	1739	rBV4	1390	1121	0.12%	0.016%
36	6.680	1752	1754	1756	rBV3	1304	815	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033528.D
 Acq On : 21 Dec 2023 12:42
 Operator : SY/MD
 Sample : 05847-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.722	1763	1767	1778	rBV8	1770	2472	0.27%	0.035%
38	6.834	1799	1802	1805	rBV5	1503	1064	0.11%	0.015%
39	6.915	1817	1827	1848	rBV	95965	183167	19.75%	2.604%
40	7.136	1894	1896	1899	rBV3	1570	1048	0.11%	0.015%
41	7.246	1919	1930	1950	rBV	364549	654914	70.62%	9.311%
42	7.554	2017	2026	2046	rBV	71071	130518	14.07%	1.856%
43	7.767	2088	2092	2095	rBV4	1351	1172	0.13%	0.017%
44	7.924	2137	2141	2144	rVB4	1437	1131	0.12%	0.016%
45	7.966	2152	2154	2157	rVB4	1160	625	0.07%	0.009%
46	8.027	2163	2173	2209	rBV	184225	415959	44.85%	5.914%
47	8.419	2293	2295	2299	rBV4	1342	1008	0.11%	0.014%
48	8.484	2311	2315	2321	rBV7	2005	2133	0.23%	0.030%
49	8.628	2358	2360	2363	rBV4	1045	553	0.06%	0.008%
50	8.709	2382	2385	2386	rBV2	1307	738	0.08%	0.010%
51	8.786	2397	2409	2426	rBV	456251	754300	81.34%	10.724%
52	8.960	2461	2463	2471	rVB8	2274	2179	0.23%	0.031%
53	9.127	2512	2515	2519	rBV5	1391	953	0.10%	0.014%
54	9.230	2543	2547	2549	rBV4	1098	880	0.09%	0.013%
55	9.323	2573	2576	2577	rBV3	1163	636	0.07%	0.009%
56	9.381	2591	2594	2596	rBV4	1182	591	0.06%	0.008%
57	9.497	2627	2630	2632	rBV4	978	647	0.07%	0.009%
58	9.609	2662	2665	2668	rBV4	1049	841	0.09%	0.012%
59	9.628	2668	2671	2675	rVB4	1308	911	0.10%	0.013%
60	9.770	2712	2715	2718	rBV4	1079	746	0.08%	0.011%
61	9.869	2742	2746	2749	rBV6	1639	1649	0.18%	0.023%
62	9.915	2758	2760	2764	rBV4	918	616	0.07%	0.009%
63	10.021	2787	2793	2795	rBV5	1115	1163	0.13%	0.017%
64	10.046	2798	2801	2807	rVB5	1434	1314	0.14%	0.019%
65	10.075	2807	2810	2811	rBV2	1157	583	0.06%	0.008%
66	10.152	2823	2834	2854	rBV	294084	470994	50.79%	6.696%
67	10.390	2904	2908	2910	rBV4	1185	957	0.10%	0.014%
68	10.545	2953	2956	2959	rVB5	1402	719	0.08%	0.010%
69	10.580	2964	2967	2969	rBV4	1062	677	0.07%	0.010%
70	10.677	2995	2997	3000	rBV4	1628	1040	0.11%	0.015%
71	10.876	3055	3059	3060	rBV4	996	689	0.07%	0.010%
72	10.918	3070	3072	3074	rBV3	1116	678	0.07%	0.010%
73	10.947	3079	3081	3086	rVB5	1192	836	0.09%	0.012%
74	11.030	3101	3107	3111	rBV7	1697	2073	0.22%	0.029%
75	11.185	3144	3155	3173	rBV	419791	654169	70.54%	9.301%
76	11.561	3259	3272	3287	rBV	409184	653329	70.45%	9.289%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033528.D
 Acq On : 21 Dec 2023 12:42
 Operator : SY/MD
 Sample : 05847-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.905	3377	3379	3381	rBV3	1440	630	0.07%	0.009%
78	11.924	3381	3385	3389	rVV4	969	955	0.10%	0.014%
79	12.075	3428	3432	3434	rBV3	720	568	0.06%	0.008%
80	12.117	3443	3445	3448	rBV4	887	596	0.06%	0.008%
81	12.178	3461	3464	3466	rBV3	1340	849	0.09%	0.012%
82	12.413	3535	3537	3542	rVB5	1094	713	0.08%	0.010%
83	12.435	3542	3544	3547	rBV3	919	626	0.07%	0.009%
84	12.506	3565	3566	3571	rVB4	1063	657	0.07%	0.009%
85	12.564	3581	3584	3585	rBV2	1752	936	0.10%	0.013%
86	12.959	3703	3707	3710	rBV4	1535	1149	0.12%	0.016%
87	13.355	3827	3830	3833	rVB4	1011	607	0.07%	0.009%
88	13.680	3927	3931	3934	rBV3	1649	1455	0.16%	0.021%
89	13.850	3980	3984	3988	rBV6	1151	1139	0.12%	0.016%
90	14.011	4031	4034	4037	rBV6	862	623	0.07%	0.009%
91	14.213	4094	4097	4099	rBV4	1295	679	0.07%	0.010%
92	14.393	4150	4153	4156	rBV5	1521	956	0.10%	0.014%
93	14.564	4202	4206	4207	rBV3	1578	1034	0.11%	0.015%
94	14.657	4230	4235	4240	rBV6	1425	1737	0.19%	0.025%
95	14.737	4258	4260	4262	rBV3	1002	575	0.06%	0.008%
96	14.815	4282	4284	4289	rBV5	1116	547	0.06%	0.008%
97	14.918	4314	4316	4320	rVB5	1079	580	0.06%	0.008%
98	14.959	4327	4329	4333	rBV4	1133	994	0.11%	0.014%
99	15.065	4360	4362	4364	rBV2	1352	617	0.07%	0.009%
100	15.297	4432	4434	4436	rBV3	1231	561	0.06%	0.008%




Sum of corrected areas: 7033581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033528.D
Acq On : 21 Dec 2023 12:42
Operator : SY/MD
Sample : 05847-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

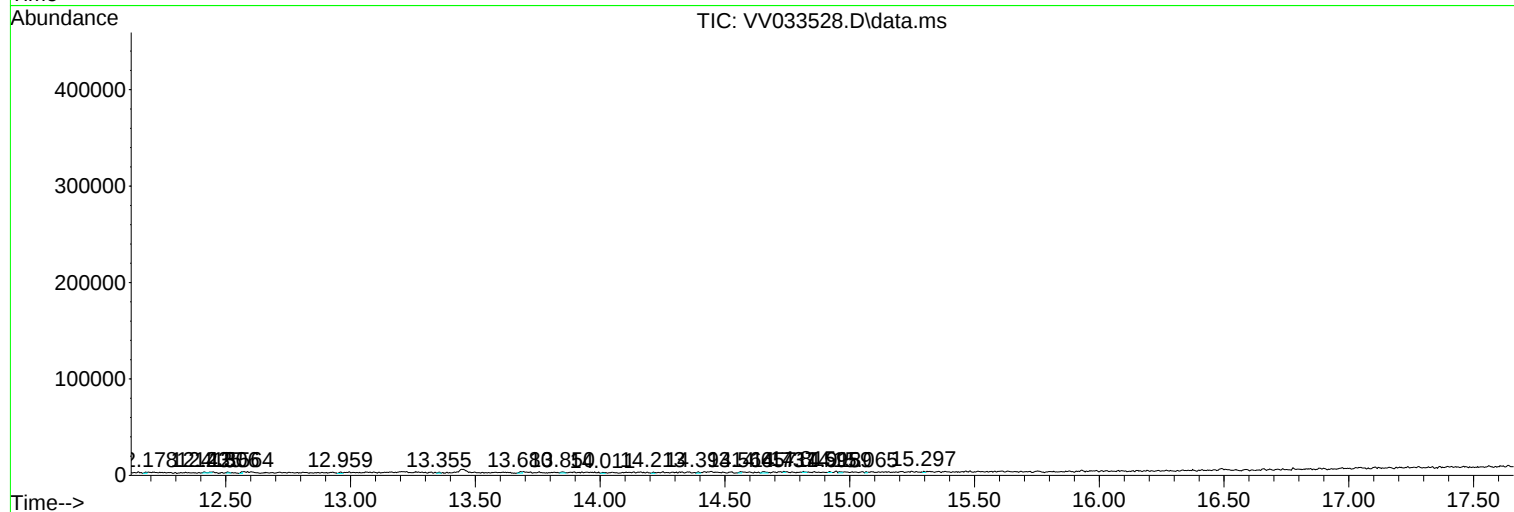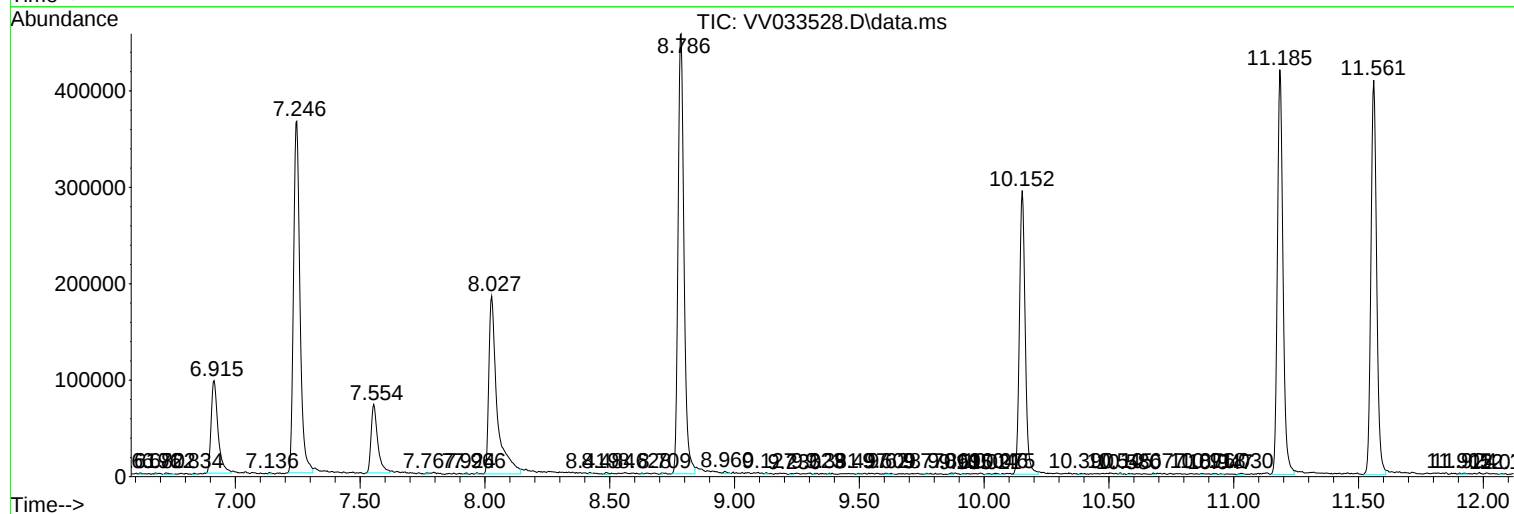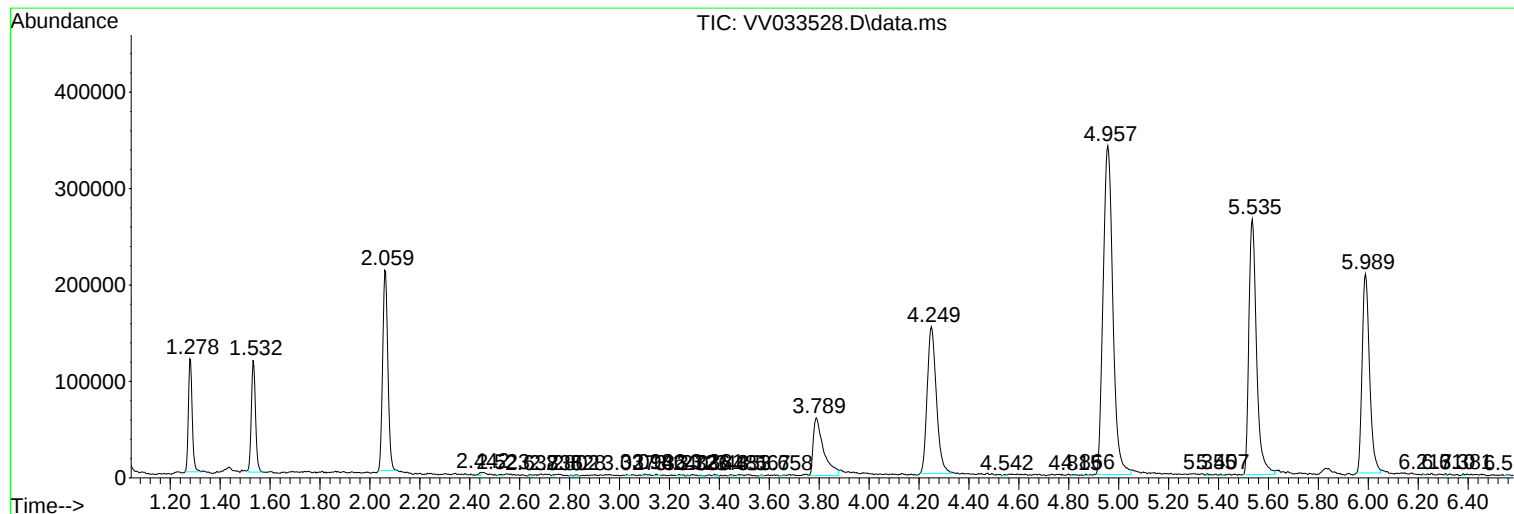

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033528.D
Acq On : 21 Dec 2023 12:42
Operator : SY/MD
Sample : 05847-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033528.D
Acq On : 21 Dec 2023 12:42
Operator : SY/MD
Sample : 05847-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------