

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122123\
 Data File : VW033533.D
 Acq On : 21 Dec 2023 14:37
 Operator : SY/MD
 Sample : 05850-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	129354	139964	13.71%	1.840%
2	1.532	146	153	167	rVB	121554	146943	14.39%	1.932%
3	2.060	308	317	333	rVB	230263	332602	32.58%	4.373%
4	2.510	453	457	459	rBV5	1325	1029	0.10%	0.014%
5	2.693	511	514	517	rBV5	1212	850	0.08%	0.011%
6	2.809	547	550	551	rBV2	777	473	0.05%	0.006%
7	3.031	616	619	622	rBV5	876	799	0.08%	0.011%
8	3.111	638	644	647	rBV6	995	1204	0.12%	0.016%
9	3.166	657	661	663	rBV5	1286	798	0.08%	0.010%
10	3.217	675	677	680	rVB4	1166	601	0.06%	0.008%
11	3.233	680	682	685	rBV4	909	732	0.07%	0.010%
12	3.288	690	699	700	rBV7	1471	1652	0.16%	0.022%
13	3.330	709	712	715	rBV5	977	672	0.07%	0.009%
14	3.346	715	717	720	rVV3	1333	847	0.08%	0.011%
15	3.391	724	731	734	rBV6	1341	1487	0.15%	0.020%
16	3.436	740	745	747	rBV4	1201	861	0.08%	0.011%
17	3.642	805	809	811	rBV4	921	673	0.07%	0.009%
18	3.677	818	820	824	rVB4	1478	1018	0.10%	0.013%
19	3.696	824	826	828	rBV2	1011	617	0.06%	0.008%
20	3.786	844	854	884	rBV2	60951	180125	17.64%	2.368%
21	4.249	985	998	1024	rVB	164465	414601	40.61%	5.451%
22	4.523	1080	1083	1087	rBV4	1020	1010	0.10%	0.013%
23	4.577	1097	1100	1104	rVB5	1663	1243	0.12%	0.016%
24	4.687	1131	1134	1136	rBV4	1066	593	0.06%	0.008%
25	4.806	1169	1171	1174	rBV4	1663	1149	0.11%	0.015%
26	4.870	1187	1191	1196	rVB7	1868	1963	0.19%	0.026%
27	4.957	1196	1218	1246	rBV2	375447	1020854	100.00%	13.422%
28	5.461	1373	1375	1376	rBV2	1392	641	0.06%	0.008%
29	5.535	1386	1398	1429	rBV	287007	612051	59.95%	8.047%
30	5.989	1526	1539	1561	rBV	227307	476033	46.63%	6.259%
31	6.314	1638	1640	1643	rBV4	1026	567	0.06%	0.007%
32	6.359	1651	1654	1657	rVB4	1388	981	0.10%	0.013%
33	6.375	1657	1659	1661	rBV2	966	568	0.06%	0.007%
34	6.603	1727	1730	1733	rVB4	1554	992	0.10%	0.013%
35	6.645	1740	1743	1744	rBV2	984	548	0.05%	0.007%
36	6.802	1787	1792	1794	rBV5	1101	1060	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122123\
 Data File : VW033533.D
 Acq On : 21 Dec 2023 14:37
 Operator : SY/MD
 Sample : 05850-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	6.879	1812	1816	1817	rBV3	898	765	0.07%	0.010%
38	6.915	1817	1827	1852	rVV	105513	206070	20.19%	2.709%
39	7.243	1918	1929	1957	rBV	401374	722423	70.77%	9.498%
40	7.555	2017	2026	2047	rBV2	75579	139227	13.64%	1.831%
41	7.831	2110	2112	2115	rBV5	1319	921	0.09%	0.012%
42	8.027	2164	2173	2207	rBV	196782	428529	41.98%	5.634%
43	8.545	2332	2334	2336	rBV2	1598	593	0.06%	0.008%
44	8.744	2394	2396	2397	rBV2	1054	554	0.05%	0.007%
45	8.786	2398	2409	2431	rVV	482338	800240	78.39%	10.521%
46	9.198	2533	2537	2542	rVB6	2037	1828	0.18%	0.024%
47	9.249	2549	2553	2554	rBV3	1169	846	0.08%	0.011%
48	9.413	2602	2604	2609	rVB5	1736	1434	0.14%	0.019%
49	9.439	2609	2612	2614	rBV4	1509	1060	0.10%	0.014%
50	9.487	2620	2627	2629	rBV7	1312	1243	0.12%	0.016%
51	9.567	2649	2652	2654	rBV4	1168	689	0.07%	0.009%
52	9.657	2677	2680	2683	rBV5	1389	1016	0.10%	0.013%
53	9.998	2782	2786	2788	rBV4	887	752	0.07%	0.010%
54	10.098	2813	2817	2818	rBV4	986	674	0.07%	0.009%
55	10.153	2823	2834	2859	rVB	313293	499066	48.89%	6.562%
56	10.423	2916	2918	2920	rBV2	1275	679	0.07%	0.009%
57	10.529	2949	2951	2954	rBV3	992	509	0.05%	0.007%
58	10.641	2981	2986	2990	rBV7	1358	1408	0.14%	0.019%
59	10.683	2997	2999	3001	rVB3	1000	472	0.05%	0.006%
60	10.696	3001	3003	3006	rBV4	1147	499	0.05%	0.007%
61	10.712	3006	3008	3011	rBV4	1591	955	0.09%	0.013%
62	10.918	3069	3072	3075	rBV5	1206	858	0.08%	0.011%
63	10.985	3090	3093	3095	rBV3	745	542	0.05%	0.007%
64	11.114	3128	3133	3135	rBV6	1145	1223	0.12%	0.016%
65	11.185	3144	3155	3179	rVV	433698	694581	68.04%	9.132%
66	11.413	3224	3226	3230	rBV3	1001	540	0.05%	0.007%
67	11.561	3258	3272	3294	rBV	441924	717192	70.25%	9.429%
68	11.854	3361	3363	3366	rBV4	1045	621	0.06%	0.008%
69	11.902	3375	3378	3381	rBV5	838	449	0.04%	0.006%
70	11.969	3397	3399	3402	rVB4	1218	682	0.07%	0.009%
71	12.040	3417	3421	3423	rBV4	1154	772	0.08%	0.010%
72	12.188	3462	3467	3470	rBV5	1347	1274	0.12%	0.017%
73	12.288	3494	3498	3502	rBV4	1111	892	0.09%	0.012%
74	12.542	3573	3577	3578	rBV3	778	517	0.05%	0.007%
75	12.580	3585	3589	3590	rBV3	999	714	0.07%	0.009%
76	12.702	3624	3627	3634	rVB6	1594	1524	0.15%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033533.D
 Acq On : 21 Dec 2023 14:37
 Operator : SY/MD
 Sample : 05850-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	12.738	3634	3638	3642	rBV5	1487	1584	0.16%	0.021%
78	12.757	3642	3644	3646	rBV3	904	463	0.05%	0.006%
79	12.934	3697	3699	3702	rVB3	1043	459	0.04%	0.006%
80	12.972	3707	3711	3713	rBV5	715	515	0.05%	0.007%
81	13.050	3732	3735	3738	rBV4	1345	1231	0.12%	0.016%
82	13.159	3766	3769	3771	rBV4	1131	866	0.08%	0.011%
83	13.313	3813	3817	3818	rBV3	971	682	0.07%	0.009%
84	13.339	3823	3825	3829	rVB4	946	603	0.06%	0.008%
85	13.464	3859	3864	3867	rBV6	1689	1824	0.18%	0.024%
86	13.654	3921	3923	3928	rVB5	1145	642	0.06%	0.008%
87	13.722	3942	3944	3947	rVB4	1010	512	0.05%	0.007%
88	13.905	3998	4001	4005	rBV5	1042	1094	0.11%	0.014%
89	13.924	4005	4007	4011	rVV3	887	615	0.06%	0.008%
90	13.966	4016	4020	4021	rBV2	1803	1177	0.12%	0.015%
91	14.056	4045	4048	4052	rBV5	1384	1034	0.10%	0.014%
92	14.185	4087	4088	4092	rBV3	781	531	0.05%	0.007%
93	14.230	4097	4102	4104	rBV6	1435	1140	0.11%	0.015%
94	14.378	4145	4148	4150	rVV3	1462	758	0.07%	0.010%
95	14.493	4180	4184	4186	rVB4	1471	924	0.09%	0.012%
96	14.516	4187	4191	4195	rVB6	1238	1262	0.12%	0.017%
97	14.947	4322	4325	4327	rBV3	2137	1391	0.14%	0.018%
98	15.233	4412	4414	4417	rBV3	1000	632	0.06%	0.008%
99	15.262	4420	4423	4425	rBV4	1297	842	0.08%	0.011%
100	15.516	4499	4502	4505	rBV4	1855	1501	0.15%	0.020%




Sum of corrected areas: 7605916

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033533.D
Acq On : 21 Dec 2023 14:37
Operator : SY/MD
Sample : 05850-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

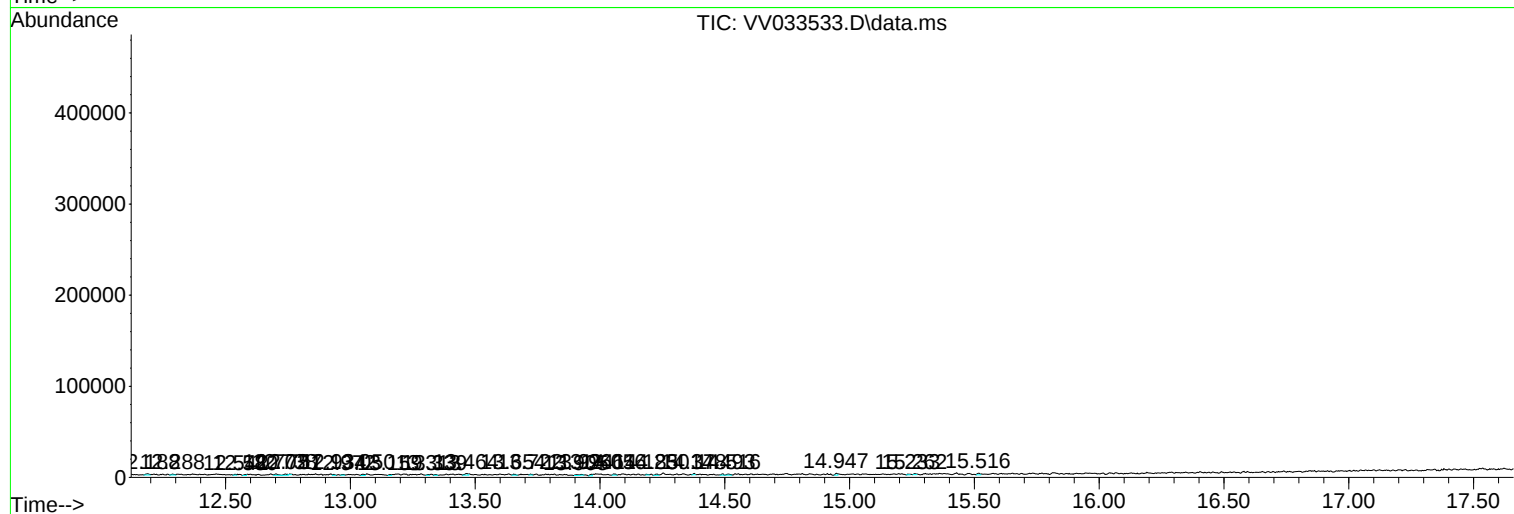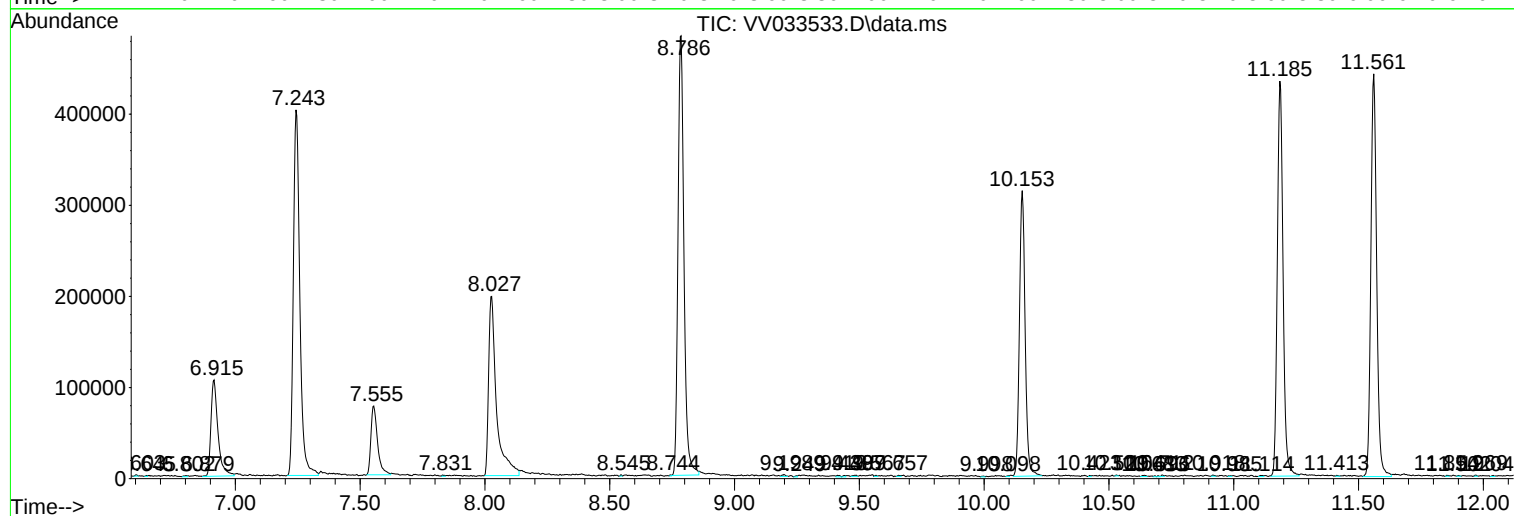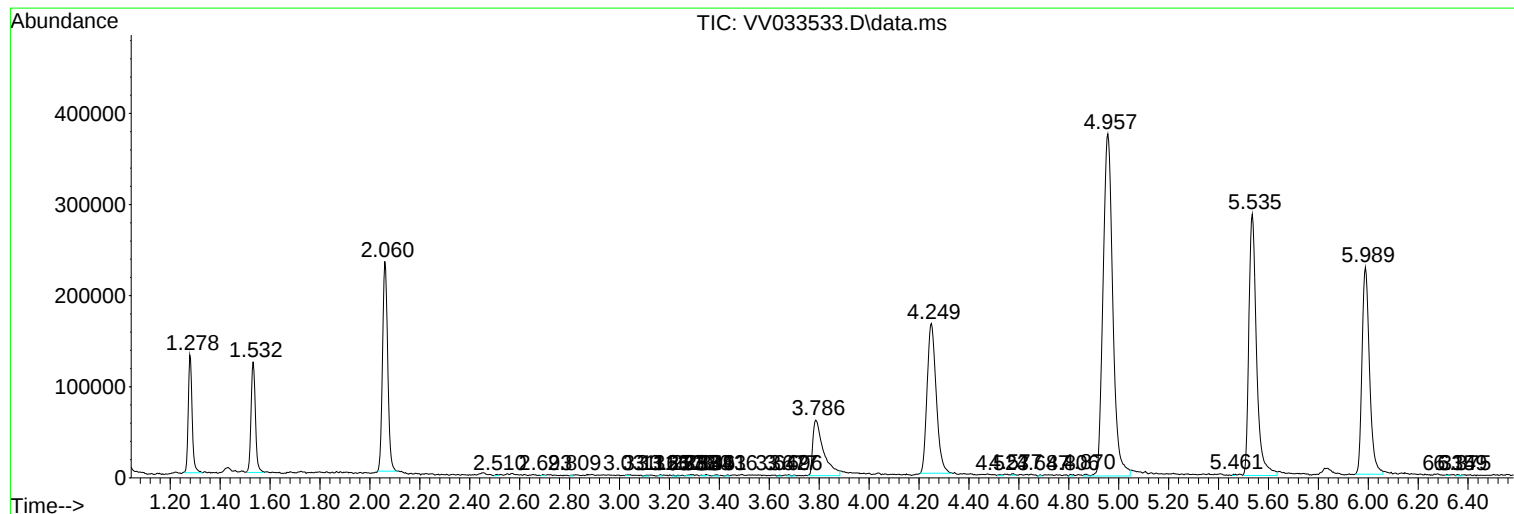

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033533.D
Acq On : 21 Dec 2023 14:37
Operator : SY/MD
Sample : 05850-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033533.D
Acq On : 21 Dec 2023 14:37
Operator : SY/MD
Sample : 05850-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------