

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122123\
 Data File : VW033534.D
 Acq On : 21 Dec 2023 15:01
 Operator : SY/MD
 Sample : 05895-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VW033534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	125849	132943	13.59%	1.802%
2	1.532	146	153	165	rVB	119666	136611	13.97%	1.852%
3	2.060	309	317	333	rVB	223927	321241	32.85%	4.354%
4	2.638	495	497	500	rBV4	649	372	0.04%	0.005%
5	2.658	500	503	504	rBV4	878	507	0.05%	0.007%
6	2.790	543	544	545	rBV2	743	196	0.02%	0.003%
7	2.908	579	581	583	rBV3	931	381	0.04%	0.005%
8	3.050	620	625	626	rBV4	1626	1171	0.12%	0.016%
9	3.140	651	653	654	rBV2	1181	481	0.05%	0.007%
10	3.236	680	683	687	rBV6	1300	889	0.09%	0.012%
11	3.285	695	698	699	rBV2	941	597	0.06%	0.008%
12	3.375	724	726	727	rBV2	692	252	0.03%	0.003%
13	3.404	733	735	738	rVB4	1130	520	0.05%	0.007%
14	3.429	740	743	746	rBV4	1080	848	0.09%	0.011%
15	3.516	768	770	772	rBV2	832	271	0.03%	0.004%
16	3.561	781	784	786	rBV3	630	504	0.05%	0.007%
17	3.616	800	801	802	rBV	392	87	0.01%	0.001%
18	3.706	824	829	831	rBV4	1328	842	0.09%	0.011%
19	3.751	841	843	844	rBV2	1082	514	0.05%	0.007%
20	3.786	846	854	887	rVV	63546	184366	18.85%	2.499%
21	4.249	986	998	1021	rVB	160921	404229	41.33%	5.479%
22	4.648	1120	1122	1124	rBV2	772	349	0.04%	0.005%
23	4.838	1179	1181	1183	rBV3	1026	425	0.04%	0.006%
24	4.879	1192	1194	1197	rBV4	1087	723	0.07%	0.010%
25	4.957	1203	1218	1248	rBV2	362562	978044	100.00%	13.256%
26	5.535	1386	1398	1427	rBV	277626	585953	59.91%	7.942%
27	5.989	1528	1539	1564	rBV	223204	455358	46.56%	6.172%
28	6.449	1680	1682	1686	rBV5	1157	436	0.04%	0.006%
29	6.802	1789	1792	1793	rBV2	925	488	0.05%	0.007%
30	6.915	1817	1827	1844	rBV	103190	195772	20.02%	2.653%
31	7.146	1897	1899	1901	rBV3	807	265	0.03%	0.004%
32	7.243	1918	1929	1951	rBV	392578	706915	72.28%	9.581%
33	7.551	2017	2025	2045	rBV2	75099	136444	13.95%	1.849%
34	7.879	2124	2127	2129	rBV4	1472	970	0.10%	0.013%
35	7.976	2154	2157	2159	rVB3	542	265	0.03%	0.004%
36	8.027	2159	2173	2211	rBV	202065	455132	46.53%	6.169%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122123\
 Data File : VW033534.D
 Acq On : 21 Dec 2023 15:01
 Operator : SY/MD
 Sample : 05895-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	8.712	2384	2386	2387	rBV2	1186	536	0.05%	0.007%
38	8.783	2398	2408	2432	rBV	471459	785822	80.35%	10.651%
39	9.882	2746	2750	2753	rVB4	1295	978	0.10%	0.013%
40	10.153	2822	2834	2854	rBV	306265	488323	49.93%	6.619%
41	10.474	2932	2934	2935	rBV2	1106	499	0.05%	0.007%
42	10.574	2962	2965	2967	rVB2	1136	589	0.06%	0.008%
43	10.635	2982	2984	2985	rBV2	679	333	0.03%	0.005%
44	10.863	3051	3055	3056	rBV3	1624	1123	0.11%	0.015%
45	11.037	3107	3109	3112	rBV4	1011	603	0.06%	0.008%
46	11.079	3120	3122	3124	rBV3	730	344	0.04%	0.005%
47	11.104	3127	3130	3131	rBV2	1399	715	0.07%	0.010%
48	11.185	3143	3155	3177	rBV	428998	678598	69.38%	9.198%
49	11.561	3261	3272	3290	rBV	431440	689608	70.51%	9.347%
50	11.808	3347	3349	3352	rBV3	1037	600	0.06%	0.008%
51	11.831	3354	3356	3358	rBV3	1367	850	0.09%	0.012%
52	11.934	3385	3388	3392	rBV6	1033	716	0.07%	0.010%
53	12.030	3416	3418	3420	rBV3	1160	513	0.05%	0.007%
54	12.043	3420	3422	3424	rBV2	824	420	0.04%	0.006%
55	12.133	3447	3450	3455	rVB5	1059	984	0.10%	0.013%
56	12.159	3455	3458	3459	rBV3	567	281	0.03%	0.004%
57	12.165	3459	3460	3462	rBV2	867	444	0.05%	0.006%
58	12.307	3502	3504	3505	rBV	1100	345	0.04%	0.005%
59	12.336	3511	3513	3515	rBV2	1040	551	0.06%	0.007%
60	12.413	3535	3537	3540	rBV3	743	552	0.06%	0.007%
61	12.445	3544	3547	3550	rBB4	1620	852	0.09%	0.012%
62	12.468	3550	3554	3555	rBV4	1125	742	0.08%	0.010%
63	12.644	3607	3609	3611	rBV3	921	484	0.05%	0.007%
64	12.850	3670	3673	3676	rVB5	940	527	0.05%	0.007%
65	13.040	3730	3732	3736	rVB3	1614	837	0.09%	0.011%
66	13.069	3736	3741	3745	rBV7	1408	1556	0.16%	0.021%
67	13.133	3758	3761	3765	rBV4	1679	1521	0.16%	0.021%
68	13.159	3767	3769	3771	rBV4	1074	550	0.06%	0.007%
69	13.194	3777	3780	3781	rBV4	1377	678	0.07%	0.009%
70	13.329	3820	3822	3823	rBV	954	358	0.04%	0.005%
71	13.406	3843	3846	3848	rBV4	1405	834	0.09%	0.011%
72	13.458	3858	3862	3865	rBV5	1448	1226	0.13%	0.017%
73	13.587	3900	3902	3904	rBV3	1260	638	0.07%	0.009%
74	13.734	3946	3948	3950	rBV3	1167	603	0.06%	0.008%
75	13.972	4019	4022	4025	rBV4	957	807	0.08%	0.011%
76	14.069	4051	4052	4056	rVB2	961	378	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033534.D
Acq On : 21 Dec 2023 15:01
Operator : SY/MD
Sample : 05895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis

77	14.088	4056	4058	4060	rBV2	1259	703	0.07%	0.010%
78	14.217	4096	4098	4101	rVB4	2119	984	0.10%	0.013%
79	14.635	4225	4228	4230	rBV4	1611	1107	0.11%	0.015%
80	14.709	4247	4251	4254	rBV4	1660	1645	0.17%	0.022%
81	15.821	4595	4597	4599	rBV3	1865	1218	0.12%	0.017%




Sum of corrected areas: 7377936

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033534.D
Acq On : 21 Dec 2023 15:01
Operator : SY/MD
Sample : 05895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

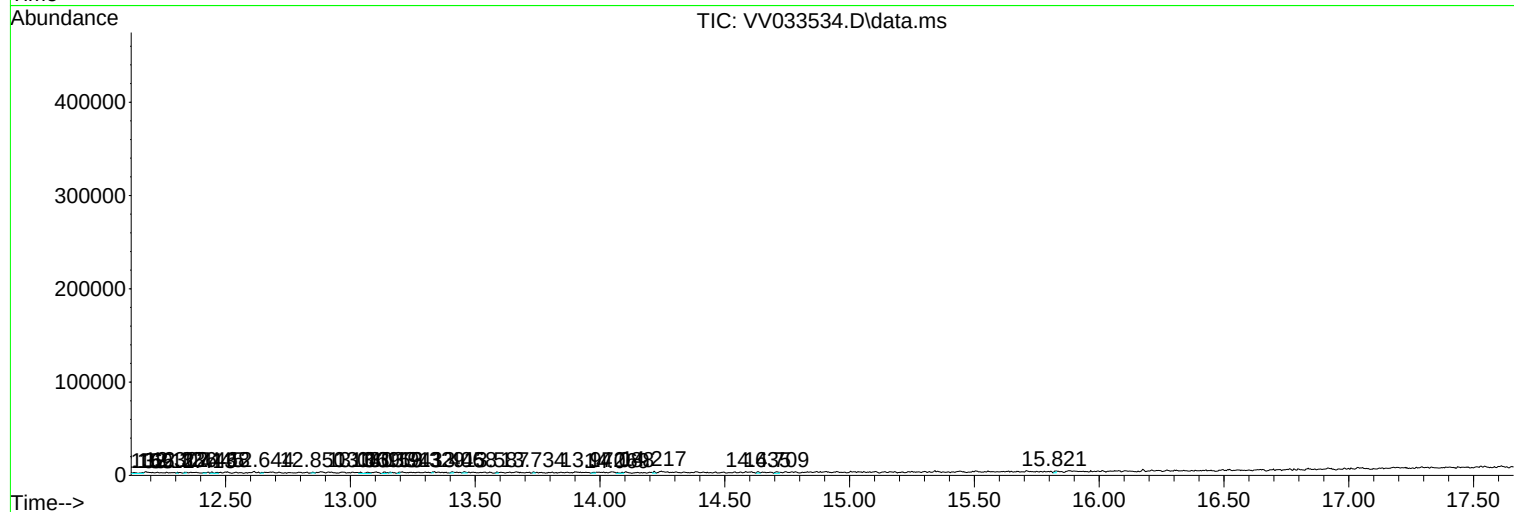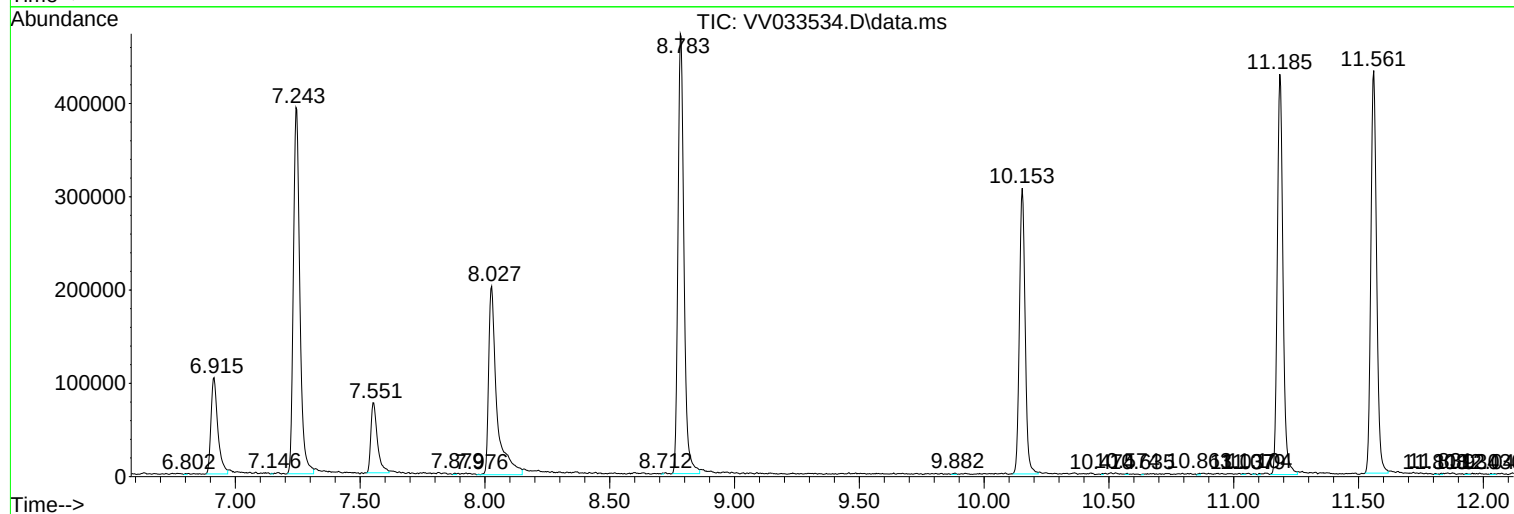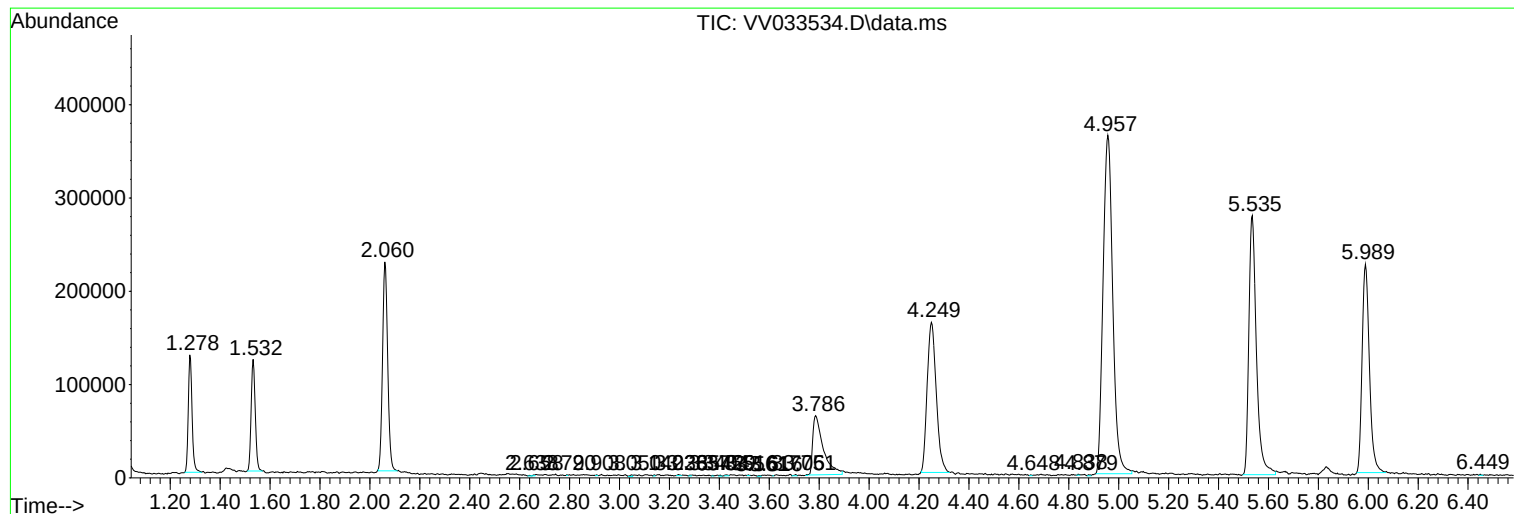

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033534.D
Acq On : 21 Dec 2023 15:01
Operator : SY/MD
Sample : 05895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033534.D
Acq On : 21 Dec 2023 15:01
Operator : SY/MD
Sample : 05895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------