

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
 Data File : VV033536.D
 Acq On : 21 Dec 2023 15:47
 Operator : SY/MD
 Sample : 05891-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCLT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

Signal : TIC: VV033536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	126886	136940	13.34%	1.792%
2	1.532	146	153	164	rBV	123641	143504	13.98%	1.878%
3	2.059	308	317	335	rBV	230816	339976	33.11%	4.449%
4	2.381	415	417	425	rBV8	1425	1624	0.16%	0.021%
5	2.670	505	507	508	rBV2	905	398	0.04%	0.005%
6	2.828	552	556	557	rBV3	649	360	0.04%	0.005%
7	2.841	557	560	563	rVB4	1591	1030	0.10%	0.013%
8	2.857	563	565	569	rBV5	779	781	0.08%	0.010%
9	2.879	569	572	574	rBV3	1085	770	0.07%	0.010%
10	2.928	582	587	590	rBV5	1161	991	0.10%	0.013%
11	2.973	595	601	604	rBV4	1369	1408	0.14%	0.018%
12	2.995	604	608	609	rBV3	927	692	0.07%	0.009%
13	3.111	641	644	650	rBV7	1186	903	0.09%	0.012%
14	3.146	653	655	656	rBV	887	380	0.04%	0.005%
15	3.156	656	658	659	rBV2	742	278	0.03%	0.004%
16	3.249	685	687	691	rVB4	1302	699	0.07%	0.009%
17	3.281	695	697	699	rBV3	693	373	0.04%	0.005%
18	3.304	702	704	706	rBV3	895	373	0.04%	0.005%
19	3.323	708	710	713	rBV4	818	542	0.05%	0.007%
20	3.432	740	744	747	rVB5	1312	1114	0.11%	0.015%
21	3.445	747	748	751	rBV3	1247	625	0.06%	0.008%
22	3.481	756	759	762	rVB5	1299	831	0.08%	0.011%
23	3.500	762	765	768	rBV5	1159	918	0.09%	0.012%
24	3.564	783	785	786	rBV2	844	271	0.03%	0.004%
25	3.590	792	793	798	rBV5	837	518	0.05%	0.007%
26	3.641	807	809	812	rBV3	889	635	0.06%	0.008%
27	3.693	823	825	828	rVB3	760	271	0.03%	0.004%
28	3.709	828	830	831	rBV	642	248	0.02%	0.003%
29	3.783	845	853	880	rBV	51949	148072	14.42%	1.938%
30	4.030	928	930	931	rBV2	1237	516	0.05%	0.007%
31	4.156	967	969	971	rBV3	1337	495	0.05%	0.006%
32	4.249	984	998	1020	rBV	167631	425968	41.49%	5.574%
33	4.471	1064	1067	1070	rBV6	1434	968	0.09%	0.013%
34	4.612	1108	1111	1115	rVB5	1372	743	0.07%	0.010%
35	4.667	1124	1128	1130	rBV5	1385	1072	0.10%	0.014%
36	4.831	1177	1179	1180	rBV2	981	368	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122123\
 Data File : VW033536.D
 Acq On : 21 Dec 2023 15:47
 Operator : SY/MD
 Sample : 05891-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCLT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

37	4.956	1202	1218	1247	rBV2	379349	1026692	100.00%	13.435%
38	5.403	1354	1357	1360	rBV5	1025	751	0.07%	0.010%
39	5.445	1365	1370	1373	rBV6	1540	1524	0.15%	0.020%
40	5.535	1386	1398	1422	rBV	294218	628383	61.20%	8.223%
41	5.918	1514	1517	1519	rBV4	1141	829	0.08%	0.011%
42	5.989	1527	1539	1560	rBV	233843	482289	46.98%	6.311%
43	6.448	1680	1682	1683	rBV2	769	253	0.02%	0.003%
44	6.535	1703	1709	1711	rBV6	1308	1397	0.14%	0.018%
45	6.828	1798	1800	1801	rBV2	1081	427	0.04%	0.006%
46	6.915	1813	1827	1843	rBV	107772	208118	20.27%	2.723%
47	7.120	1889	1891	1894	rBV5	949	576	0.06%	0.008%
48	7.243	1919	1929	1952	rBV	412252	736445	71.73%	9.637%
49	7.551	2017	2025	2048	rBV2	78166	142003	13.83%	1.858%
50	8.024	2164	2172	2207	rBV	178585	393768	38.35%	5.153%
51	8.570	2339	2342	2344	rBV3	817	621	0.06%	0.008%
52	8.596	2349	2350	2351	rBV	720	252	0.02%	0.003%
53	8.786	2398	2409	2435	rBV	503118	832773	81.11%	10.898%
54	9.130	2513	2516	2518	rBV4	1352	913	0.09%	0.012%
55	9.220	2542	2544	2547	rBV3	1564	1022	0.10%	0.013%
56	9.333	2576	2579	2580	rBV2	1283	603	0.06%	0.008%
57	9.644	2674	2676	2677	rBV2	1148	383	0.04%	0.005%
58	9.979	2776	2780	2782	rBV2	1547	1083	0.11%	0.014%
59	10.011	2789	2790	2792	rBV2	658	302	0.03%	0.004%
60	10.107	2818	2820	2821	rBV2	988	426	0.04%	0.006%
61	10.152	2822	2834	2850	rVV	300187	476629	46.42%	6.237%
62	10.326	2879	2888	2890	rBV9	4470	5216	0.51%	0.068%
63	10.410	2912	2914	2917	rBV4	1050	561	0.05%	0.007%
64	10.593	2970	2971	2972	rBV	946	255	0.02%	0.003%
65	10.673	2994	2996	3000	rVB5	1646	1172	0.11%	0.015%
66	10.699	3000	3004	3007	rBV4	621	559	0.05%	0.007%
67	10.722	3007	3011	3012	rBV3	1427	1087	0.11%	0.014%
68	10.767	3021	3025	3027	rBV4	952	698	0.07%	0.009%
69	10.792	3030	3033	3037	rVV6	1410	872	0.08%	0.011%
70	10.860	3052	3054	3058	rBV4	1372	827	0.08%	0.011%
71	10.905	3064	3068	3071	rBV6	1723	1356	0.13%	0.018%
72	11.011	3100	3101	3105	rVB3	1345	560	0.05%	0.007%
73	11.066	3115	3118	3122	rVB6	1018	863	0.08%	0.011%
74	11.098	3125	3128	3130	rBV4	952	768	0.07%	0.010%
75	11.185	3144	3155	3173	rBV	461208	714190	69.56%	9.346%
76	11.426	3228	3230	3233	rBV3	1243	696	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122123\
 Data File : VW033536.D
 Acq On : 21 Dec 2023 15:47
 Operator : SY/MD
 Sample : 05891-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCLT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
 Title : VOC Analysis

77	11.561	3263	3272	3289	rVB	474021	737107	71.79%	9.646%
78	12.152	3451	3456	3457	rBV5	1486	1071	0.10%	0.014%
79	12.586	3588	3591	3593	rBV2	2169	1187	0.12%	0.016%
80	13.024	3723	3727	3730	rBV6	1898	1339	0.13%	0.018%
81	13.043	3731	3733	3734	rBV3	1109	357	0.03%	0.005%
82	13.104	3750	3752	3756	rBV5	1218	906	0.09%	0.012%
83	13.300	3811	3813	3817	rBV5	1169	815	0.08%	0.011%
84	13.352	3825	3829	3832	rBV6	1541	1402	0.14%	0.018%
85	13.400	3842	3844	3847	rVB3	1767	835	0.08%	0.011%
86	13.506	3875	3877	3880	rBV3	1119	424	0.04%	0.006%
87	13.554	3890	3892	3895	rBV5	883	466	0.05%	0.006%
88	13.853	3983	3985	3986	rBV2	774	335	0.03%	0.004%
89	13.914	3999	4004	4006	rBV5	1619	1173	0.11%	0.015%
90	13.982	4022	4025	4028	rBV5	2068	1542	0.15%	0.020%
91	14.059	4047	4049	4052	rBV4	935	547	0.05%	0.007%
92	14.287	4117	4120	4121	rBV3	1447	707	0.07%	0.009%
93	14.329	4131	4133	4136	rVB4	1294	470	0.05%	0.006%
94	14.393	4152	4153	4155	rBV3	955	404	0.04%	0.005%
95	14.458	4169	4173	4175	rBV4	1192	1086	0.11%	0.014%
96	14.795	4276	4278	4281	rBV4	1020	710	0.07%	0.009%
97	15.213	4405	4408	4409	rBV3	928	649	0.06%	0.008%
98	15.509	4496	4500	4502	rBV3	2440	2033	0.20%	0.027%
99	15.667	4546	4549	4550	rBV3	1756	1095	0.11%	0.014%
100	16.001	4651	4653	4656	rBV3	1714	1188	0.12%	0.016%


Sum of corrected areas: 7641645

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033536.D
Acq On : 21 Dec 2023 15:47
Operator : SY/MD
Sample : 05891-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCLT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

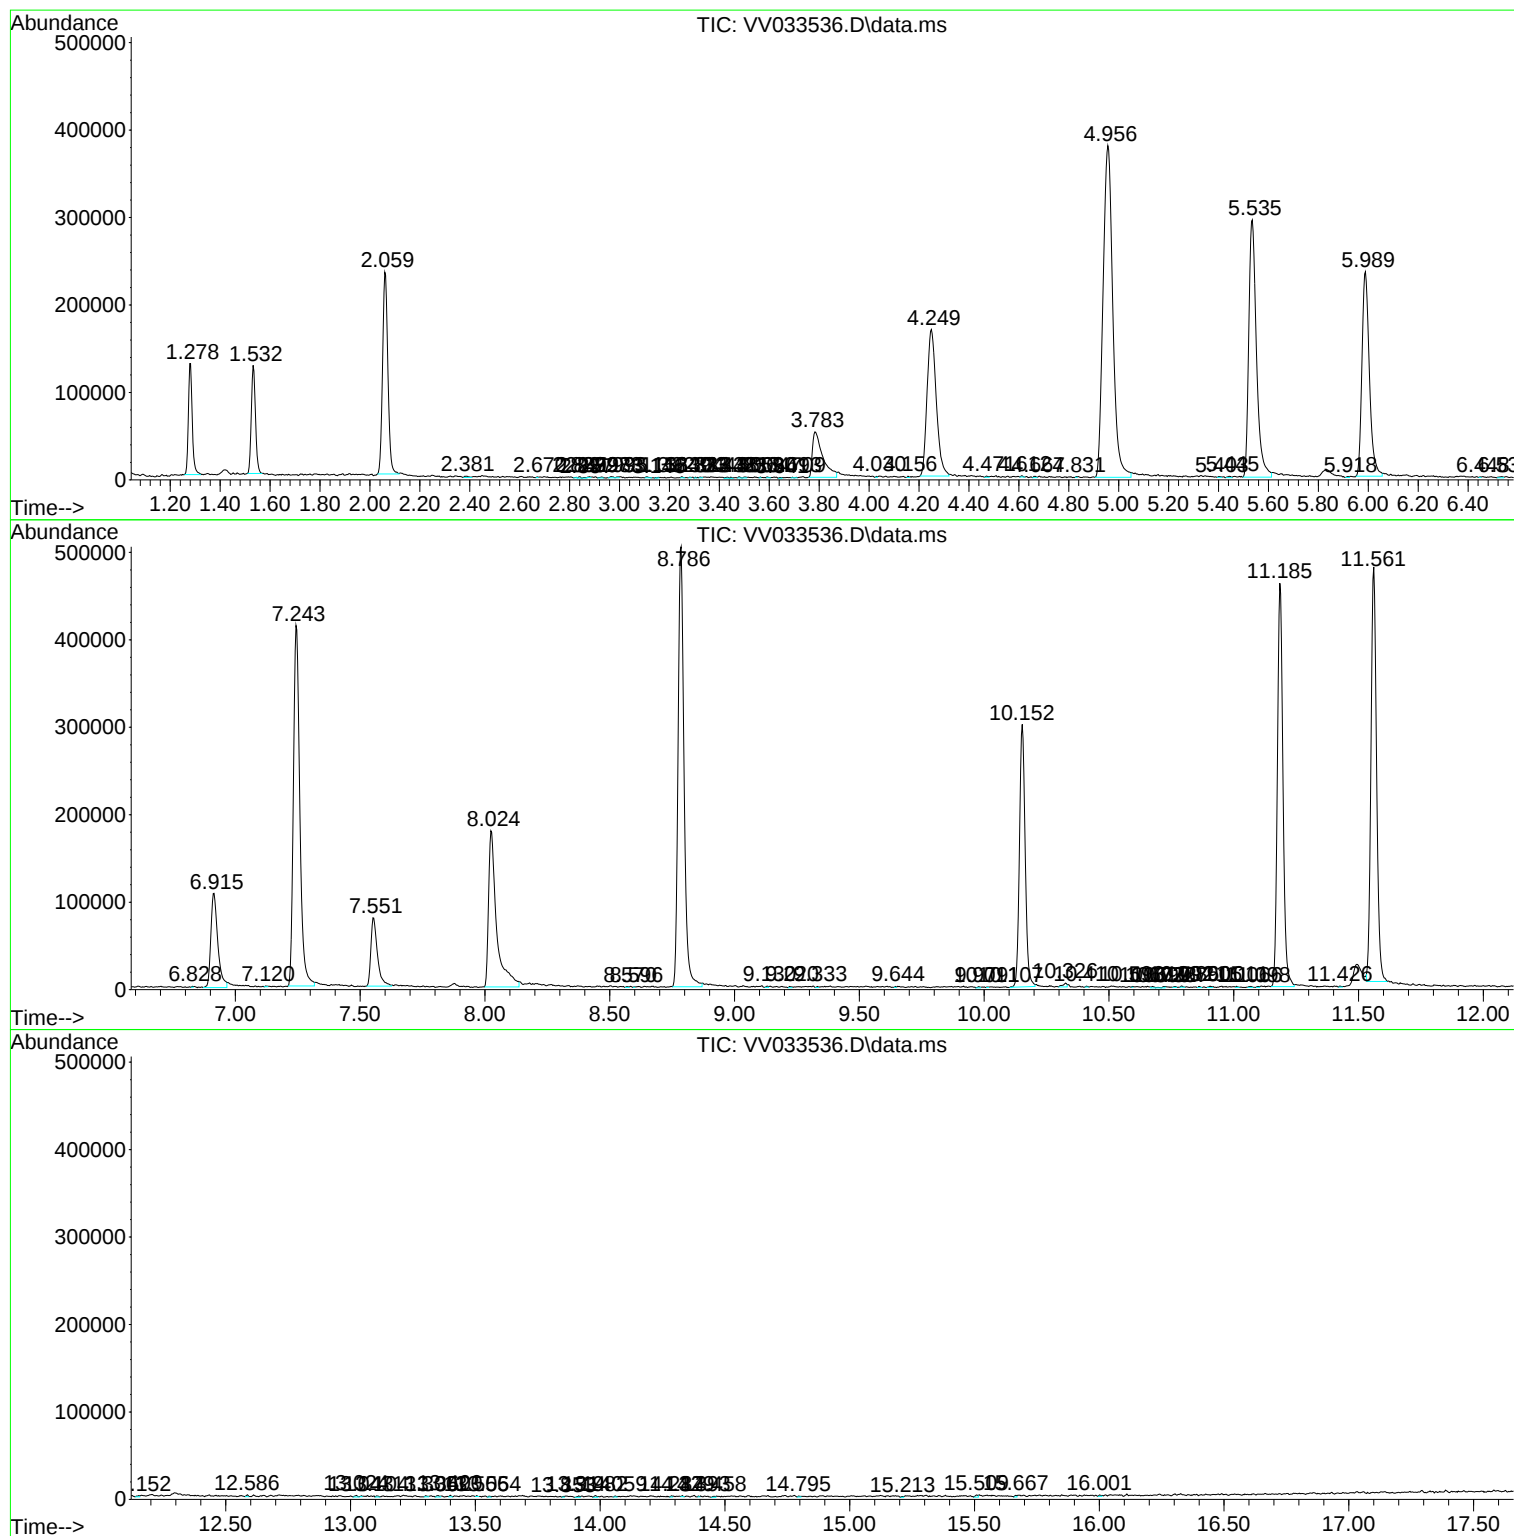

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033536.D
Acq On : 21 Dec 2023 15:47
Operator : SY/MD
Sample : 05891-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCLT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033536.D
Acq On : 21 Dec 2023 15:47
Operator : SY/MD
Sample : 05891-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCLT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------