


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122123\
Data File : VV033524.D
Acq On : 21 Dec 2023 10:50
Operator : SY/MD
Sample : BFB251
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB251

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM121523WMA.M
Title : VOC Analysis
Last Update : Fri Dec 22 01:45:30 2023

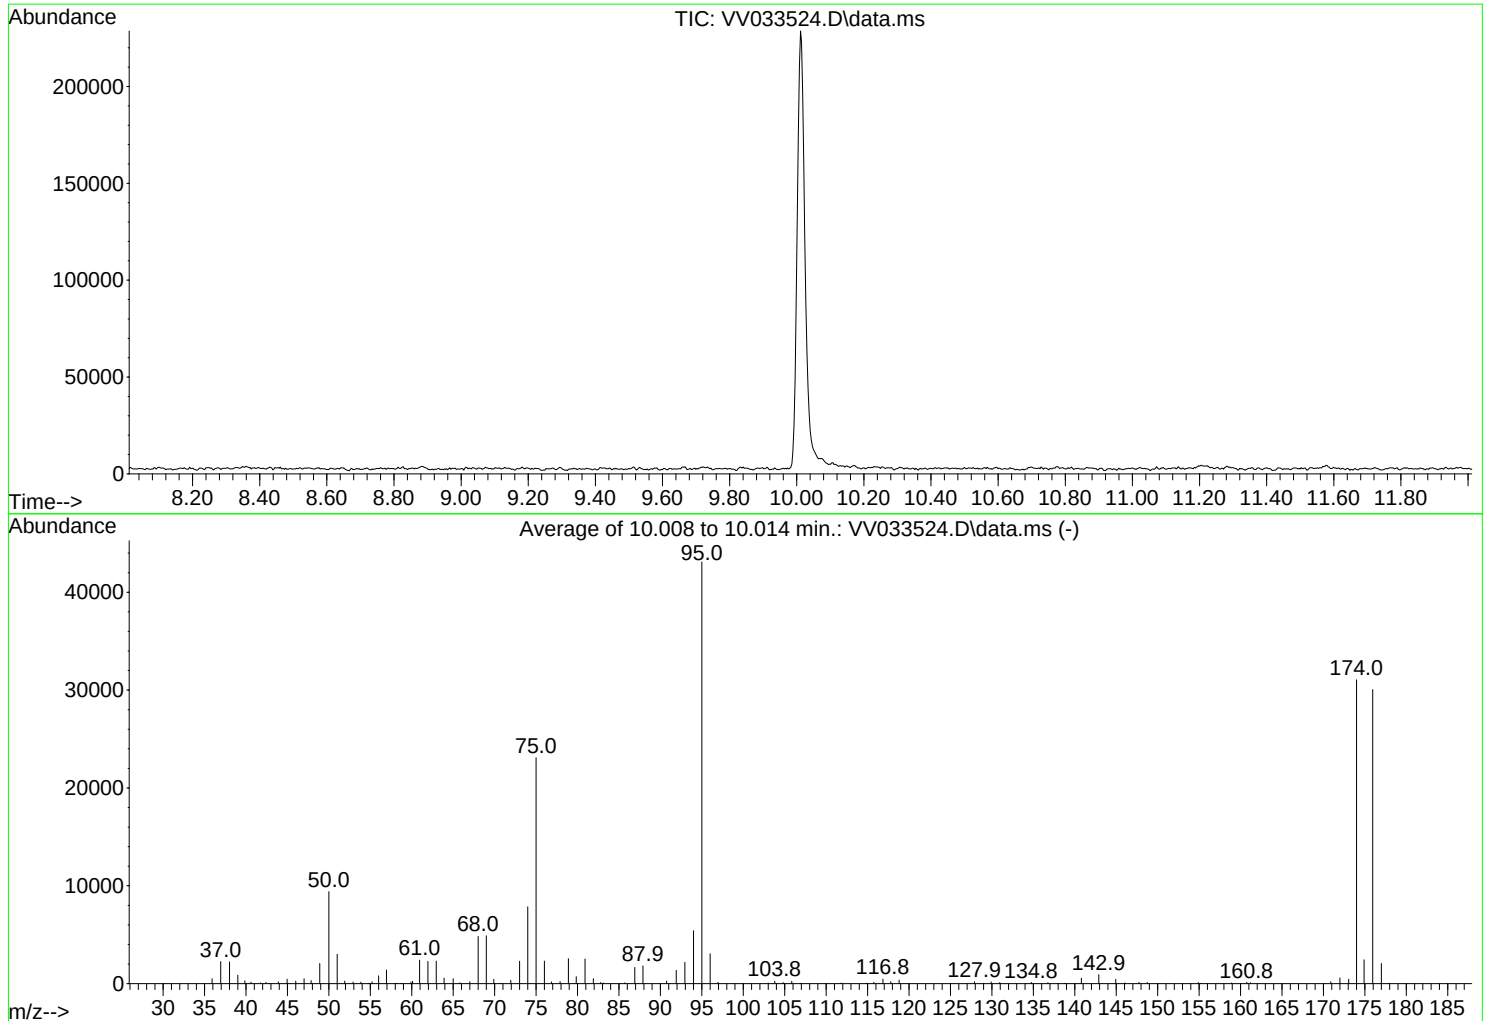

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	9397	PASS
75	95	30	80	53.6	23093	PASS
95	95	100	100	100.0	43107	PASS
96	95	5	9	7.1	3060	PASS
173	174	0.00	2	1.5	465	PASS
174	95	50	120	72.0	31053	PASS
175	174	5	9	7.9	2439	PASS
176	174	95	105	96.8	30051	PASS
177	176	5	10	6.8	2057	PASS

m/z	Abundance
35.20	109.0
36.90	139.0
38.30	146.0
39.20	154.0
39.80	355.0
41.30	114.0
42.70	130.0
43.90	387.0
45.20	102.0
48.80	132.0
50.00	100.0
52.40	118.0
60.10	101.0
61.80	116.0
77.00	108.0
77.80	113.0
94.60	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251

m/z	Abundance
35.90	512.0
37.00	2442.0
38.00	2180.0
39.00	1028.0
39.90	580.0
41.80	116.0
42.40	148.0
42.90	148.0
43.90	552.0
45.00	439.0
45.90	250.0
46.90	566.0
47.90	265.0
49.00	2114.0
50.00	9043.0
51.00	2983.0
51.90	270.0
52.90	131.0
53.80	110.0
54.80	115.0
55.30	167.0
56.00	829.0
56.90	1341.0
57.90	110.0
59.90	484.0
61.00	2327.0
62.00	2197.0
63.00	2363.0
63.90	556.0
65.00	429.0
66.90	198.0
68.00	4922.0
69.00	4742.0
69.90	482.0
70.70	103.0
71.90	299.0
73.00	2154.0
74.00	7635.0
75.00	22072.0
76.00	2291.0
76.90	238.0
77.90	348.0
78.90	2470.0
79.80	612.0
80.90	2352.0
81.90	457.0
82.80	105.0
83.10	109.0
85.70	156.0
86.90	1636.0
87.90	1595.0
90.80	251.0
91.90	1169.0
93.00	2117.0
94.00	5056.0
95.00	41336.0
96.00	3034.0
97.00	135.0
103.80	261.0
104.80	104.0
105.90	244.0
106.90	118.0
115.70	137.0
116.90	466.0
117.80	215.0
118.80	363.0
127.90	199.0
129.80	178.0
131.00	102.0
134.80	116.0
136.80	161.0
138.00	108.0
140.80	513.0
142.90	914.0
144.90	481.0
146.00	127.0
147.80	122.0
148.80	103.0
154.90	108.0
155.20	103.0
160.80	109.0
161.20	166.0
170.90	167.0
172.00	537.0
173.00	688.0
174.00	28336.0
174.90	2473.0
175.90	28328.0
177.00	1820.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251

m/z	Abundance
35.90	518.0
37.00	2468.0
38.00	2333.0
39.00	1059.0
39.90	690.0
40.60	215.0
41.70	117.0
42.40	149.0
42.90	150.0
44.00	570.0
45.00	464.0
46.00	241.0
47.00	494.0
47.90	313.0
49.00	2248.0
50.00	9886.0
51.00	3121.0
51.90	280.0
52.90	182.0
53.90	148.0
55.20	191.0
56.00	835.0
57.00	1416.0
58.20	108.0
60.10	514.0
61.00	2559.0
62.00	2442.0
62.90	2354.0
63.90	604.0
65.00	537.0
65.80	140.0
67.00	191.0
68.00	4962.0
69.00	5061.0
69.90	454.0
71.90	351.0
73.00	2350.0
74.00	8142.0
75.00	23888.0
76.00	2384.0
76.90	312.0
78.00	344.0
78.90	2621.0
79.90	735.0
80.90	2610.0
81.90	497.0
82.80	124.0
83.10	116.0
85.70	102.0
86.90	1704.0
87.90	1891.0
90.70	268.0
91.90	1376.0
93.00	2251.0
94.00	5583.0
95.00	44688.0
96.00	3287.0
96.90	135.0
103.80	246.0
104.80	106.0
105.90	258.0
111.80	104.0
115.70	132.0
116.90	465.0
117.80	204.0
118.80	404.0
127.90	196.0
129.90	176.0
131.00	114.0
134.70	125.0
136.70	138.0
140.80	583.0
142.90	933.0
145.00	435.0
146.10	121.0
147.70	133.0
148.80	131.0
154.90	132.0
159.00	105.0
160.70	146.0
161.20	130.0
170.90	204.0
172.00	635.0
173.10	707.0
174.00	32048.0
174.90	2488.0
176.00	31008.0
177.00	2150.0
177.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251

m/z	Abundance
35.90	491.0
37.00	2289.0
38.00	2146.0
39.00	974.0
39.90	677.0
40.60	215.0
42.40	121.0
42.90	127.0
44.00	576.0
44.90	489.0
46.10	270.0
47.10	439.0
47.80	361.0
48.90	2214.0
50.00	9561.0
51.00	2927.0
51.90	253.0
52.90	207.0
53.80	189.0
55.10	230.0
56.00	759.0
57.00	1404.0
58.70	110.0
60.10	530.0
60.90	2354.0
62.00	2521.0
62.90	2208.0
63.90	570.0
65.00	550.0
65.80	131.0
67.10	194.0
68.00	4595.0
69.00	4849.0
69.90	373.0
72.00	360.0
73.00	2344.0
74.00	7782.0
75.00	23320.0
76.00	2246.0
76.80	324.0
78.00	264.0
78.90	2545.0
79.90	802.0
80.90	2609.0
81.90	566.0
82.80	122.0
86.90	1602.0
87.90	1938.0
90.70	245.0
91.90	1522.0
92.90	2143.0
94.00	5591.0
95.00	43296.0
96.00	2860.0
96.90	129.0
103.00	126.0
103.80	230.0
104.80	116.0
105.80	219.0
111.80	109.0
114.80	134.0
115.80	152.0
116.80	435.0
117.80	214.0
118.80	356.0
127.90	190.0
129.00	119.0
130.00	175.0
130.90	116.0
134.70	136.0
138.80	103.0
140.80	557.0
142.90	893.0
145.00	408.0
147.70	132.0
148.70	141.0
154.90	130.0
158.80	109.0
160.70	126.0
170.90	214.0
172.00	608.0
174.00	32776.0
174.90	2357.0
176.00	30816.0
177.00	2202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB251