

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019790.D
 Acq On : 22 Dec 2020 10:55
 Operator : SY/MD
 Sample : VV1222WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK80

Quant Time: Dec 23 01:06:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 23 01:05:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	691677	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	652194	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.26	152	298293	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	178316	35.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.90%
7) Chloroethane-d5	1.57	69	158221	40.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.90%
11) 1,1-Dichloroethene-d2	2.11	63	277307	30.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.24%
21) 2-Butanone-d5	3.89	46	335900	124.60	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	124.60%
24) Chloroform-d	4.35	84	387435	43.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.68%
26) 1,2-Dichloroethane-d4	5.04	65	275729	47.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.40%
32) Benzene-d6	5.05	84	763885	43.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.84%
36) 1,2-Dichloropropane-d6	6.07	67	252009	46.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.50%
41) Toluene-d8	7.32	98	658851	42.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.14%
43) trans-1,3-Dichloropropene-	7.62	79	119223	38.47	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.94%
47) 2-Hexanone-d5	8.09	63	206707	96.66	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.66%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	323478	43.89	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.78%
64) 1,2-Dichlorobenzene-d4	11.63	152	251223	45.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.10%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.25	75	42508	6.866 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122220\
Data File : VV019790.D
Acq On : 22 Dec 2020 10:55
Operator : SY/MD
Sample : VV1222WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK80

Quant Time: Dec 23 01:06:30 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 23 01:05:06 2020
Response via : Initial Calibration

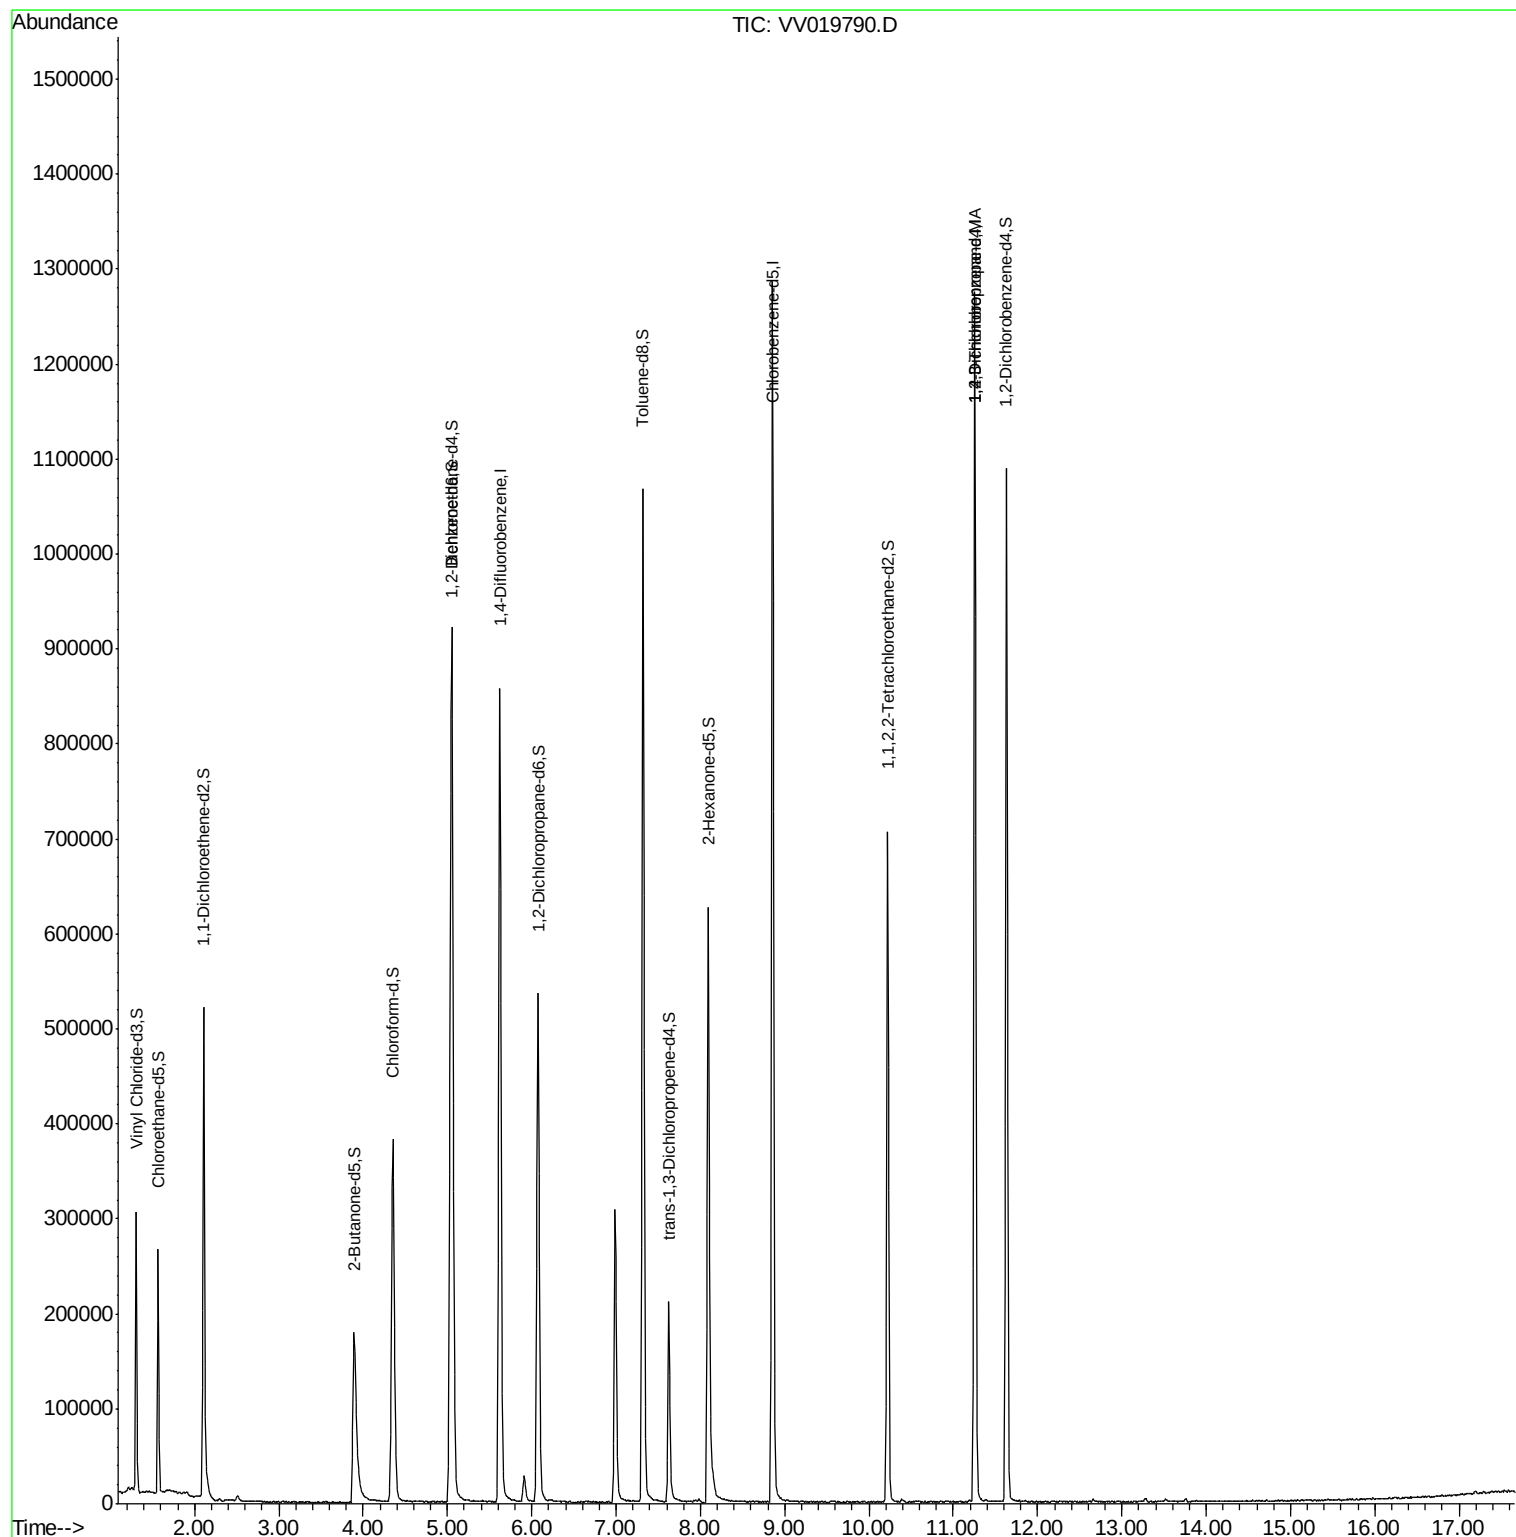

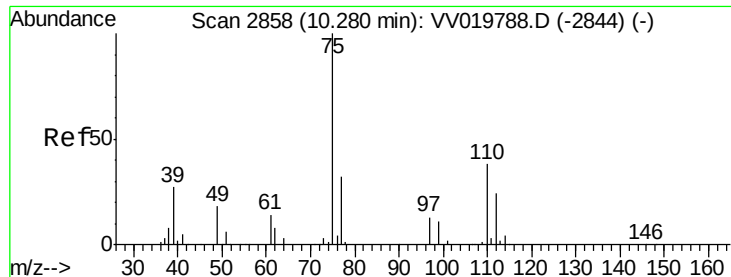

#59

1,2,3-Trichloropropane

Concen: 6.866 ug/L

RT: 11.25 min Scan# 3161

Delta R.T. 0.97 min

Lab File: VV019790.D

Acq: 22 Dec 2020 10:55

Instrument :

MSVOA_V

ClientSampleId :


VBLK80

Tot Ion: 75 Resp: 42508

Ion Ratio Lower Upper

75 100

77 37.5 25.8 38.8

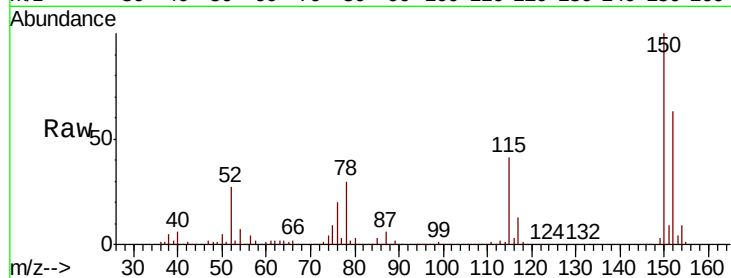

Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 77.00 (76.70 to 77.70): VV0

