

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019799.D
 Acq On : 22 Dec 2020 16:45
 Operator : SY/MD
 Sample : VIBLK76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	85	rVB	409876	418447	14.91%	1.947%
2	1.569	142	149	163	rVB	330907	373360	13.30%	1.737%
3	2.110	308	317	352	rVB	660164	1024358	36.49%	4.766%
4	2.566	457	459	464	rBV2	752	612	0.02%	0.003%
5	2.589	464	466	471	rVV3	765	559	0.02%	0.003%
6	2.782	523	526	529	rVB4	554	340	0.01%	0.002%
7	2.881	554	557	562	rBV6	1066	820	0.03%	0.004%
8	3.016	597	599	603	rBV3	516	369	0.01%	0.002%
9	3.113	626	629	632	rVB2	706	496	0.02%	0.002%
10	3.126	632	633	635	rBV	311	152	0.01%	0.001%
11	3.142	636	638	640	rVB2	760	334	0.01%	0.002%
12	3.155	640	642	647	rBV3	448	416	0.01%	0.002%
13	3.203	655	657	661	rBV4	622	519	0.02%	0.002%
14	3.270	675	678	681	rBV3	573	432	0.02%	0.002%
15	3.412	720	722	723	rBV	448	162	0.01%	0.001%
16	3.438	729	730	733	rBV3	437	194	0.01%	0.001%
17	3.479	741	743	745	rBV2	615	267	0.01%	0.001%
18	3.505	750	751	752	rBV2	451	145	0.01%	0.001%
19	3.515	752	754	757	rBV3	469	307	0.01%	0.001%
20	3.611	781	784	789	rBV3	841	808	0.03%	0.004%
21	3.656	794	798	802	rBV4	834	753	0.03%	0.004%
22	3.675	802	804	806	rBV3	520	279	0.01%	0.001%
23	3.727	819	820	824	rBV3	479	269	0.01%	0.001%
24	3.743	824	825	828	rVB	324	153	0.01%	0.001%
25	3.823	846	850	853	rBV3	729	652	0.02%	0.003%
26	3.846	853	857	860	rVB3	690	371	0.01%	0.002%
27	3.894	860	872	915	rBV	196516	633855	22.58%	2.949%
28	4.354	999	1015	1041	rBV	439868	1082410	38.56%	5.036%
29	4.872	1173	1176	1181	rBV5	667	467	0.02%	0.002%
30	4.894	1181	1183	1185	rVB3	731	313	0.01%	0.001%
31	4.907	1185	1187	1190	rBV2	643	361	0.01%	0.002%
32	4.923	1190	1192	1193	rBV2	452	158	0.01%	0.001%
33	4.991	1211	1213	1214	rBV	610	276	0.01%	0.001%
34	5.052	1214	1232	1262	rBV2	1087609	2807385	100.00%	13.061%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019799.D
 Acq On : 22 Dec 2020 16:45
 Operator : SY/MD
 Sample : VIBLK76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	5.572	1391	1394	1395	rBV3	677	406	0.01%	0.002%
36	5.621	1396	1409	1440	rVV	895053	1780805	63.43%	8.285%
37	5.910	1487	1499	1515	rBV3	34266	75855	2.70%	0.353%
38	6.074	1535	1550	1575	rBV	629831	1280621	45.62%	5.958%
39	6.441	1660	1664	1667	rBV3	990	811	0.03%	0.004%
40	6.476	1672	1675	1676	rBV2	605	333	0.01%	0.002%
41	6.582	1706	1708	1709	rBV2	317	137	0.00%	0.001%
42	6.672	1734	1736	1743	rVB6	1038	873	0.03%	0.004%
43	6.698	1743	1744	1748	rVB3	638	271	0.01%	0.001%
44	6.852	1787	1792	1794	rBV4	1143	908	0.03%	0.004%
45	6.929	1812	1816	1821	rBV6	1009	879	0.03%	0.004%
46	6.990	1821	1835	1863	rBV	353190	644597	22.96%	2.999%
47	7.264	1918	1920	1922	rVB3	770	310	0.01%	0.001%
48	7.322	1925	1938	1965	rVV	1262123	2192760	78.11%	10.201%
49	7.624	2022	2032	2059	rBV	240728	421707	15.02%	1.962%
50	7.865	2105	2107	2109	rBV2	720	396	0.01%	0.002%
51	7.984	2134	2144	2160	rVB3	13998	25773	0.92%	0.120%
52	8.039	2160	2161	2163	rBV	627	234	0.01%	0.001%
53	8.093	2167	2178	2217	rBV	685061	1292389	46.04%	6.013%
54	8.781	2390	2392	2394	rVB3	739	252	0.01%	0.001%
55	8.855	2403	2415	2438	rBV	1330735	2159145	76.91%	10.045%
56	9.460	2601	2603	2606	rVB5	1068	527	0.02%	0.002%
57	9.482	2606	2610	2611	rBV2	832	594	0.02%	0.003%
58	9.553	2629	2632	2636	rBV4	916	879	0.03%	0.004%
59	9.617	2648	2652	2654	rBV3	787	698	0.02%	0.003%
60	9.701	2674	2678	2679	rBV2	645	423	0.02%	0.002%
61	9.743	2689	2691	2694	rVB	464	244	0.01%	0.001%
62	9.762	2694	2697	2698	rBV3	630	248	0.01%	0.001%
63	9.781	2701	2703	2705	rBV2	723	362	0.01%	0.002%
64	9.926	2746	2748	2749	rBV2	532	147	0.01%	0.001%
65	9.936	2749	2751	2752	rBV2	434	147	0.01%	0.001%
66	10.084	2794	2797	2798	rBV2	649	363	0.01%	0.002%
67	10.106	2802	2804	2807	rVB4	853	458	0.02%	0.002%
68	10.125	2807	2810	2813	rBV2	841	489	0.02%	0.002%
69	10.145	2813	2816	2820	rBV3	773	648	0.02%	0.003%
70	10.222	2828	2840	2860	rBV	754995	1181134	42.07%	5.495%
71	10.383	2889	2890	2893	rBV3	524	288	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019799.D
 Acq On : 22 Dec 2020 16:45
 Operator : SY/MD
 Sample : VIBLK76
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.566	2945	2947	2949	rBV2	681	421	0.01%	0.002%
73	10.579	2949	2951	2953	rBV2	764	546	0.02%	0.003%
74	10.685	2982	2984	2988	rBV3	667	373	0.01%	0.002%
75	11.045	3094	3096	3097	rBV	728	226	0.01%	0.001%
76	11.077	3104	3106	3107	rBV	504	206	0.01%	0.001%
77	11.125	3117	3121	3122	rBV2	1049	609	0.02%	0.003%
78	11.254	3150	3161	3181	rBV	1388803	2121694	75.58%	9.871%
79	11.482	3230	3232	3238	rBV3	786	657	0.02%	0.003%
80	11.630	3267	3278	3307	rVB	1236299	1946921	69.35%	9.058%
81	12.013	3393	3397	3402	rBV5	1034	1103	0.04%	0.005%
82	12.251	3469	3471	3474	rBV4	856	554	0.02%	0.003%
83	12.373	3507	3509	3511	rBV3	851	396	0.01%	0.002%
84	12.476	3535	3541	3544	rBV5	1300	1661	0.06%	0.008%
85	12.829	3648	3651	3655	rVB4	1117	620	0.02%	0.003%
86	13.196	3762	3765	3767	rBV3	1085	879	0.03%	0.004%


Sum of corrected areas: 21494776

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122220\
Data File : VV019799.D
Acq On : 22 Dec 2020 16:45
Operator : SY/MD
Sample : VIBLK76
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

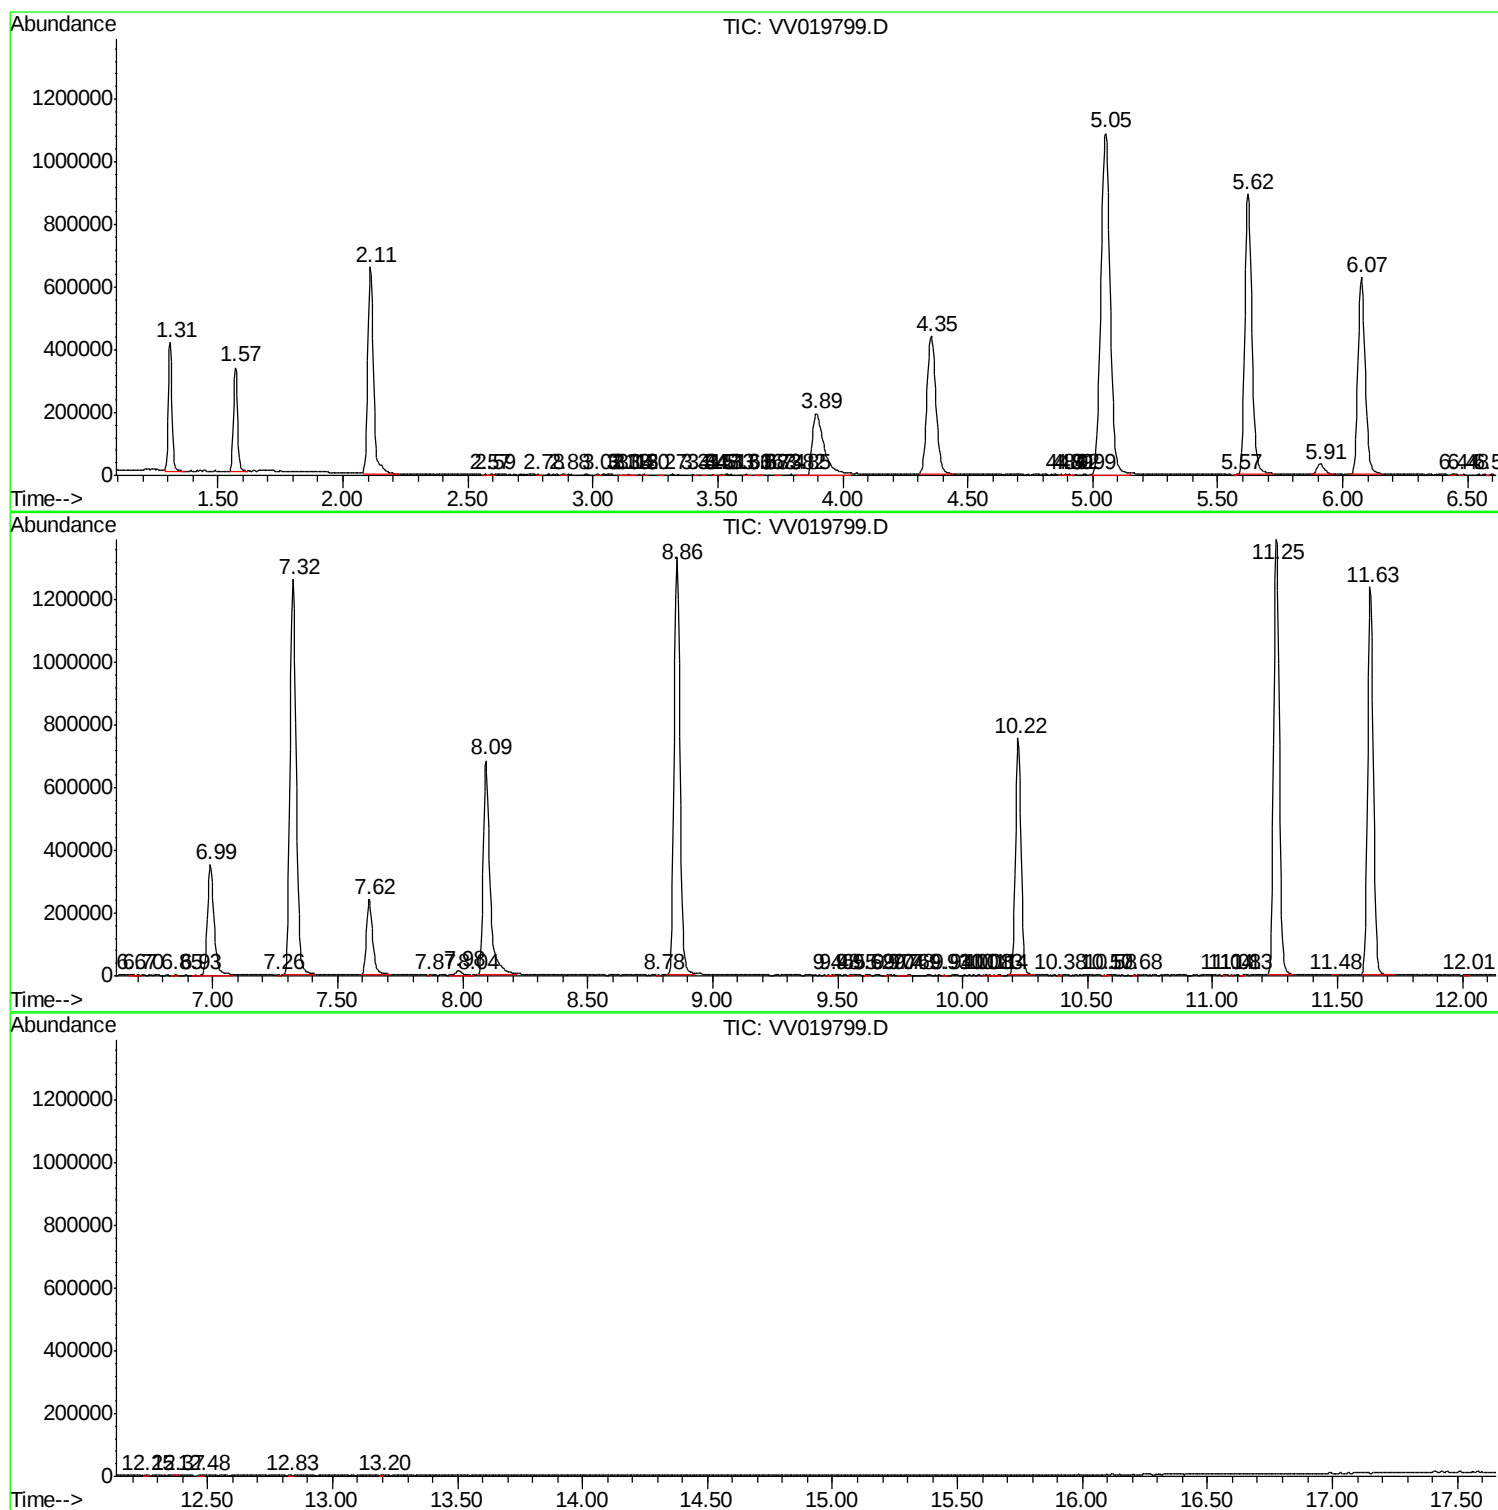

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122220\
Data File : VV019799.D
Acq On : 22 Dec 2020 16:45
Operator : SY/MD
Sample : VIBLK76
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122220\
Data File : VV019799.D
Acq On : 22 Dec 2020 16:45
Operator : SY/MD
Sample : VIBLK76
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc