

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019801.D
 Acq On : 22 Dec 2020 17:33
 Operator : SY/MD
 Sample : VIBLK77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	401789	407552	14.71%	1.917%
2	1.569	142	149	164	rBV	326138	365537	13.19%	1.719%
3	2.110	307	317	346	rVB	652953	999142	36.07%	4.700%
4	2.740	510	513	516	rBV4	740	484	0.02%	0.002%
5	2.762	517	520	525	rVV6	907	680	0.02%	0.003%
6	2.788	526	528	530	rVV3	662	216	0.01%	0.001%
7	2.823	537	539	541	rVB	288	95	0.00%	0.000%
8	2.843	541	545	548	rBV4	826	835	0.03%	0.004%
9	3.026	599	602	603	rBV	621	353	0.01%	0.002%
10	3.129	629	634	636	rBV3	724	720	0.03%	0.003%
11	3.142	636	638	641	rVB2	665	255	0.01%	0.001%
12	3.158	641	643	645	rBV2	877	507	0.02%	0.002%
13	3.206	656	658	661	rBV2	611	363	0.01%	0.002%
14	3.248	668	671	673	rBV3	518	220	0.01%	0.001%
15	3.303	683	688	693	rBV4	880	1035	0.04%	0.005%
16	3.325	693	695	697	rVB2	829	263	0.01%	0.001%
17	3.338	697	699	701	rVB2	609	247	0.01%	0.001%
18	3.364	705	707	709	rBV2	354	205	0.01%	0.001%
19	3.383	709	713	716	rBV4	976	713	0.03%	0.003%
20	3.444	730	732	734	rBV2	383	153	0.01%	0.001%
21	3.528	753	758	760	rBV	912	653	0.02%	0.003%
22	3.540	760	762	763	rBV	283	142	0.01%	0.001%
23	3.605	780	782	785	rBV2	617	310	0.01%	0.001%
24	3.624	785	788	789	rVV2	541	355	0.01%	0.002%
25	3.634	789	791	795	rVB3	1128	455	0.02%	0.002%
26	3.672	800	803	805	rBV	477	283	0.01%	0.001%
27	3.717	814	817	821	rVB3	752	552	0.02%	0.003%
28	3.737	821	823	824	rBV	755	275	0.01%	0.001%
29	3.762	829	831	832	rBV	425	132	0.00%	0.001%
30	3.814	845	847	849	rVB2	590	179	0.01%	0.001%
31	3.830	851	852	854	rBV2	350	129	0.00%	0.001%
32	3.843	854	856	858	rBV2	866	474	0.02%	0.002%
33	3.894	861	872	915	rBV	191740	627947	22.67%	2.954%
34	4.354	993	1015	1040	rBV	431435	1070813	38.65%	5.037%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019801.D
 Acq On : 22 Dec 2020 17:33
 Operator : SY/MD
 Sample : VIBLK77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	4.794	1150	1152	1155	rBV2	522	310	0.01%	0.001%
36	4.807	1155	1156	1157	rBV	554	154	0.01%	0.001%
37	4.839	1163	1166	1168	rBV3	855	519	0.02%	0.002%
38	4.878	1176	1178	1179	rBV2	536	184	0.01%	0.001%
39	4.920	1187	1191	1192	rBV4	471	362	0.01%	0.002%
40	5.052	1214	1232	1269	rBV2	1070737	2770391	100.00%	13.032%
41	5.621	1396	1409	1441	rBV	895664	1786707	64.49%	8.404%
42	5.910	1491	1499	1514	rVB	31492	60710	2.19%	0.286%
43	6.074	1536	1550	1576	rBV	618806	1259010	45.45%	5.922%
44	6.296	1617	1619	1621	rVB2	1458	578	0.02%	0.003%
45	6.470	1671	1673	1674	rBV2	600	243	0.01%	0.001%
46	6.502	1681	1683	1685	rBV2	452	193	0.01%	0.001%
47	6.515	1685	1687	1691	rVB4	888	623	0.02%	0.003%
48	6.544	1694	1696	1697	rBV	436	149	0.01%	0.001%
49	6.553	1697	1699	1700	rVB2	431	122	0.00%	0.001%
50	6.589	1708	1710	1713	rVB3	573	308	0.01%	0.001%
51	6.765	1761	1765	1770	rBV7	881	862	0.03%	0.004%
52	6.843	1787	1789	1791	rBV	790	407	0.01%	0.002%
53	6.917	1809	1812	1815	rBV5	694	552	0.02%	0.003%
54	6.990	1823	1835	1861	rBV	345245	623495	22.51%	2.933%
55	7.318	1924	1937	1969	rBV	1229678	2163979	78.11%	10.179%
56	7.624	2022	2032	2061	rBV	236059	414372	14.96%	1.949%
57	7.984	2135	2144	2150	rBV8	7231	13174	0.48%	0.062%
58	8.093	2167	2178	2207	rBV	679322	1265812	45.69%	5.954%
59	8.855	2403	2415	2441	rBV	1339375	2178332	78.63%	10.247%
60	9.267	2539	2543	2545	rBV4	1030	817	0.03%	0.004%
61	9.360	2570	2572	2577	rVB5	662	552	0.02%	0.003%
62	9.434	2592	2595	2596	rBV	476	245	0.01%	0.001%
63	9.672	2665	2669	2671	rBV4	859	767	0.03%	0.004%
64	9.714	2678	2682	2685	rBV3	842	585	0.02%	0.003%
65	9.820	2713	2715	2716	rBV2	634	233	0.01%	0.001%
66	10.222	2824	2840	2864	rBV	743490	1164586	42.04%	5.478%
67	10.402	2892	2896	2898	rBV5	596	423	0.02%	0.002%
68	10.498	2925	2926	2927	rBV	542	137	0.00%	0.001%
69	10.572	2947	2949	2951	rBV3	848	473	0.02%	0.002%
70	10.785	3010	3015	3016	rBV4	813	725	0.03%	0.003%
71	10.839	3030	3032	3033	rBV	588	251	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122220\
 Data File : VV019801.D
 Acq On : 22 Dec 2020 17:33
 Operator : SY/MD
 Sample : VIBLK77
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.878	3042	3044	3047	rBV3	630	340	0.01%	0.002%
73	10.923	3056	3058	3059	rBV	520	187	0.01%	0.001%
74	10.942	3062	3064	3065	rBV2	402	129	0.00%	0.001%
75	10.974	3072	3074	3079	rVB3	757	494	0.02%	0.002%
76	11.000	3079	3082	3083	rBV2	619	347	0.01%	0.002%
77	11.029	3088	3091	3094	rVB3	718	440	0.02%	0.002%
78	11.071	3101	3104	3105	rBV2	650	427	0.02%	0.002%
79	11.116	3116	3118	3121	rVB2	1067	516	0.02%	0.002%
80	11.135	3121	3124	3134	rBV6	1138	1510	0.05%	0.007%
81	11.254	3148	3161	3188	rBV	1408046	2151017	77.64%	10.118%
82	11.498	3232	3237	3241	rBV5	1494	1714	0.06%	0.008%
83	11.630	3266	3278	3296	rBV	1207112	1905857	68.79%	8.965%
84	11.984	3386	3388	3392	rBV3	1026	626	0.02%	0.003%
85	12.045	3404	3407	3408	rBV2	822	426	0.02%	0.002%
86	12.338	3495	3498	3502	rBV3	869	896	0.03%	0.004%
87	13.032	3712	3714	3717	rBV4	682	300	0.01%	0.001%
88	13.556	3875	3877	3878	rBV2	934	296	0.01%	0.001%


Sum of corrected areas: 21259138

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122220\
Data File : VV019801.D
Acq On : 22 Dec 2020 17:33
Operator : SY/MD
Sample : VIBLK77
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

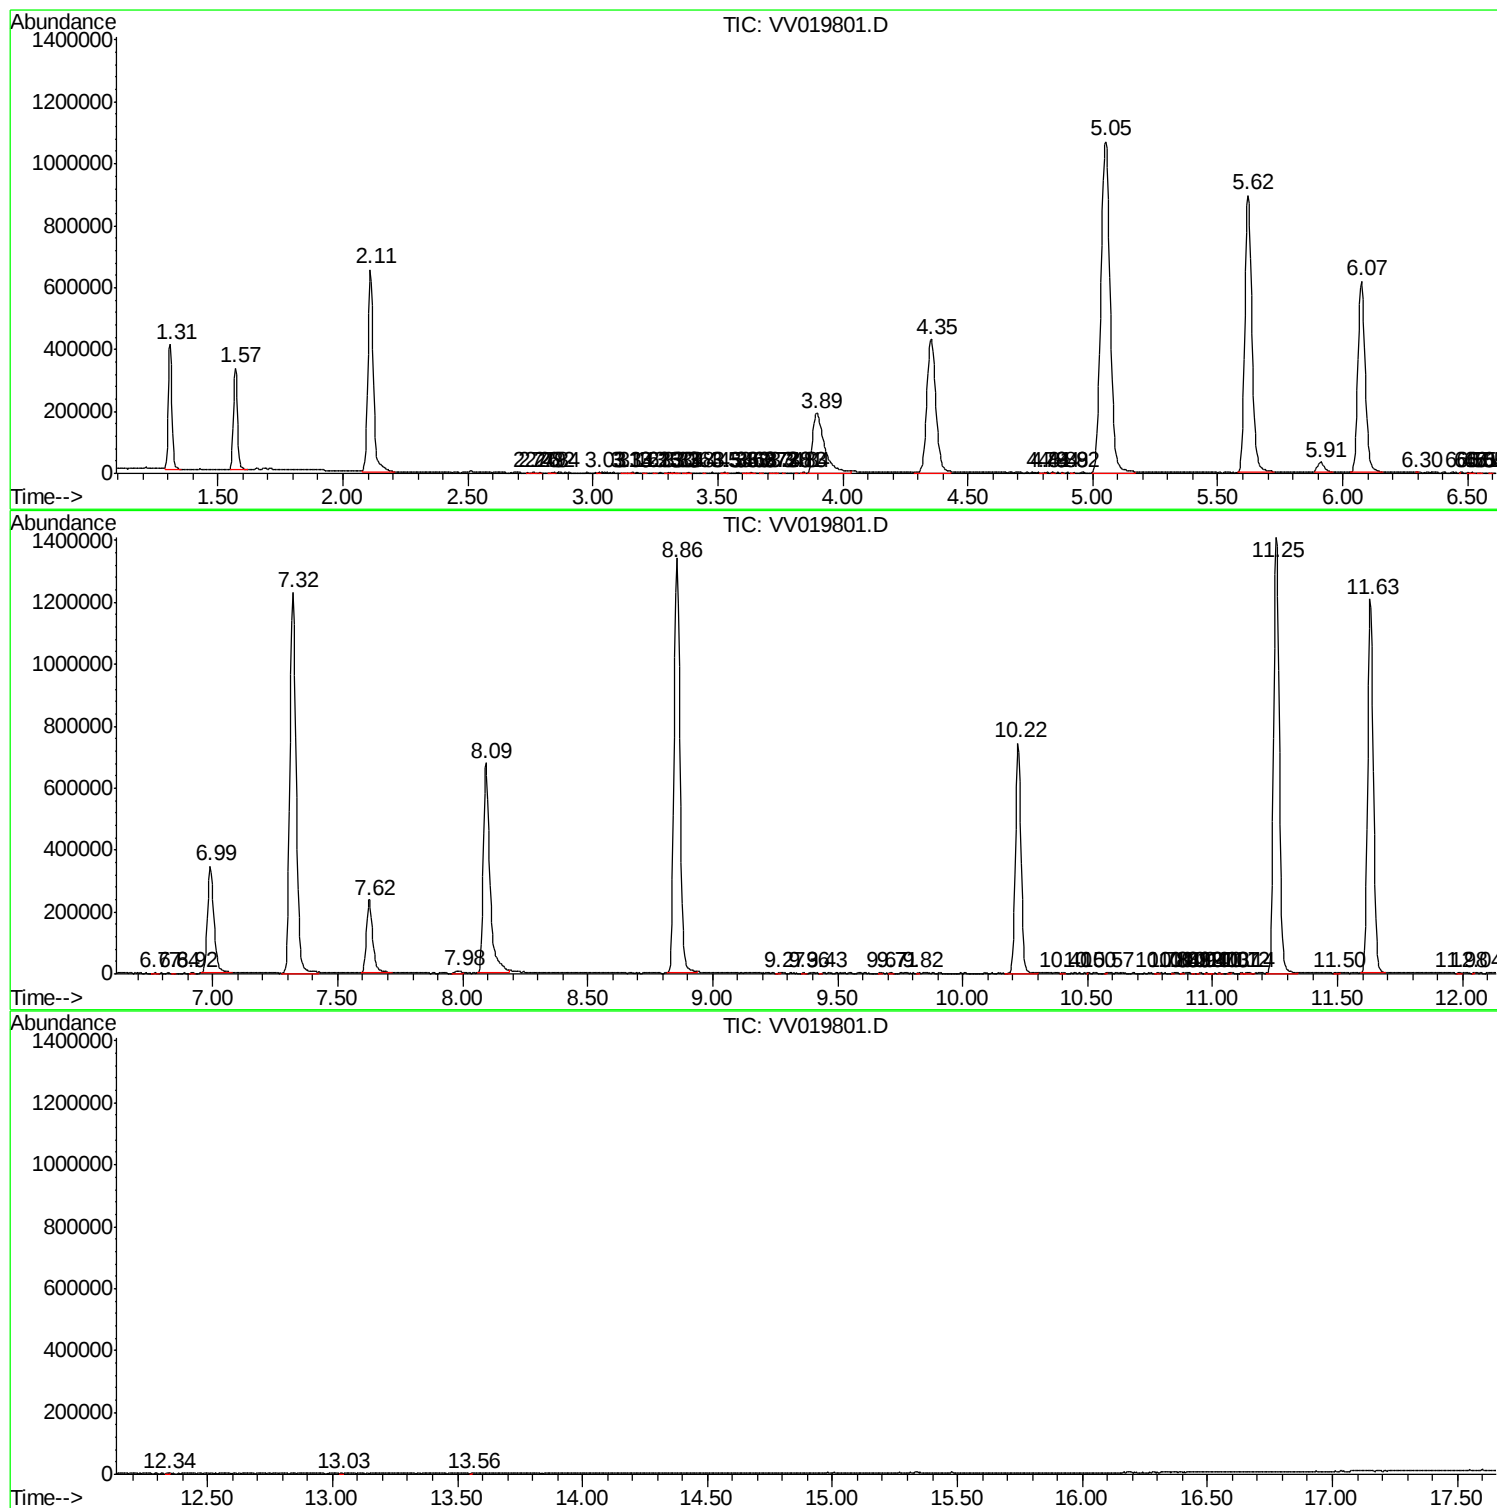

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122220\
Data File : VV019801.D
Acq On : 22 Dec 2020 17:33
Operator : SY/MD
Sample : VIBLK77
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122220\
Data File : VV019801.D
Acq On : 22 Dec 2020 17:33
Operator : SY/MD
Sample : VIBLK77
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc