


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV122220\
 Data File : VV019787.D
 Acq On : 22 Dec 2020 09:06
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 23 08:29:21 2020

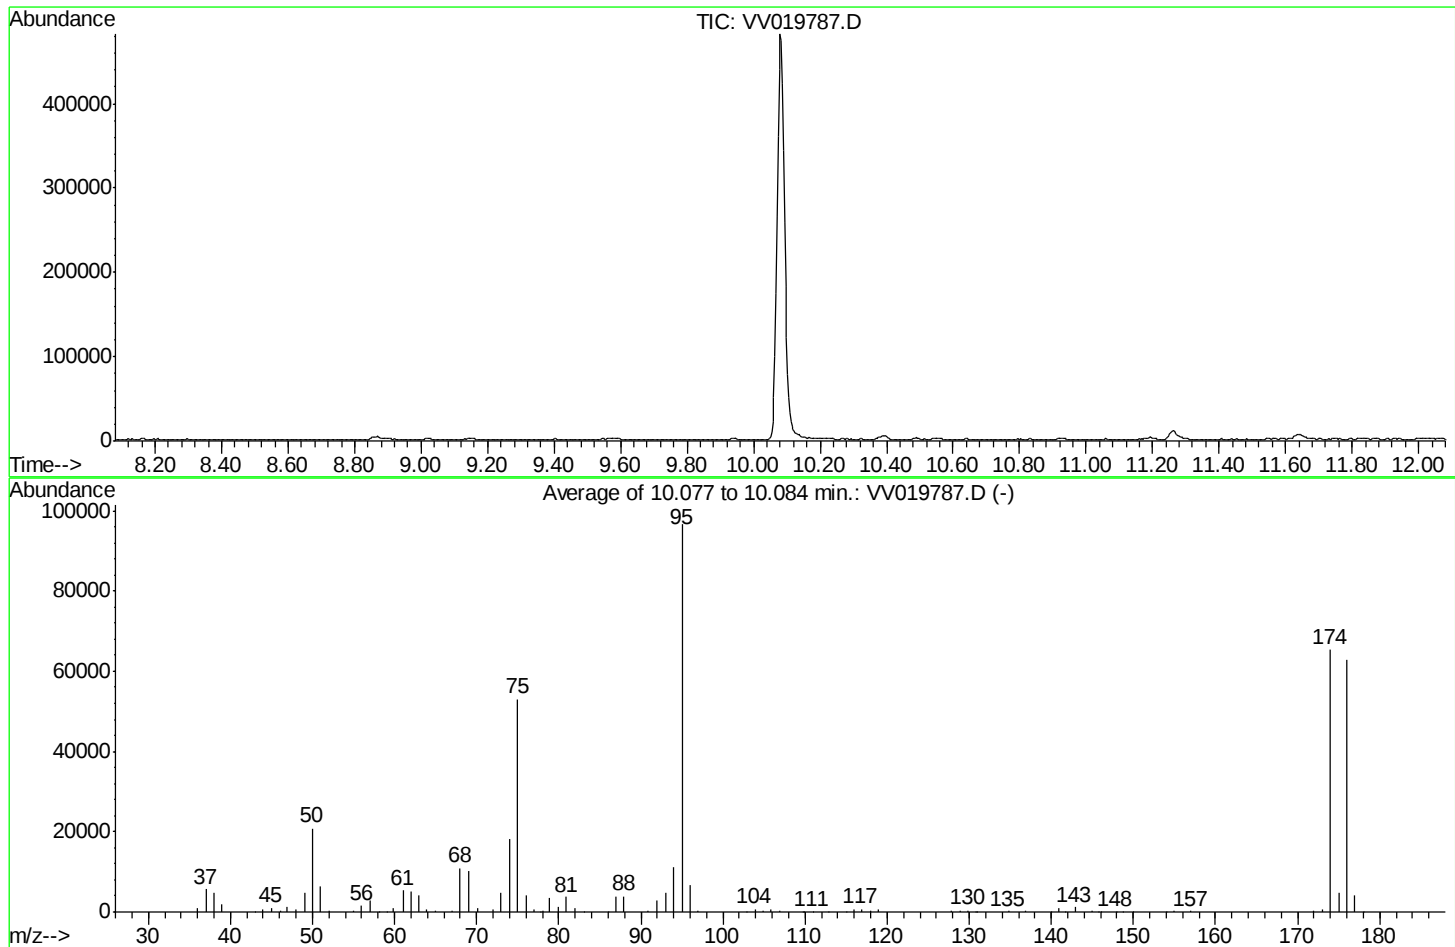

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	20856	PASS
75	95	30	80	54.8	52970	PASS
95	95	100	100	100.0	96602	PASS
96	95	5	9	6.9	6694	PASS
173	174	0.00	2	1.2	789	PASS
174	95	50	120	67.6	65344	PASS
175	174	5	9	7.5	4901	PASS
176	174	95	101	96.1	62792	PASS
177	176	5	9	6.5	4077	PASS

m/z	Abundance
36.00	1041.0
37.00	5349.0
38.00	4521.0
39.00	2140.0
39.90	330.0
43.10	143.0
44.00	1474.0
45.00	1140.0
46.10	214.0
47.00	1358.0
48.00	622.0
49.00	4476.0
50.00	19888.0
51.00	6433.0
52.00	291.0
55.00	406.0
56.00	1374.0
57.00	2856.0
58.00	192.0
59.90	1045.0
61.00	5097.0
62.00	4806.0
63.00	3887.0
63.90	595.0
64.90	303.0
67.00	221.0
68.00	10390.0
69.00	10091.0
70.00	842.0
71.90	631.0
73.00	4243.0
74.00	17176.0
75.00	50800.0
76.00	4241.0
77.00	645.0
78.10	383.0
78.90	3426.0
79.90	1275.0
80.90	3594.0
81.90	950.0
83.00	112.0
86.00	188.0
86.90	3434.0
87.90	3788.0
90.90	396.0
92.00	2718.0
93.00	4255.0
94.00	10658.0
95.00	91736.0
96.00	6552.0
97.00	242.0
102.80	147.0
103.90	626.0
104.90	215.0
105.90	486.0
107.00	211.0
110.90	117.0
112.80	115.0
114.90	120.0
115.90	467.0
116.90	593.0
118.00	440.0
118.90	589.0
127.90	335.0
129.00	257.0
129.80	386.0
130.80	159.0
134.70	221.0
136.90	221.0
140.00	107.0
140.90	1066.0
142.90	1166.0
144.90	213.0
147.90	128.0
154.00	101.0
155.00	208.0
157.00	248.0
171.90	369.0
173.00	669.0
174.00	60120.0
175.00	4620.0
176.00	58120.0
177.00	3835.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	1097.0
37.00	5900.0
38.00	4997.0
39.00	2216.0
39.90	231.0
43.10	151.0
44.00	1535.0
45.00	1161.0
46.10	211.0
46.90	1389.0
48.10	640.0
49.00	4894.0
50.00	21664.0
51.00	6847.0
52.00	303.0
55.00	388.0
56.00	1649.0
57.00	3072.0
58.10	171.0
59.00	100.0
59.90	1038.0
61.00	5584.0
62.00	5244.0
63.00	4222.0
63.90	655.0
64.90	379.0
66.90	233.0
68.00	11418.0
69.00	10626.0
70.10	942.0
72.00	749.0
73.00	4865.0
74.00	19016.0
75.00	54776.0
76.00	4393.0
77.00	675.0
78.10	348.0
78.90	3794.0
79.90	1367.0
80.90	3896.0
81.90	1030.0
83.00	118.0
86.00	171.0
86.90	3922.0
87.90	4061.0
90.90	426.0
92.00	2857.0
93.00	4880.0
94.00	11640.0
95.00	100208.0
96.00	6966.0
97.00	270.0
102.80	133.0
103.90	716.0
104.80	226.0
105.90	514.0
107.00	226.0
109.70	103.0
110.90	120.0
112.80	128.0
115.00	144.0
115.90	526.0
116.90	665.0
117.90	507.0
118.90	660.0
127.80	425.0
128.90	287.0
129.80	457.0
130.80	138.0
134.80	244.0
136.90	230.0
139.90	126.0
140.90	1180.0
141.70	125.0
142.90	1243.0
144.90	278.0
145.70	106.0
146.10	116.0
147.80	147.0
154.00	109.0
155.00	238.0
157.00	298.0
171.90	436.0
172.90	809.0
174.00	67544.0
175.00	5019.0
176.00	64824.0
176.90	4179.0
178.00	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	1061.0
37.00	5771.0
38.00	4891.0
39.00	2025.0
40.00	231.0
43.00	178.0
44.00	1605.0
45.00	1157.0
46.10	191.0
46.90	1251.0
48.00	544.0
49.00	4746.0
50.00	21016.0
51.00	6571.0
52.00	276.0
55.00	316.0
56.00	1731.0
57.00	3010.0
58.20	147.0
59.90	947.0
61.00	5466.0
62.00	5204.0
63.00	3913.0
63.90	579.0
64.90	402.0
66.90	263.0
68.00	11204.0
69.00	10043.0
70.00	922.0
72.00	676.0
73.00	4918.0
74.00	18712.0
75.00	53336.0
76.00	4146.0
77.00	509.0
77.80	279.0
78.90	3702.0
79.90	1321.0
80.90	3878.0
81.90	964.0
86.00	142.0
86.90	3969.0
88.00	3780.0
90.90	443.0
92.00	2781.0
93.00	4942.0
94.00	11699.0
95.00	97864.0
96.00	6565.0
97.00	232.0
103.90	649.0
104.80	210.0
105.90	514.0
106.90	188.0
109.90	120.0
110.90	111.0
112.80	114.0
115.00	177.0
115.90	505.0
116.90	702.0
117.90	522.0
118.90	592.0
127.80	445.0
128.80	266.0
129.90	485.0
131.00	142.0
134.80	232.0
136.90	218.0
139.90	170.0
140.90	1099.0
141.80	124.0
142.90	1180.0
144.90	273.0
145.90	161.0
147.80	183.0
148.70	137.0
150.00	105.0
154.90	231.0
157.00	292.0
172.00	470.0
172.90	891.0
174.00	68368.0
175.00	5065.0
176.00	65432.0
176.90	4219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Scan 2784 (10.042 min): VV019787.D
BFB71

m/z	Abundance
38.30	113.0
38.90	130.0
40.00	364.0
40.90	115.0
44.00	799.0
44.90	111.0
50.90	120.0
106.40	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71