

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024132.D
 Acq On : 22 Dec 2021 11:19
 Operator : SY/MD
 Sample : VV1222WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 23 06:12:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.615	114	9843	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.848	117	9673	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	5504	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.303	65	4938	0.451	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	90.000%
4) 1,2-Dichloroethane-d4	5.019	65	3767	0.534	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
7) 1,2-Dichloropropane-d6	6.069	67	3647	0.512	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	102.000%
8) Toluene-d8	7.317	98	12883	0.508	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.199	84	2411	0.531	ug/L	-0.02
Spiked Amount	0.500	Range	65 - 120	Recovery	=	106.000%
Target Compounds						
3) Vinyl chloride	1.303	62	103	0.011	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024132.D
Acq On : 22 Dec 2021 11:19
Operator : SY/MD
Sample : VV1222WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 23 06:12:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

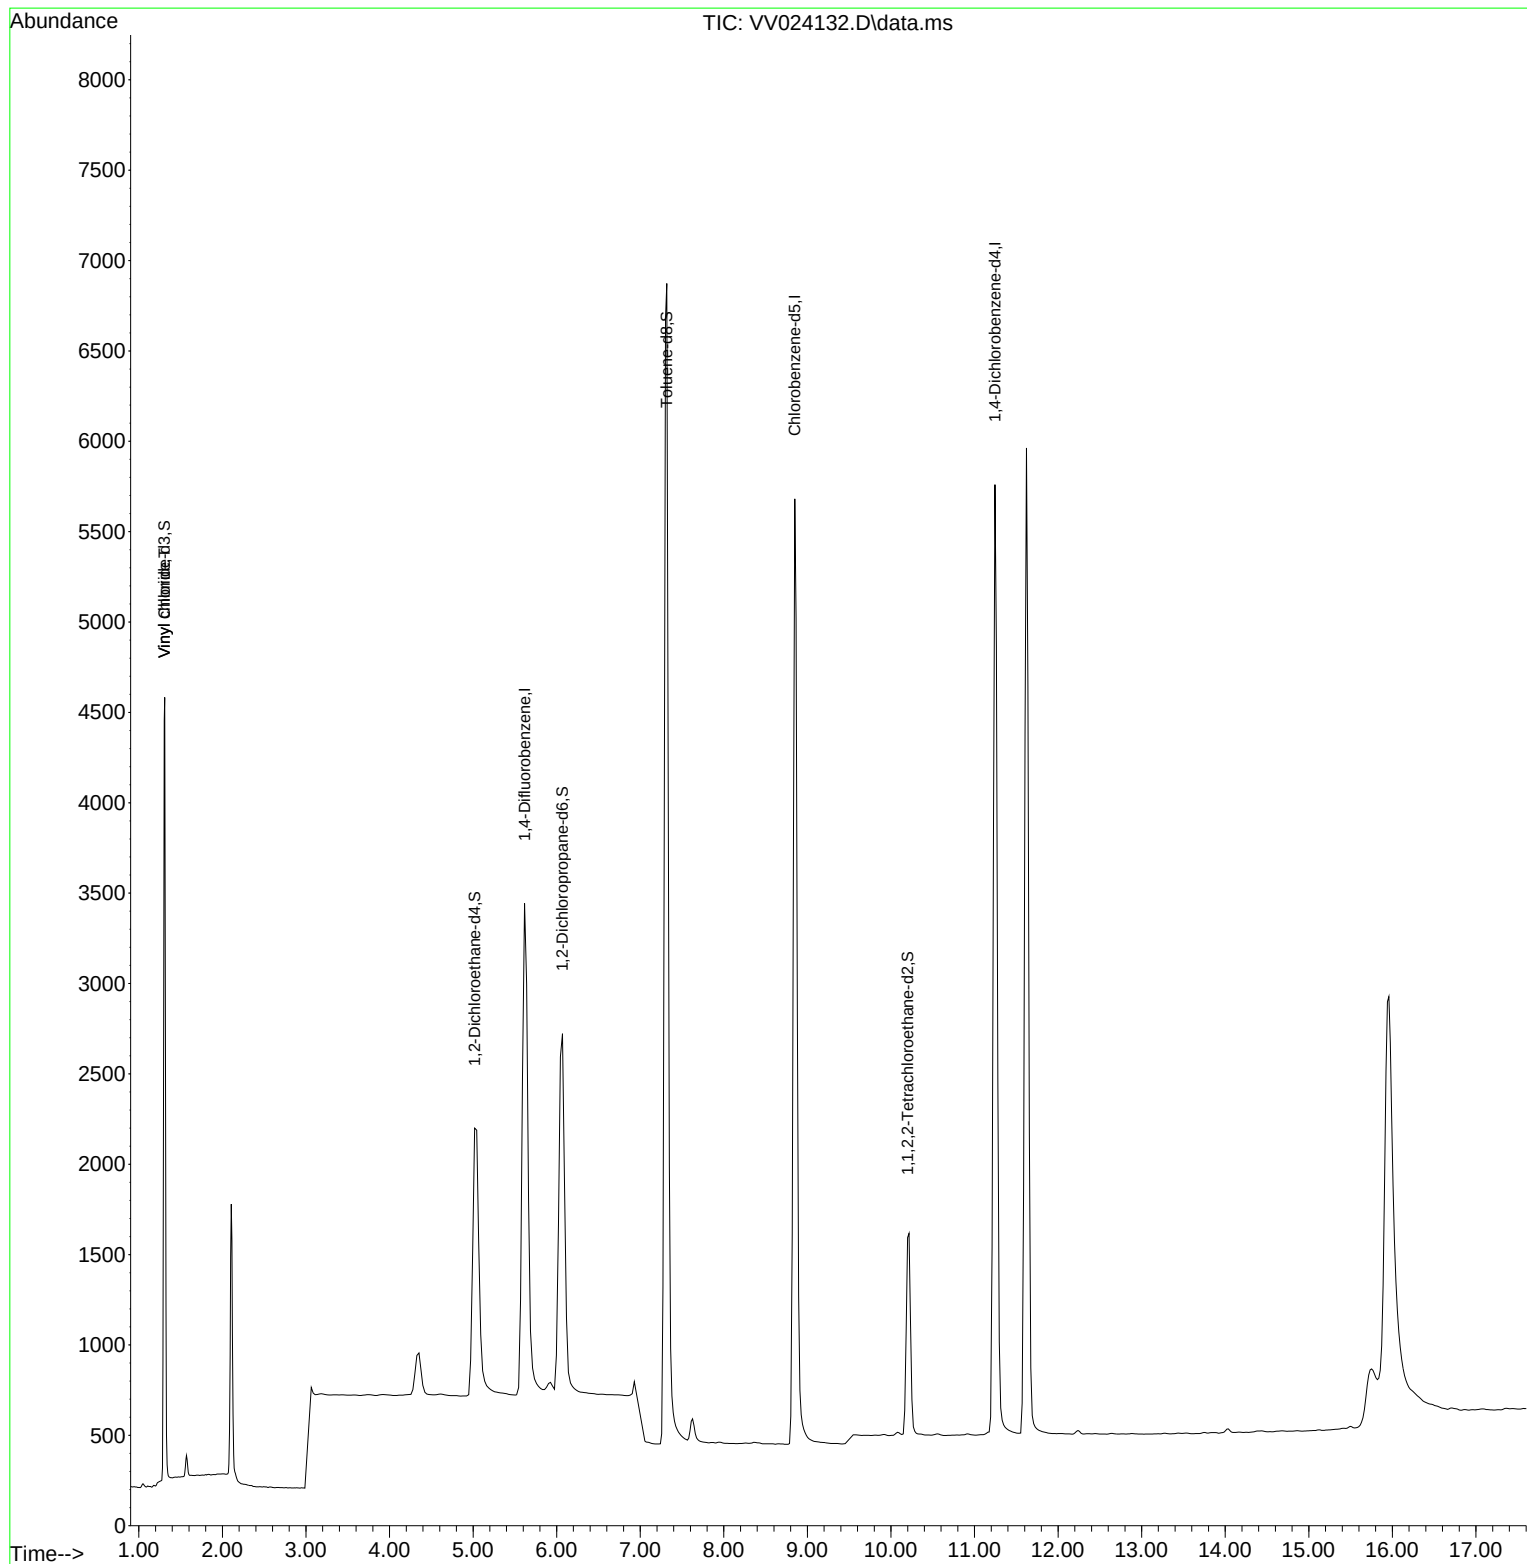

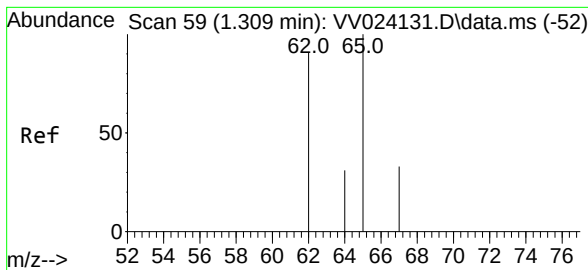

#3
Vinyl chloride
Concen: 0.011 ug/L
RT: 1.303 min Scan# 51
Delta R.T. -0.006 min
Lab File: VV024132.D
Acq: 22 Dec 2021 11:19

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 62 Resp: 103
Ion Ratio Lower Upper
62 100
64 134.1 25.3 46.9#

