

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024137.D
 Acq On : 22 Dec 2021 13:48
 Operator : SY/MD
 Sample : M5090-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 23 06:13:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7607	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.863	117	7442	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	4364	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	3825	0.452	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	90.000%		
4) 1,2-Dichloroethane-d4	5.042	65	2770	0.509	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
7) 1,2-Dichloropropane-d6	6.068	67	2840	0.518	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	104.000%		
8) Toluene-d8	7.317	98	9780	0.501	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	100.000%		
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1745	0.500	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	100.000%		
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.310	62	82	0.012	ug/L #	1
12) 1,2,3-Trichloropropane	10.370	75	86	0.030	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024137.D
Acq On : 22 Dec 2021 13:48
Operator : SY/MD
Sample : M5090-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 23 06:13:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

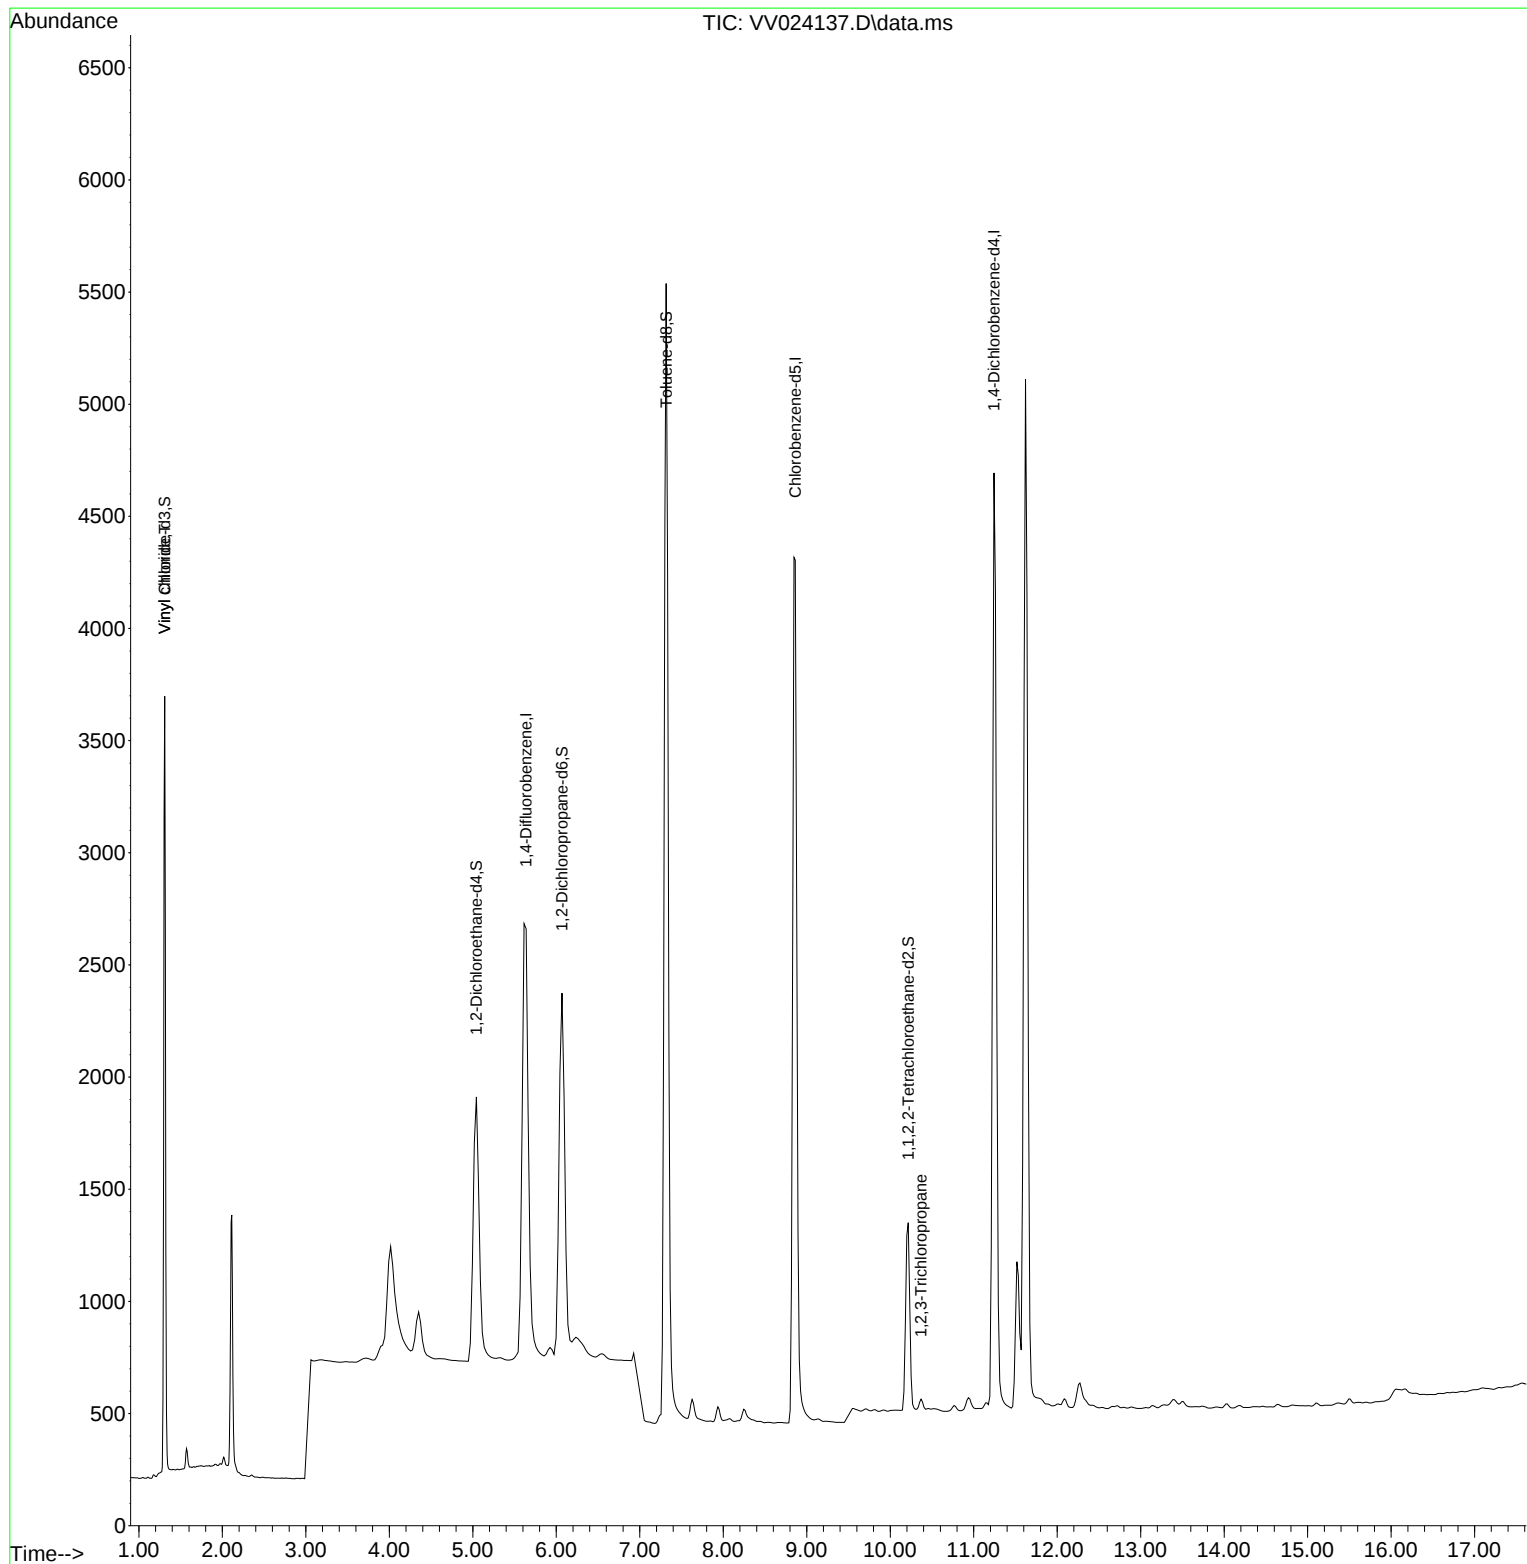

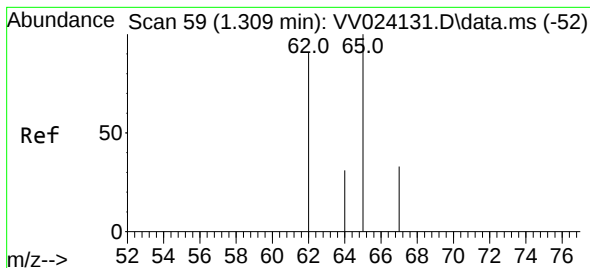

#3

Vinyl chloride

Concen: 0.012 ug/L

RT: 1.310 min Scan# 59

Delta R.T. 0.000 min

Lab File: VV024137.D

Acq: 22 Dec 2021 13:48

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 62 Resp: 82

Ion Ratio Lower Upper

62 100

64 131.2 25.3 46.9#

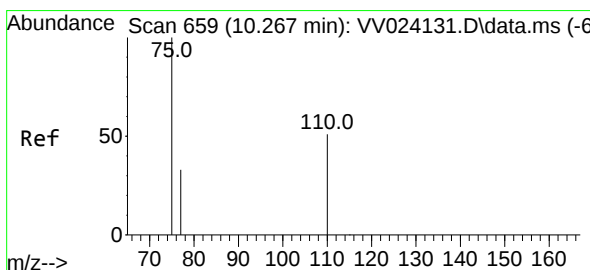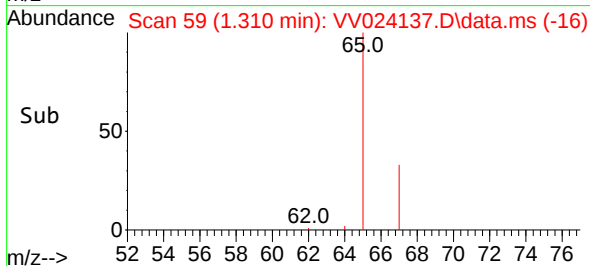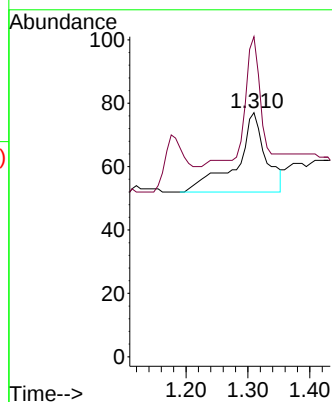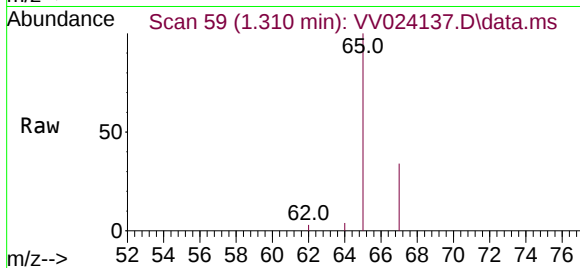

#12

1,2,3-Trichloropropane

Concen: 0.030 ug/L

RT: 10.370 min Scan# 665

Delta R.T. 0.103 min

Lab File: VV024137.D

Acq: 22 Dec 2021 13:48

Tgt Ion: 75 Resp: 86

Ion Ratio Lower Upper

75 100

110 36.0 38.2 57.4#

77 31.4 27.8 41.6

