

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024139.D
 Acq On : 22 Dec 2021 14:36
 Operator : SY/MD
 Sample : M5090-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 23 06:13:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7742	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.864	117	7584	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	4376	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	3819	0.444	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	88.000%
4) 1,2-Dichloroethane-d4	5.043	65	2822	0.509	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
7) 1,2-Dichloropropane-d6	6.069	67	2922	0.523	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.317	98	9847	0.495	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1790	0.503	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	100.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.238	75	123	0.215	ug/L	Qvalue # 46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024139.D
Acq On : 22 Dec 2021 14:36
Operator : SY/MD
Sample : M5090-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 23 06:13:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

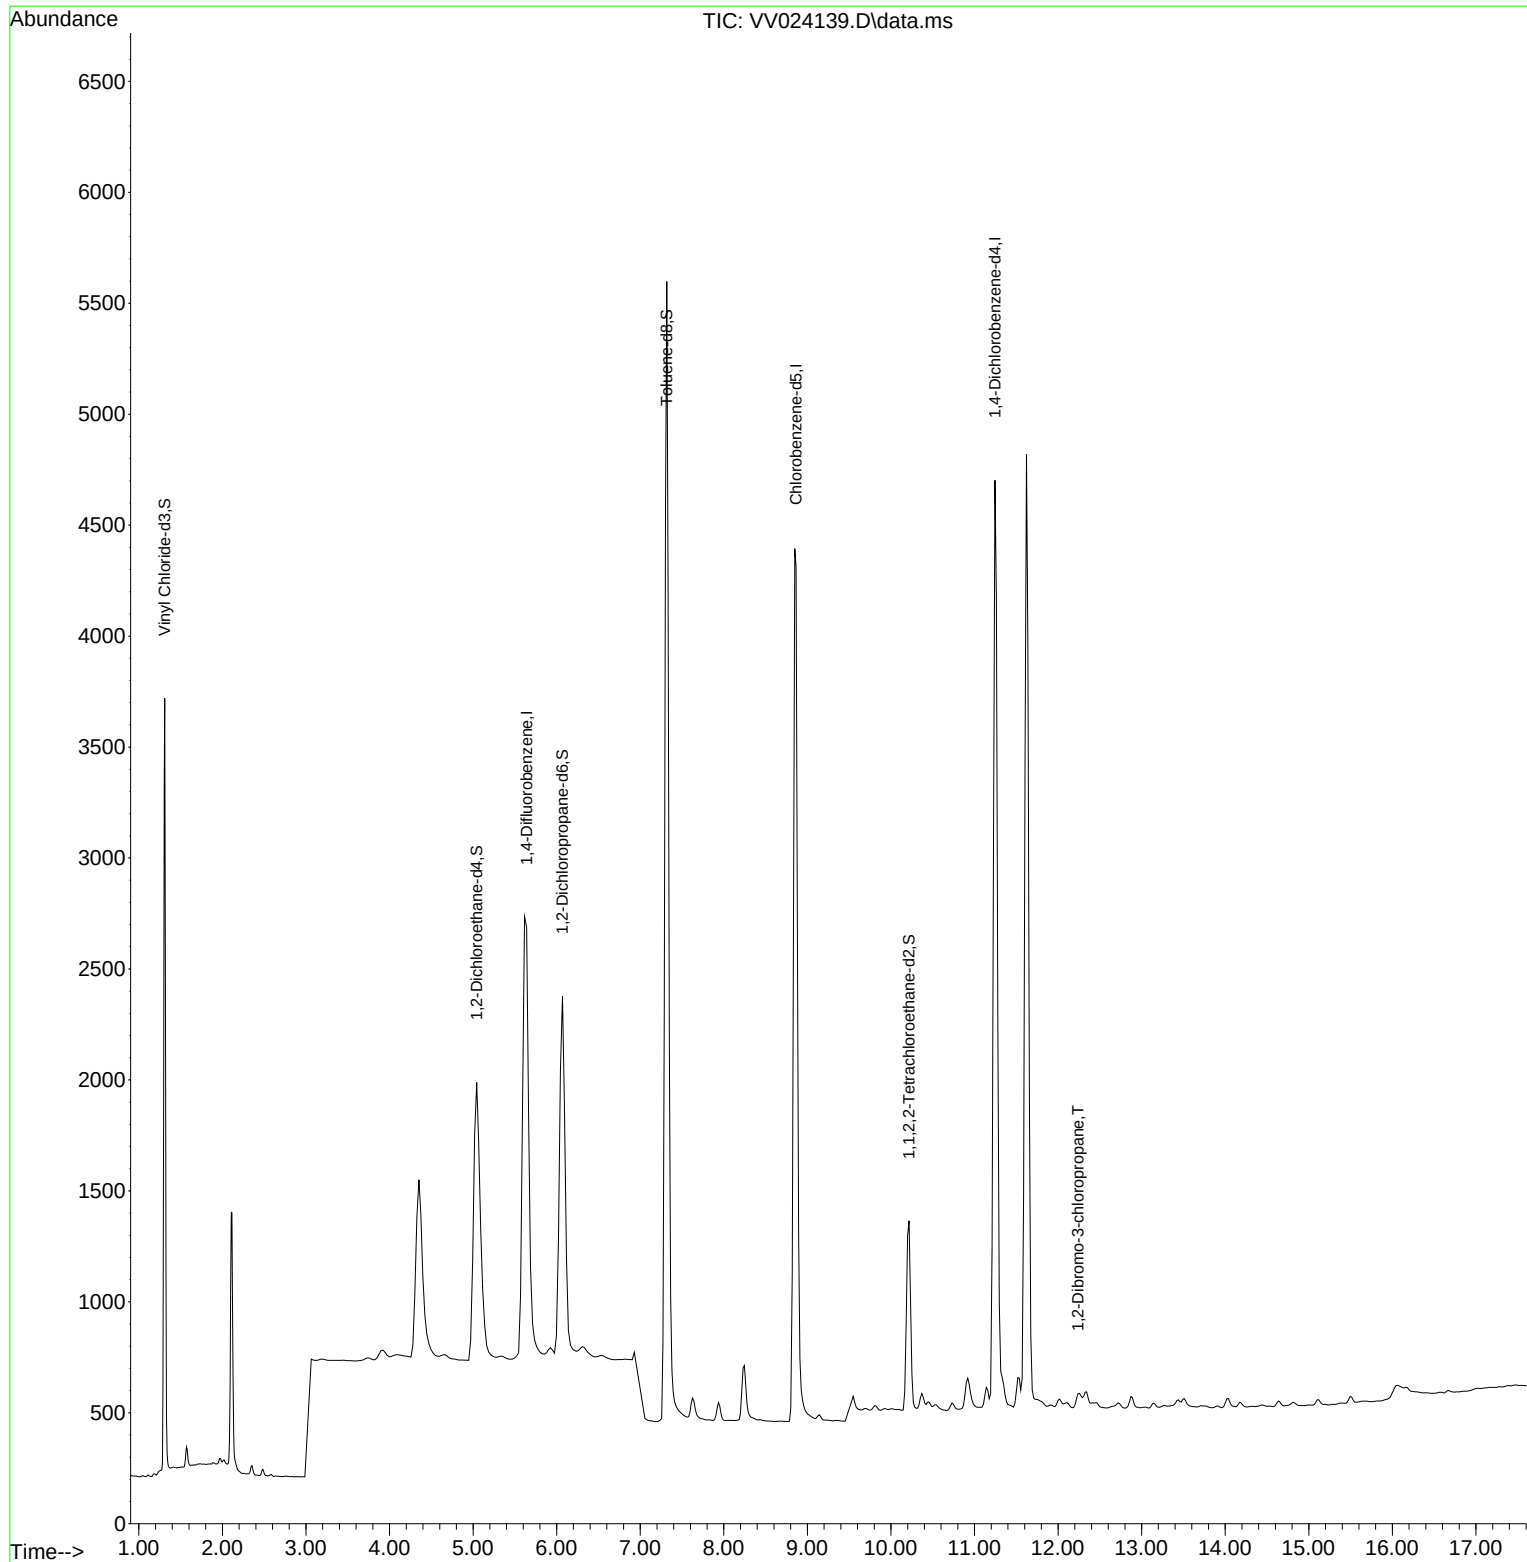

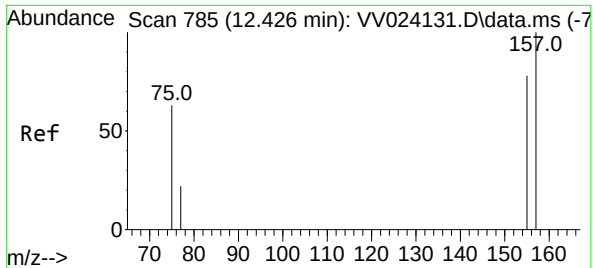

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.215 ug/L
 RT: 12.238 min Scan# 71
 Delta R.T. -0.188 min
 Lab File: VV024139.D
 Acq: 22 Dec 2021 14:36

Instrument :
 MSVOA_V
 ClientSampleId :

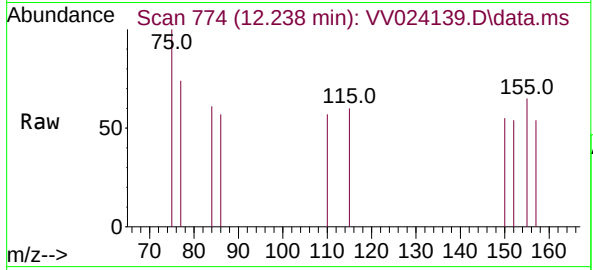

Tgt Ion:	75	Resp:	123
Ion	Ratio	Lower	Upper
75	100		
157	54.3	102.9	154.3#
155	65.2	87.6	131.4#

