

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024148.D
 Acq On : 22 Dec 2021 18:11
 Operator : SY/MD
 Sample : M5152-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 23 06:14:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	11214	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.864	117	11081	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	6038	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	5588	0.448	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	90.000%
4) 1,2-Dichloroethane-d4	5.042	65	4563	0.568	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	114.000%
7) 1,2-Dichloropropane-d6	6.069	67	5424	0.665	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	132.000%
8) Toluene-d8	7.317	98	15113	0.520	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	3232	0.622	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	124.000%#
Target Compounds						
12) 1,2,3-Trichloropropane	10.370	75	94	0.024	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024148.D
Acq On : 22 Dec 2021 18:11
Operator : SY/MD
Sample : M5152-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 23 06:14:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

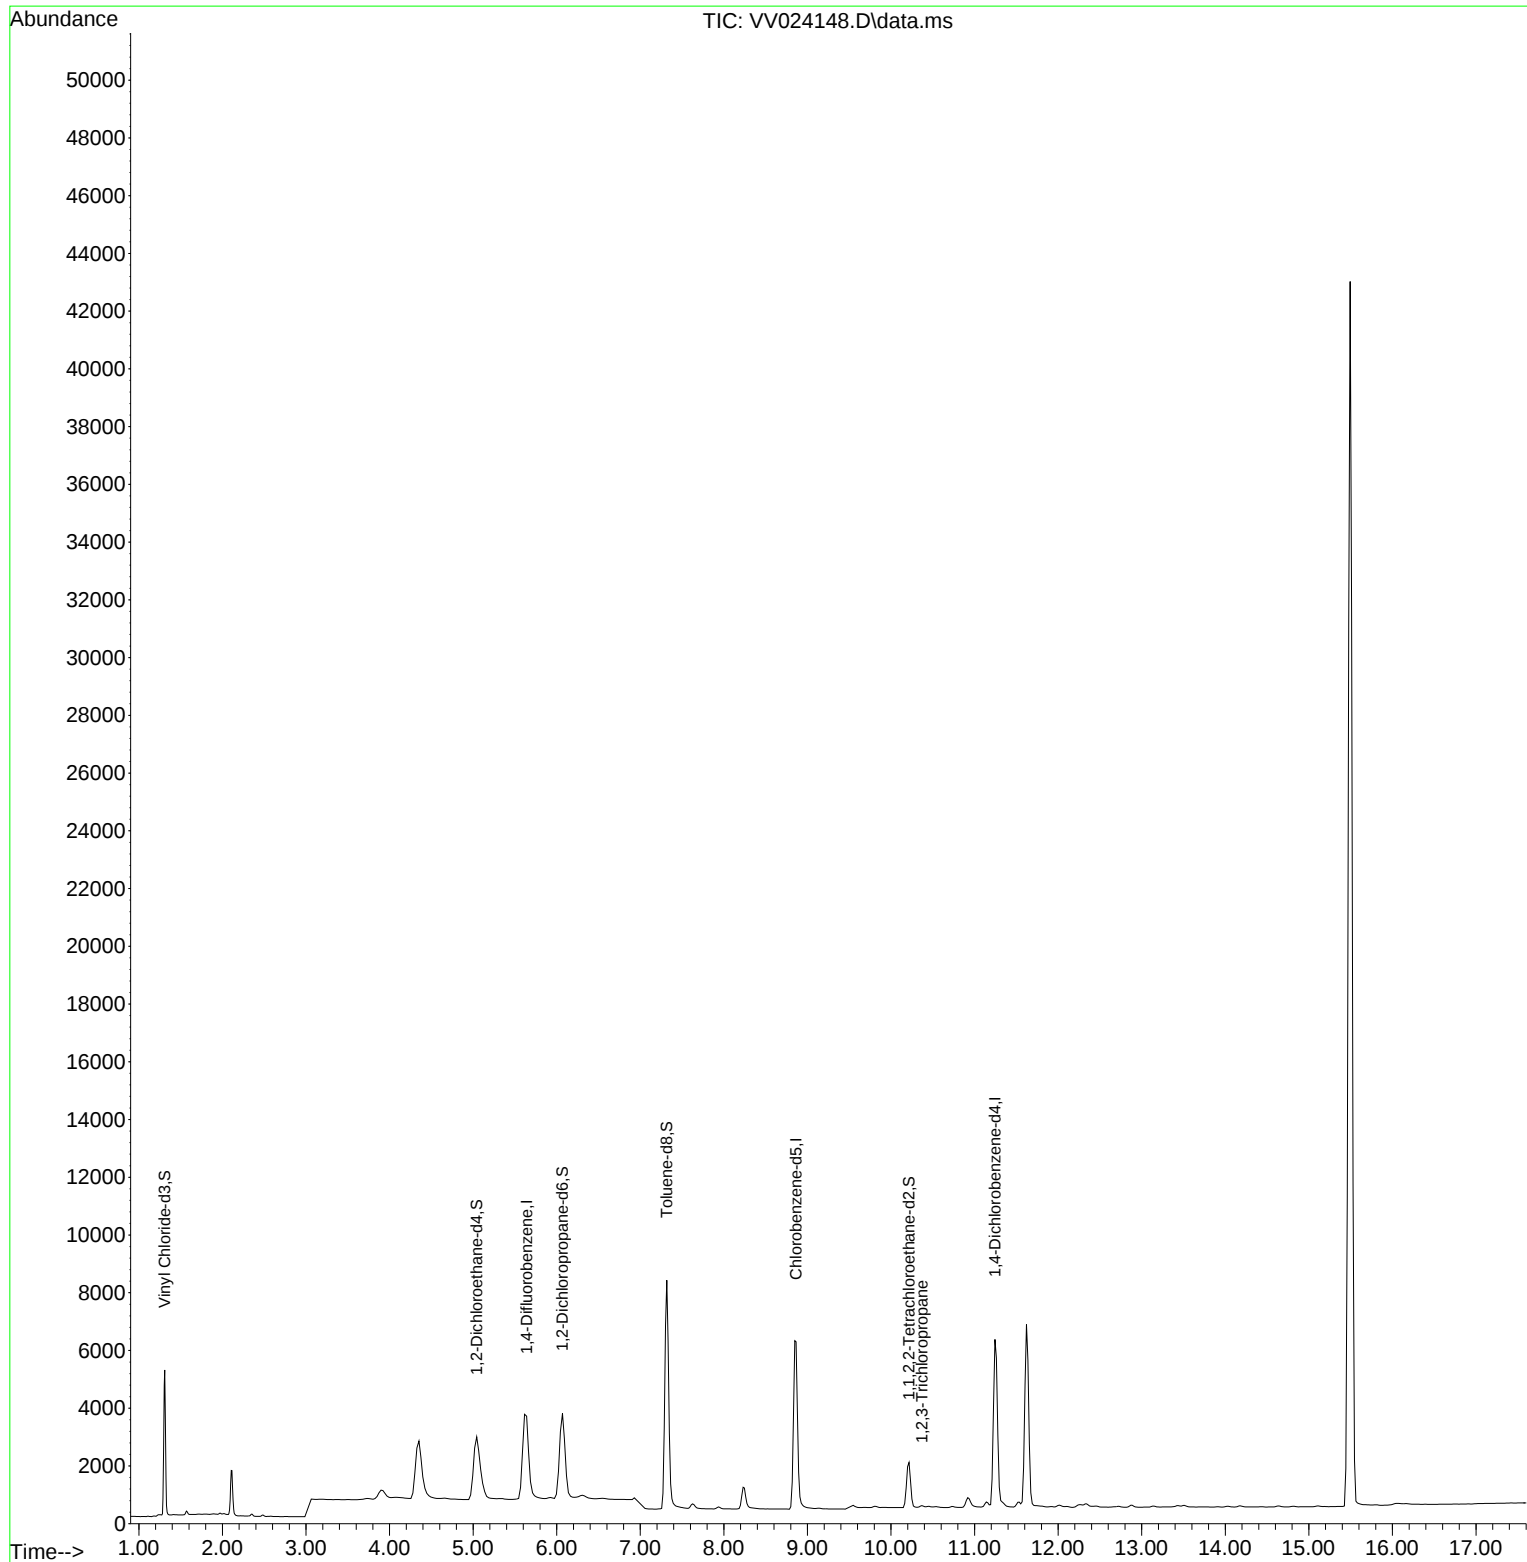

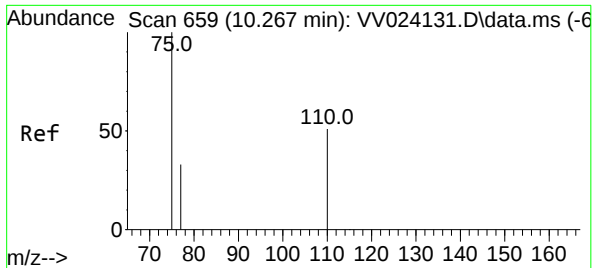

#12
 1,2,3-Trichloropropane
 Concen: 0.024 ug/L
 RT: 10.370 min Scan# 60
 Delta R.T. 0.103 min
 Lab File: VV024148.D
 Acq: 22 Dec 2021 18:11

Instrument :
 MSVOA_V
 ClientSampleId :

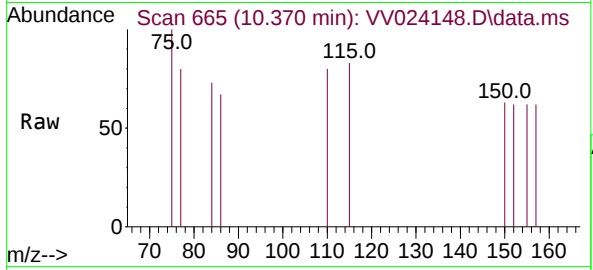

Tgt Ion: 75	Resp:	94
Ion	Ratio	Lower Upper
75	100	
110	59.6	38.2 57.4#
77	8.5	27.8 41.6#

