

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024149.D
 Acq On : 22 Dec 2021 18:35
 Operator : SY/MD
 Sample : M5152-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 23 06:14:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	10611	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.863	117	10346	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	5643	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	5165	0.438	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	88.000%		
4) 1,2-Dichloroethane-d4	5.042	65	4224	0.556	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	112.000%		
7) 1,2-Dichloropropane-d6	6.068	67	5009	0.657	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	132.000%		
8) Toluene-d8	7.317	98	13929	0.514	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2869	0.591	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	118.000%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.238	75	118	0.160	ug/L	Qvalue # 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024149.D
Acq On : 22 Dec 2021 18:35
Operator : SY/MD
Sample : M5152-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 23 06:14:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

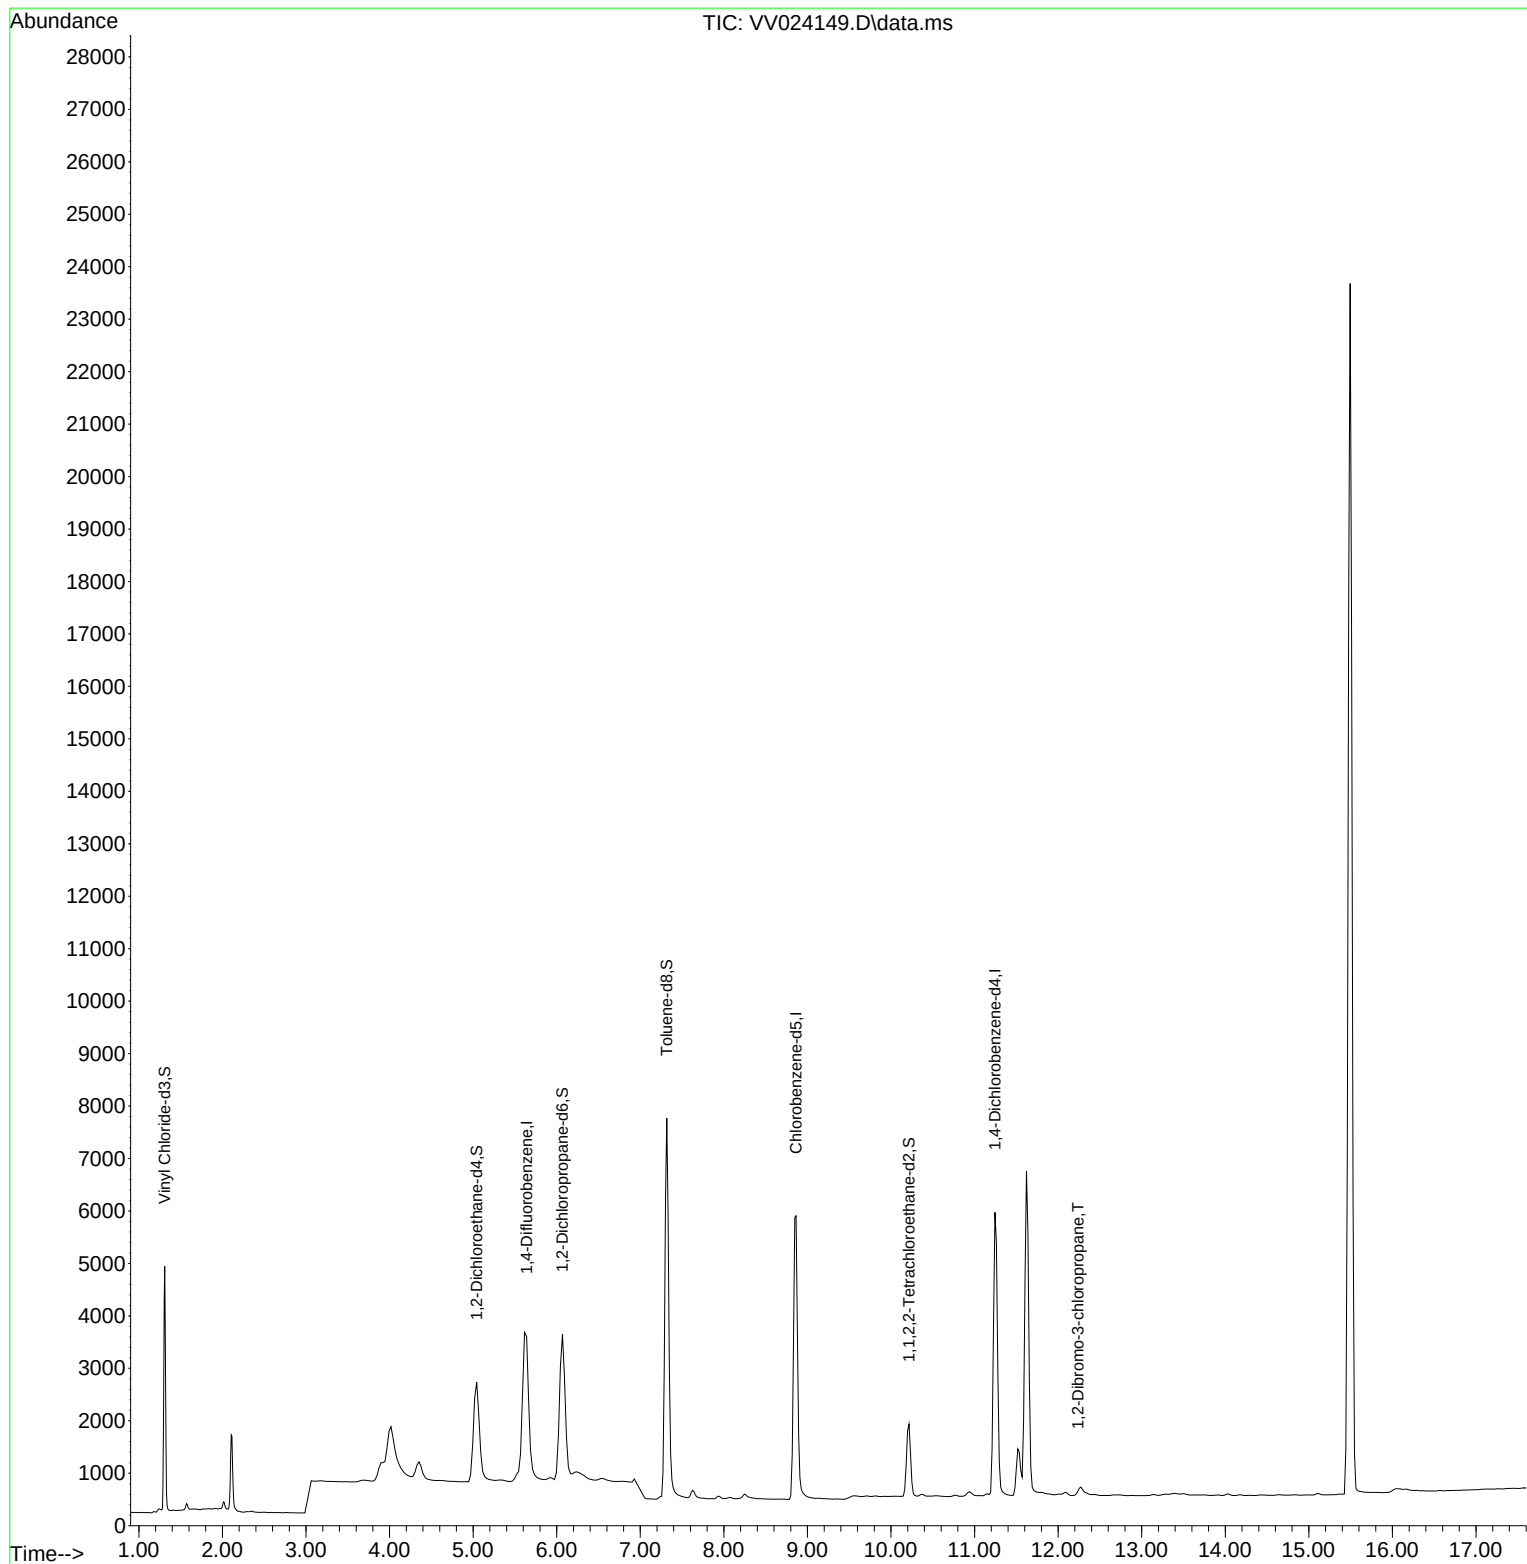

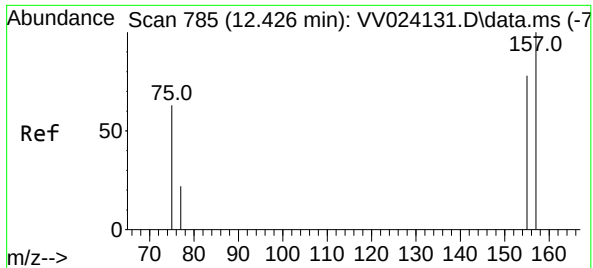

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.160 ug/L
 RT: 12.238 min Scan# 71
 Delta R.T. -0.188 min
 Lab File: VV024149.D
 Acq: 22 Dec 2021 18:35

Instrument :
 MSVOA_V
 ClientSampleId :

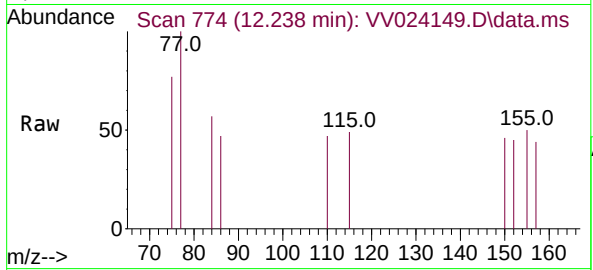

Tgt Ion: 75 Resp: 118
 Ion Ratio Lower Upper
 75 100
 157 57.1 102.9 154.3#
 155 64.8 87.6 131.4#

