

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122221\
 Data File : VV024151.D
 Acq On : 22 Dec 2021 19:22
 Operator : SY/MD
 Sample : M5152-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 23 06:15:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7979	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.863	117	7830	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	4665	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	4867	0.548	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	110.000%
4) 1,2-Dichloroethane-d4	5.042	65	2893	0.506	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
7) 1,2-Dichloropropane-d6	6.068	67	3002	0.521	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.317	98	10036	0.489	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1924	0.524	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.238	75	173	0.283	ug/L	Qvalue # 41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024151.D
Acq On : 22 Dec 2021 19:22
Operator : SY/MD
Sample : M5152-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 23 06:15:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

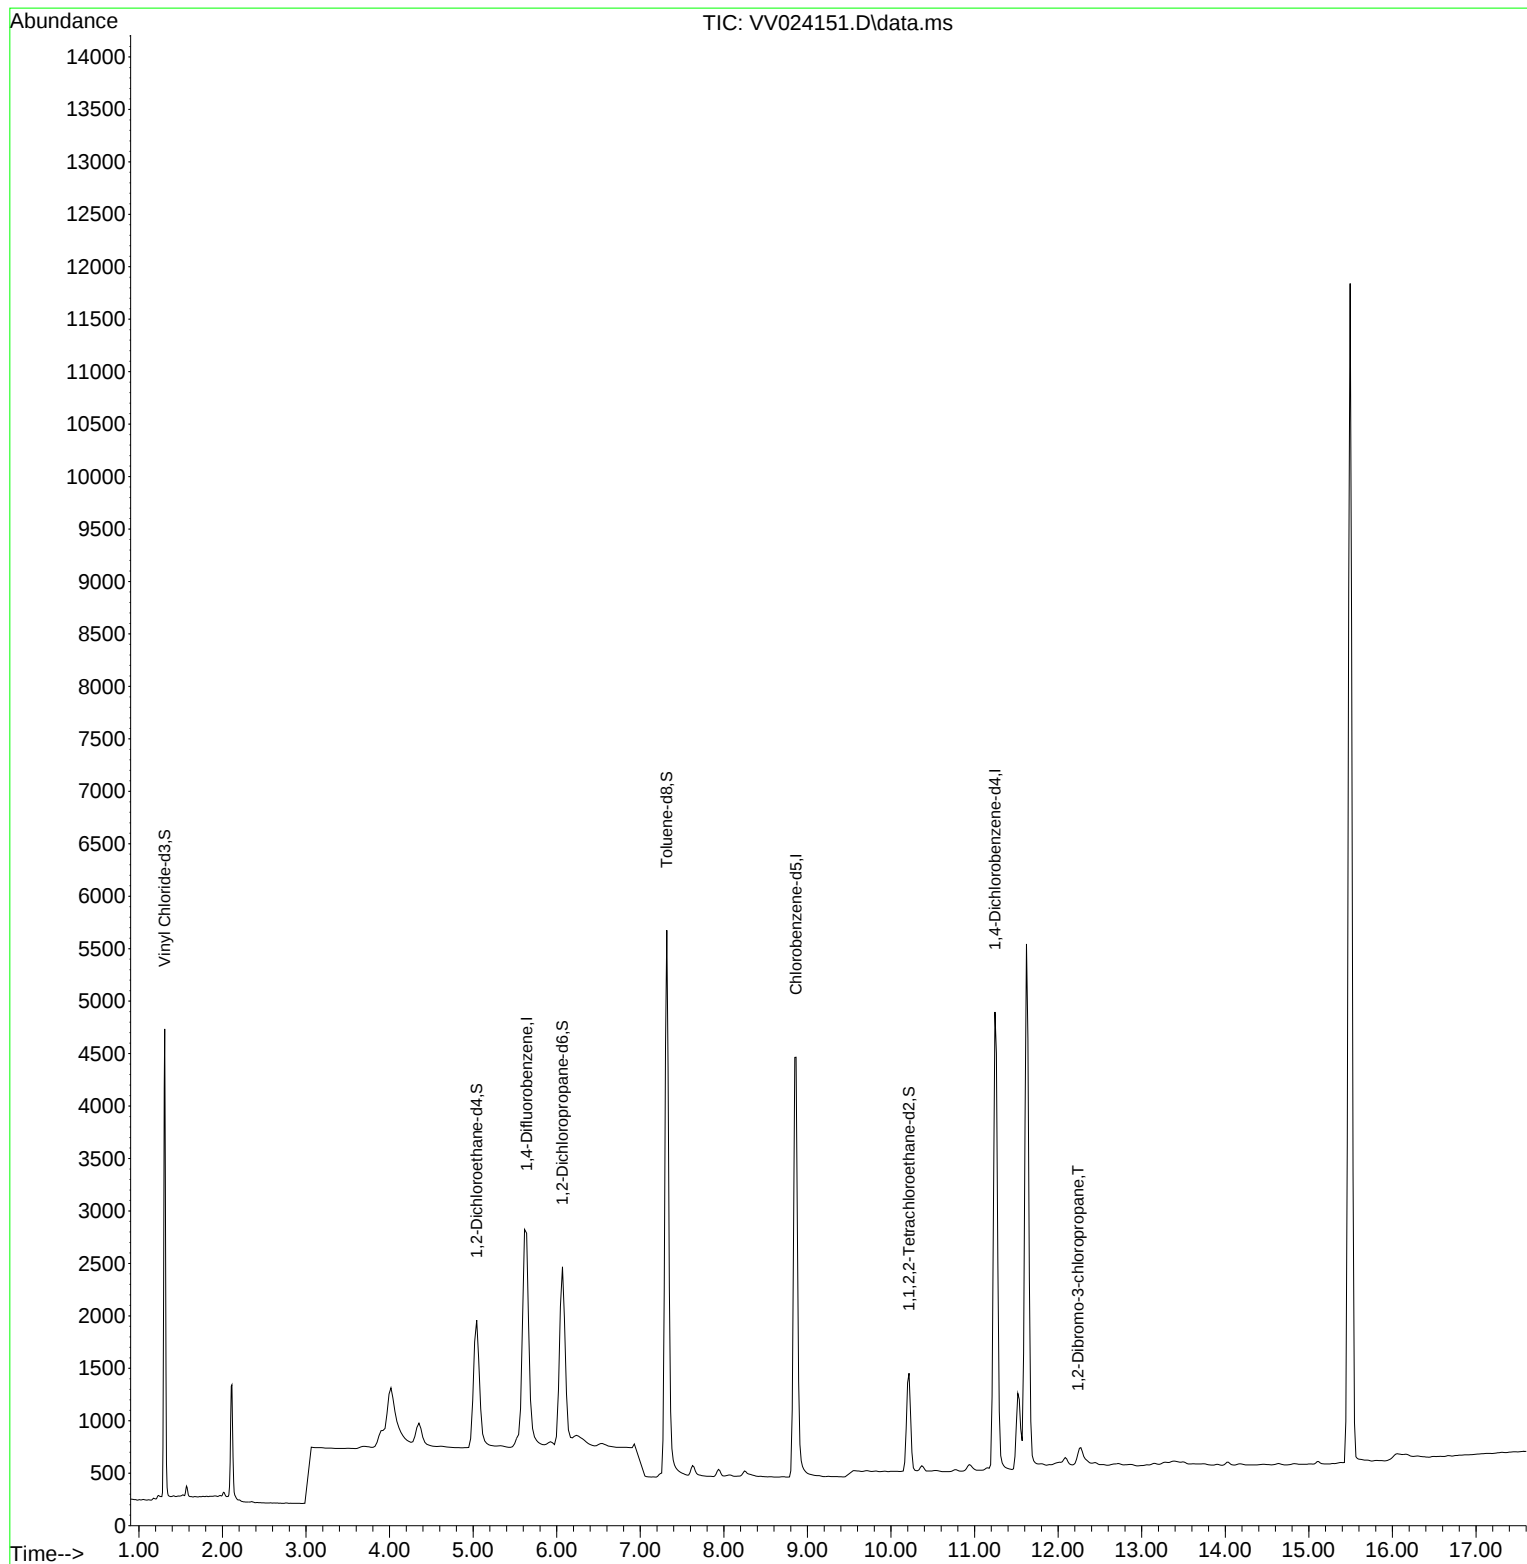

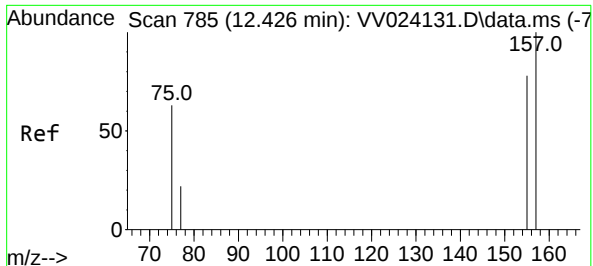

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.283 ug/L
 RT: 12.238 min Scan# 71
 Delta R.T. -0.188 min
 Lab File: VV024151.D
 Acq: 22 Dec 2021 19:22

Instrument :
 MSVOA_V
 ClientSampleId :

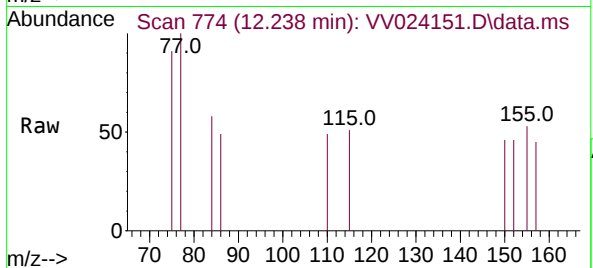

Tgt Ion: 75 Resp: 173
 Ion Ratio Lower Upper
 75 100
 157 49.5 102.9 154.3#
 155 57.9 87.6 131.4#

