




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024135.D
 Acq On : 22 Dec 2021 13:00
 Operator : SY/MD
 Sample : M5090-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D3

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Mahesh Dadoda 12/25/2021

Quant Time: Dec 23 07:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

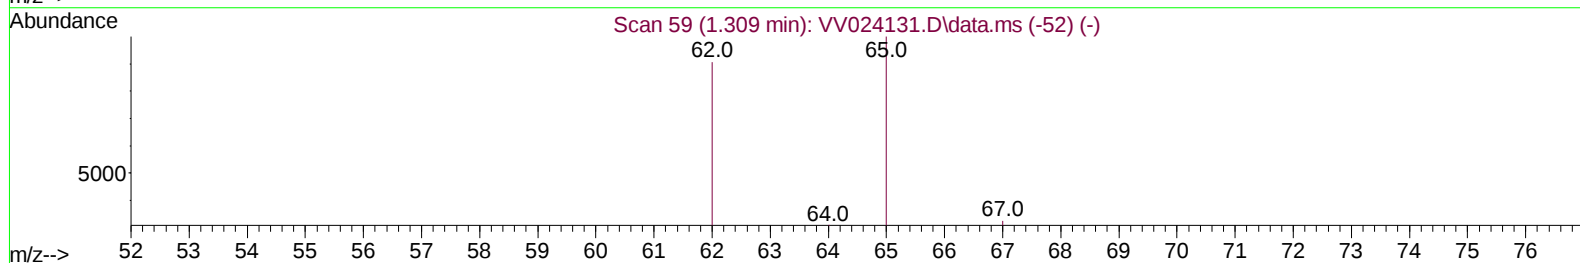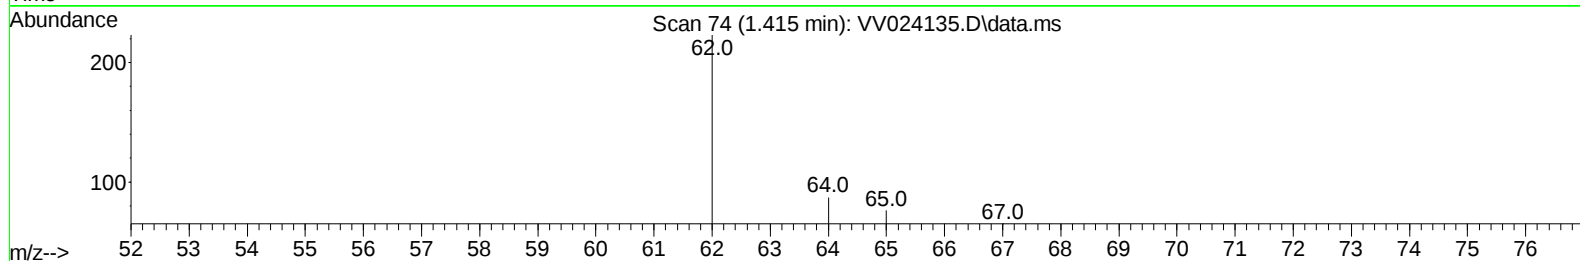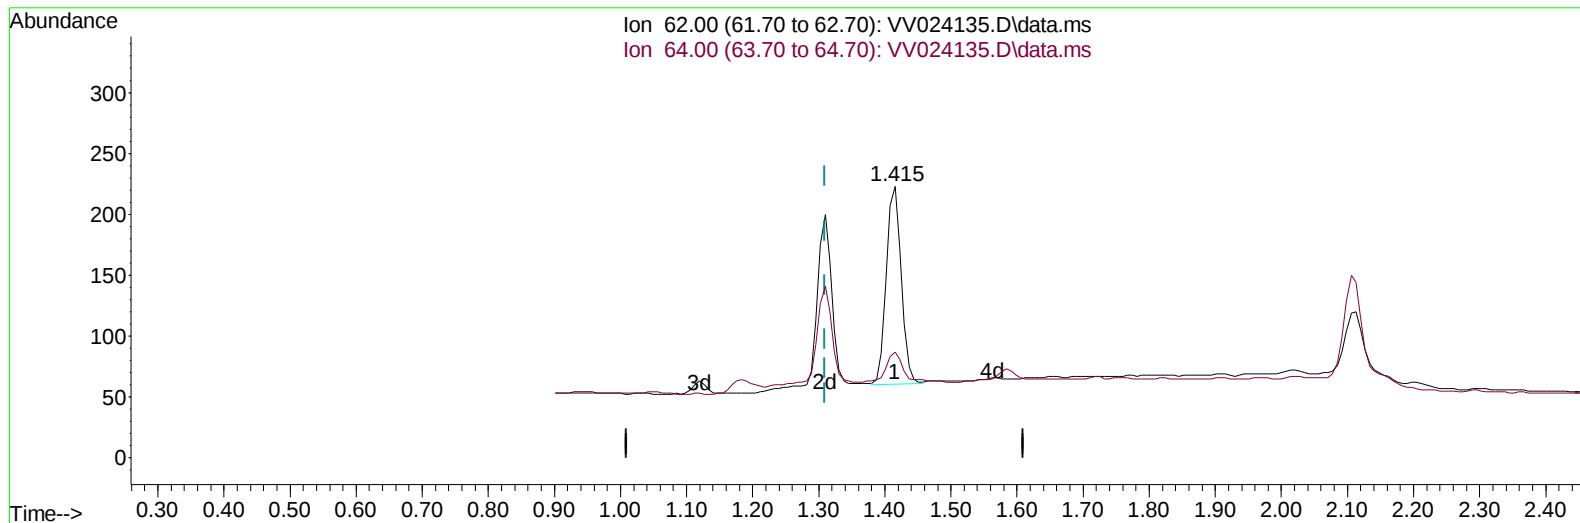

TIC: VV024135.D\data.ms

(3) Vinyl chloride (T)

1.415min (+ 0.106) 0.04 ug/L

response 255

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	36.10	39.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024135.D
 Acq On : 22 Dec 2021 13:00
 Operator : SY/MD
 Sample : M5090-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D3

Manual IntegrationsAPPROVED

Quant Time: Dec 23 07:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Mahesh Dadoda 12/25/2021

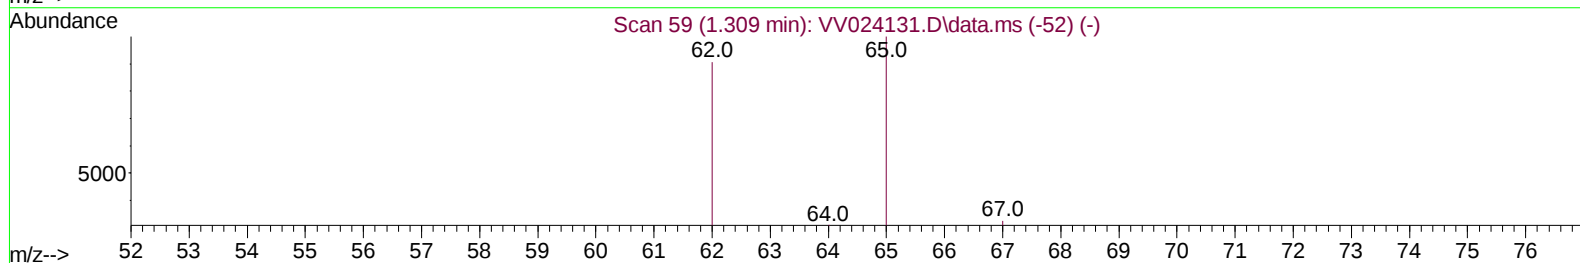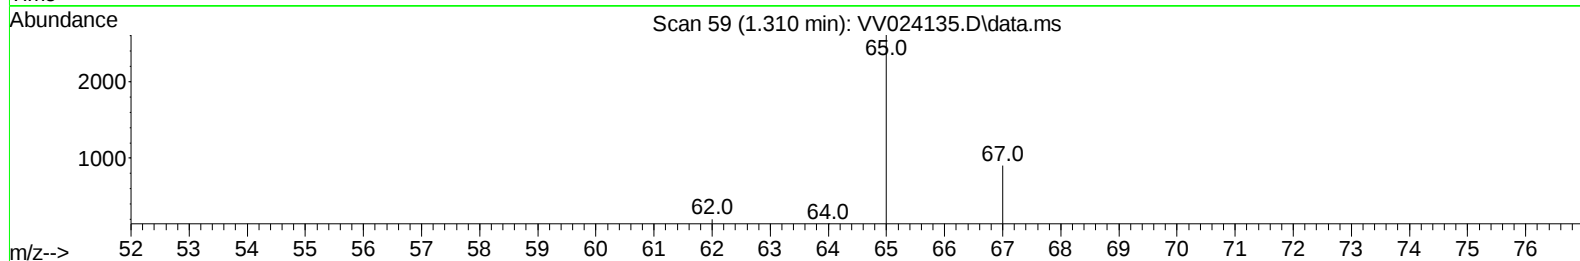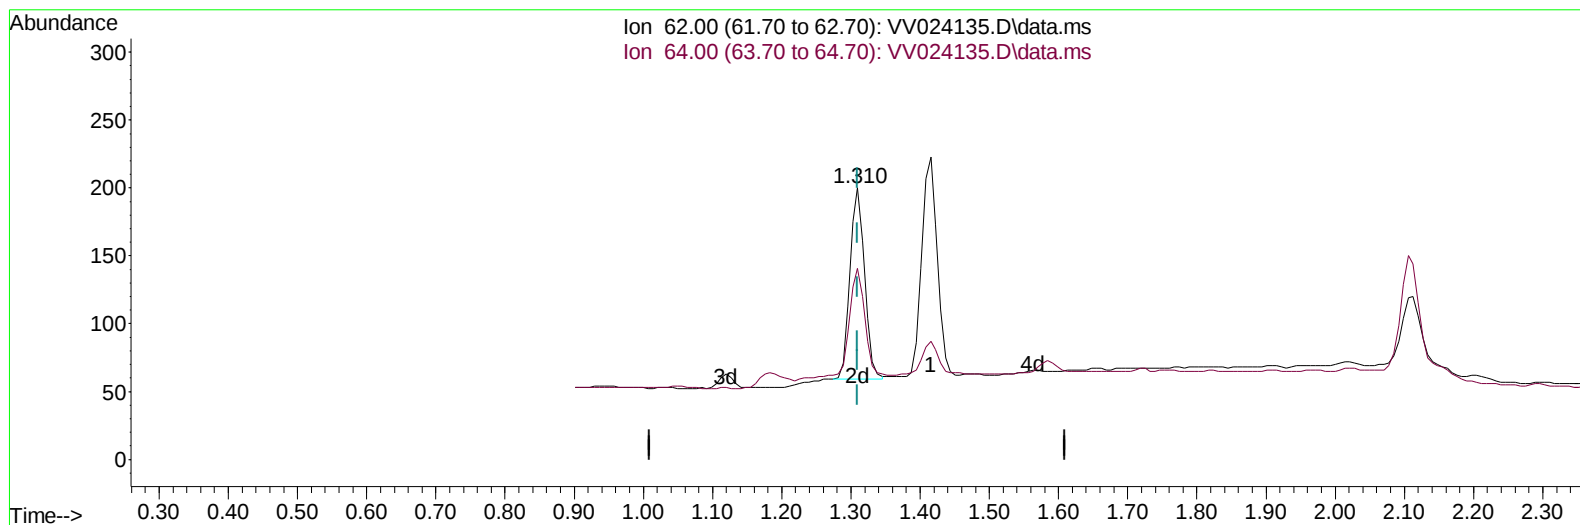

TIC: VV024135.D\data.ms

(3) Vinyl chloride (T)

1.310min (+ 0.000) 0.03 ug/L m

response 207

Ion	Exp%	Act%
62.00	100.00	100.00
64.00	36.10	70.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024135.D
 Acq On : 22 Dec 2021 13:00
 Operator : SY/MD
 Sample : M5090-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3D3

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Mahesh Dadoda 12/25/2021

Quant Time: Dec 23 07:09:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7518	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.863	117	7395	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	4251	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	3842	0.460	ug/L	0.00
Spiked Amount	0.500	Range 40 - 130	Recovery	=	92.000%	
4) 1,2-Dichloroethane-d4	5.042	65	2805	0.521	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	104.000%	
7) 1,2-Dichloropropane-d6	6.068	67	2852	0.524	ug/L	0.00
Spiked Amount	0.500	Range 60 - 140	Recovery	=	104.000%	
8) Toluene-d8	7.317	98	9786	0.505	ug/L	0.00
Spiked Amount	0.500	Range 70 - 130	Recovery	=	100.000%	
10) 1,1,2,2-Tetrachloroeth...	10.216	84	1903	0.549	ug/L	0.00
Spiked Amount	0.500	Range 65 - 120	Recovery	=	110.000%	
Target Compounds						
3) Vinyl chloride	1.310	62	207m	0.030	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024135.D
Acq On : 22 Dec 2021 13:00
Operator : SY/MD
Sample : M5090-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3D3

Manual IntegrationsAPPROVED

Quant Time: Dec 23 07:09:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
Supervised By :Mahesh Dadoda 12/25/2021

