

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024141.D
 Acq On : 22 Dec 2021 15:24
 Operator : SY/MD
 Sample : M5090-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3C5

Quant Time: Dec 23 06:13:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 23 06:11:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7871	0.500	ug/L	0.02
5) Chlorobenzene-d5	8.863	117	8000	0.500	ug/L	0.02
11) 1,4-Dichlorobenzene-d4	11.244	152	5144	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	4055	0.463	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	92.000%		
4) 1,2-Dichloroethane-d4	5.042	65	2896	0.514	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
7) 1,2-Dichloropropane-d6	6.068	67	3087	0.524	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	104.000%		
8) Toluene-d8	7.317	98	10323	0.492	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2284	0.609	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	122.000%#		
Target Compounds						
3) Vinyl chloride	1.310	62	123	0.017	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
Data File : VV024141.D
Acq On : 22 Dec 2021 15:24
Operator : SY/MD
Sample : M5090-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3C5

Quant Time: Dec 23 06:13:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 23 06:11:19 2021
Response via : Initial Calibration

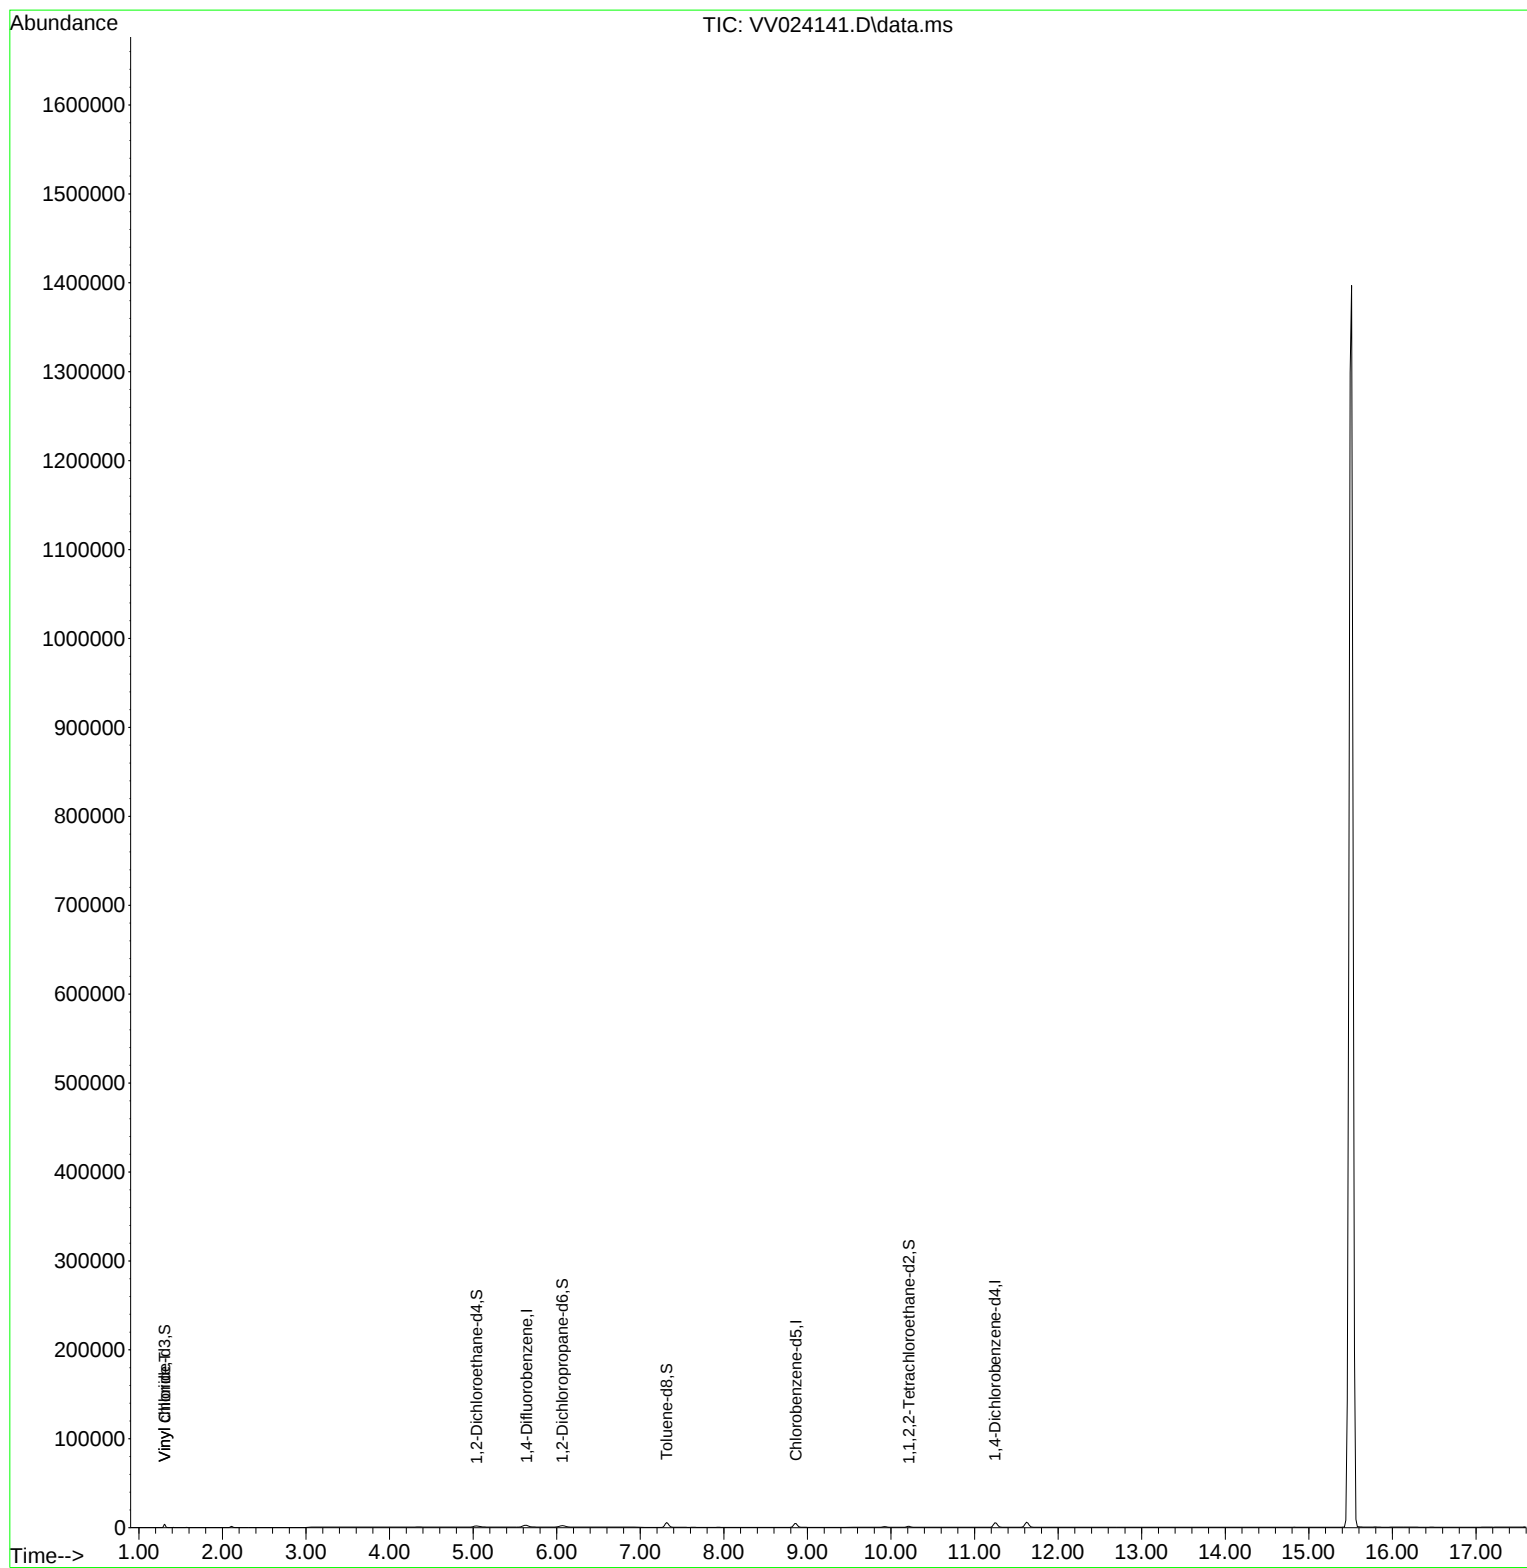

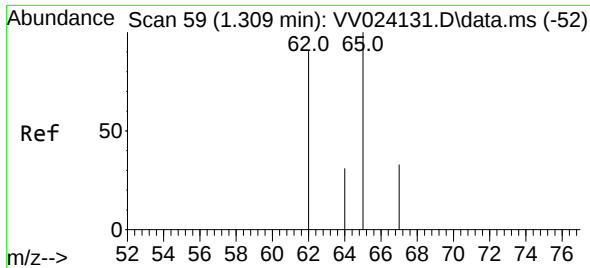

#3
Vinyl chloride
Concen: 0.017 ug/L
RT: 1.310 min Scan# 59
Delta R.T. 0.000 min
Lab File: VV024141.D
Acq: 22 Dec 2021 15:24

Instrument :
MSVOA_V
ClientSampleId :
BG3C5

Tgt Ion: 62 Resp: 123
Ion Ratio Lower Upper
62 100
64 112.2 25.3 46.9#

