
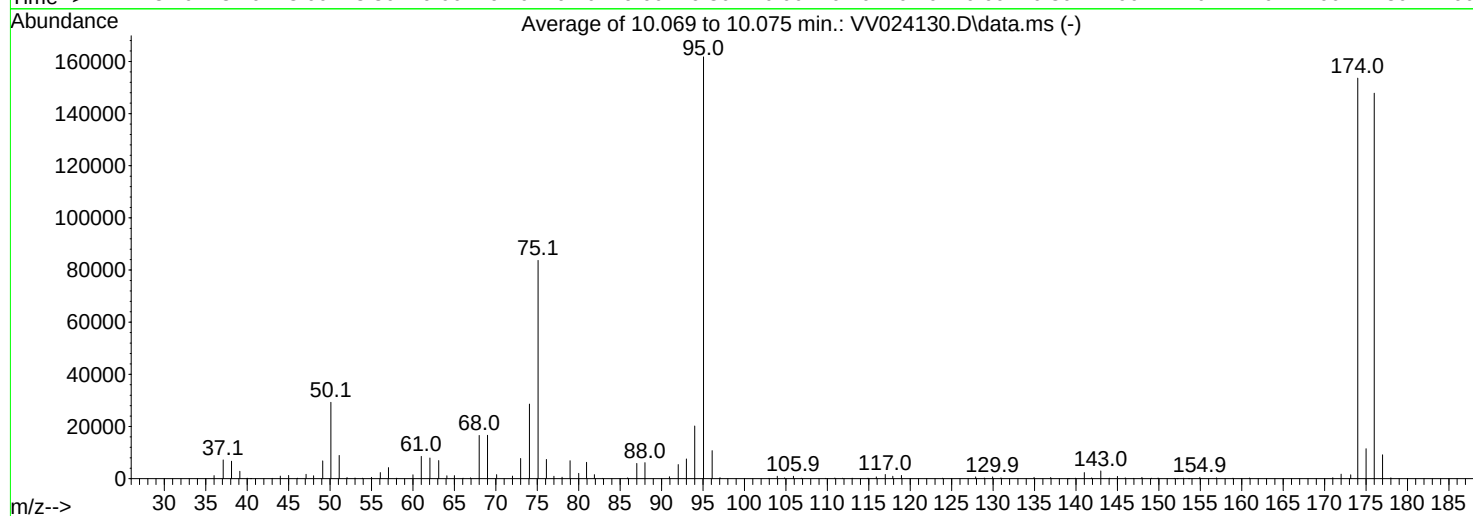


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122221\
 Data File : VV024130.D
 Acq On : 22 Dec 2021 10:04
 Operator : SY/MD
 Sample : BFB209
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB209

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122121.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Dec 23 07:39:59 2021

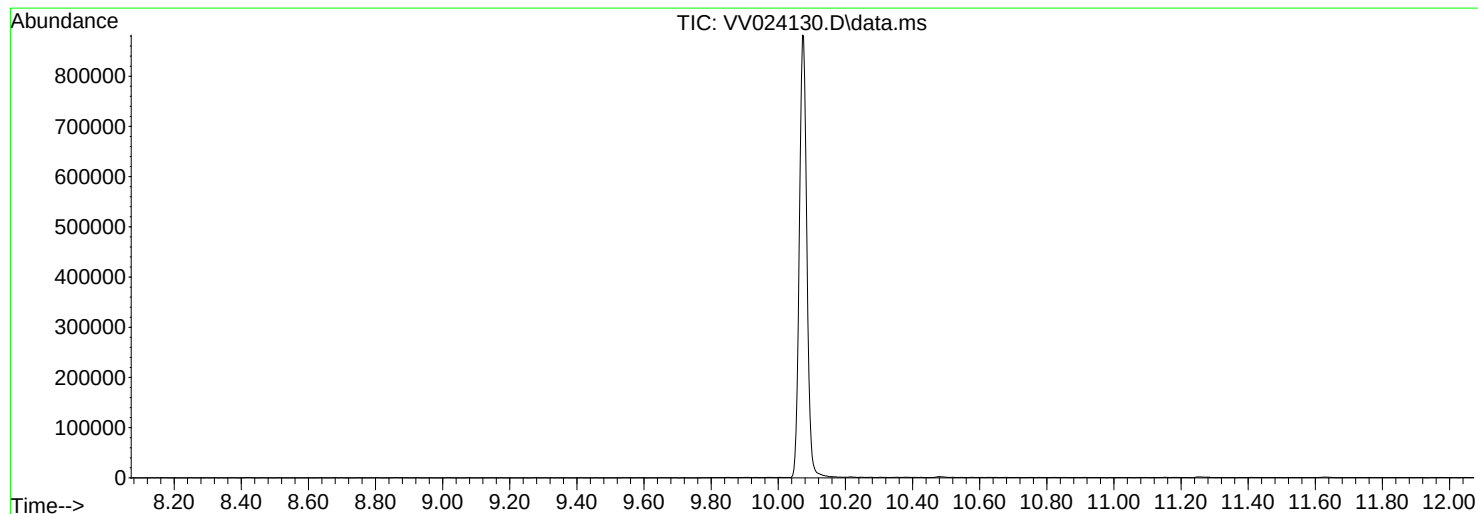

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	29296	PASS
75	95	30	80	51.7	83715	PASS
95	95	100	100	100.0	161771	PASS
96	95	5	9	6.7	10761	PASS
173	174	0.00	2	0.9	1454	PASS
174	95	50	120	94.9	153600	PASS
175	174	5	9	7.5	11497	PASS
176	174	95	101	96.2	147819	PASS
177	176	5	9	6.2	9160	PASS

m/z	Abundance
36.00	615.0
37.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	1748.0
37.10	6893.0
38.10	6342.0
39.10	2776.0
40.00	223.0
44.00	984.0
45.00	1194.0
46.00	181.0
47.10	1504.0
48.00	969.0
49.10	6518.0
50.10	27952.0
51.10	8033.0
52.00	436.0
53.00	191.0
53.90	133.0
55.00	446.0
56.10	2126.0
57.00	3839.0
58.10	176.0
60.00	1457.0
61.00	8080.0
62.10	7364.0
63.10	6710.0
64.10	1070.0
65.00	1069.0
66.10	164.0
67.00	295.0
68.00	15364.0
69.00	15539.0
70.10	1420.0
72.00	878.0
73.00	7203.0
74.00	26792.0
75.10	78320.0
76.10	6779.0
77.00	770.0
78.00	553.0
79.00	6493.0
80.00	1822.0
81.00	6015.0
81.90	1438.0
82.90	142.0
85.90	283.0
87.00	5567.0
88.00	5460.0
91.00	718.0
92.00	5121.0
93.00	6984.0
94.00	18888.0
95.00	152448.0
96.10	10747.0
97.10	355.0
103.00	117.0
104.00	962.0
104.90	346.0
105.90	896.0
106.80	175.0
109.70	130.0
110.90	268.0
111.90	176.0
113.00	180.0
114.90	209.0
115.90	688.0
117.00	1387.0
117.90	827.0
119.00	1062.0
123.90	157.0
127.90	560.0
128.90	252.0
130.00	672.0
131.00	256.0
134.90	447.0
137.00	357.0
139.90	158.0
141.00	2112.0
141.90	219.0
143.00	2730.0
144.00	162.0
145.00	979.0
145.90	270.0
146.90	112.0
147.90	430.0
149.10	113.0
149.90	210.0
151.80	103.0
152.20	112.0
153.00	181.0
154.90	471.0
157.00	311.0
158.90	186.0
161.00	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

170.90	365.0
172.00	1546.0
173.10	2003.0
174.00	141184.0
175.00	10977.0
176.00	134720.0
177.00	8342.0
178.00	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	1812.0
37.10	7414.0
38.10	6994.0
39.10	2945.0
40.00	212.0
43.00	142.0
44.00	1021.0
45.00	1252.0
46.10	203.0
47.10	1724.0
48.00	1161.0
49.10	7061.0
50.10	30232.0
51.10	9227.0
52.10	461.0
53.00	243.0
53.90	219.0
55.00	479.0
56.00	2341.0
57.10	4428.0
58.10	204.0
60.00	1542.0
61.00	8940.0
62.10	8242.0
63.10	7282.0
64.10	1149.0
65.00	1213.0
66.00	186.0
66.90	284.0
68.00	17312.0
69.00	17272.0
70.10	1623.0
72.00	993.0
73.00	7956.0
74.10	29576.0
75.10	86640.0
76.10	7756.0
77.00	933.0
78.00	525.0
78.90	7046.0
80.00	2120.0
80.90	6449.0
81.90	1594.0
82.90	147.0
85.90	310.0
87.00	6040.0
88.00	6304.0
91.00	762.0
92.00	5567.0
93.00	7821.0
94.00	20960.0
95.00	167168.0
96.10	11123.0
97.00	368.0
103.00	161.0
104.00	982.0
104.90	342.0
105.90	1015.0
106.90	183.0
109.80	140.0
110.90	260.0
111.90	172.0
113.00	214.0
114.90	189.0
115.90	708.0
117.00	1674.0
117.90	945.0
118.90	1232.0
123.90	197.0
127.90	669.0
129.00	273.0
129.90	706.0
130.90	287.0
135.00	503.0
137.00	493.0
140.00	174.0
141.00	2428.0
141.90	317.0
143.00	3035.0
144.10	170.0
145.00	934.0
146.00	307.0
147.00	130.0
148.00	522.0
149.10	175.0
149.90	240.0
151.90	128.0
153.00	194.0
154.90	504.0
156.90	336.0
158.90	217.0
161.00	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

171.00	389.0
172.00	1772.0
173.20	2358.0
174.00	158848.0
175.00	11890.0
176.00	152576.0
177.00	9504.0
178.00	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	1805.0
37.10	7263.0
38.10	6839.0
39.10	2774.0
40.00	204.0
40.40	112.0
43.00	179.0
44.00	1009.0
45.00	1292.0
46.10	216.0
47.10	1677.0
48.00	1141.0
49.10	6786.0
50.10	29704.0
51.10	9386.0
52.10	444.0
53.00	237.0
53.90	244.0
55.00	501.0
56.00	2448.0
57.10	4404.0
58.00	203.0
60.00	1507.0
61.00	8631.0
62.00	8107.0
63.10	6885.0
64.10	1046.0
65.00	1193.0
66.00	200.0
66.90	315.0
68.00	17096.0
69.00	17144.0
70.10	1524.0
72.00	1008.0
73.00	8019.0
74.10	29408.0
75.10	86184.0
76.10	7626.0
77.00	998.0
78.00	534.0
78.90	7026.0
80.00	2147.0
80.90	6357.0
81.90	1610.0
82.90	163.0
85.90	277.0
87.00	5931.0
88.00	6571.0
90.90	710.0
92.00	5480.0
93.00	7766.0
94.00	20736.0
95.10	165696.0
96.10	10414.0
97.00	363.0
102.90	145.0
103.90	867.0
104.80	307.0
105.90	938.0
106.90	164.0
109.90	146.0
110.90	237.0
111.80	162.0
113.00	229.0
114.90	170.0
115.90	707.0
117.00	1738.0
117.90	981.0
118.90	1344.0
123.90	180.0
127.90	751.0
129.00	271.0
129.90	673.0
130.90	301.0
135.00	475.0
136.90	514.0
139.10	113.0
139.90	170.0
141.00	2515.0
141.90	355.0
143.00	3064.0
144.00	182.0
145.00	748.0
146.00	339.0
147.00	160.0
148.00	499.0
149.10	195.0
149.90	267.0
151.90	150.0
153.00	174.0
153.60	113.0
155.00	520.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

157.00	330.0
159.00	240.0
160.90	287.0
171.10	416.0
172.00	1810.0
174.00	160768.0
175.00	11624.0
176.00	156160.0
177.00	9633.0
178.00	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209