

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029769.D
 Acq On : 22 Dec 2022 19:25
 Operator : SY/MD
 Sample : N6195-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN8

Quant Time: Dec 23 02:10:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	477453	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	460685	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	243441	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	162544	55.595	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	111.180%
7) Chloroethane-d5	1.564	69	134987	60.548	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	121.100%
11) 1,1-Dichloroethene-d2	2.104	63	204928	44.938	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.880%
21) 2-Butanone-d5	3.870	46	179495	100.639	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.640%
24) Chloroform-d	4.339	84	263303	47.857	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.720%
26) 1,2-Dichloroethane-d4	5.024	65	159219	50.669	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.340%
32) Benzene-d6	5.043	84	588278	48.327	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.660%
36) 1,2-Dichloropropane-d6	6.063	67	182760	49.152	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.300%
41) Toluene-d8	7.307	98	516565	45.038	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.080%
43) trans-1,3-Dichloroprop...	7.612	79	75977	40.466	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.940%
47) 2-Hexanone-d5	8.082	63	151099	95.164	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.160%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	252379	47.499	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	11.612	152	209836	45.280	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.560%
Target Compounds						
					Qvalue	
10) 1,1,2-Trichloro-1,2,2-...	2.104	101	1962	0.786	ug/L	# 18
13) Acetone	2.162	43	8550	7.359	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029769.D
Acq On : 22 Dec 2022 19:25
Operator : SY/MD
Sample : N6195-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN8

Quant Time: Dec 23 02:10:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration




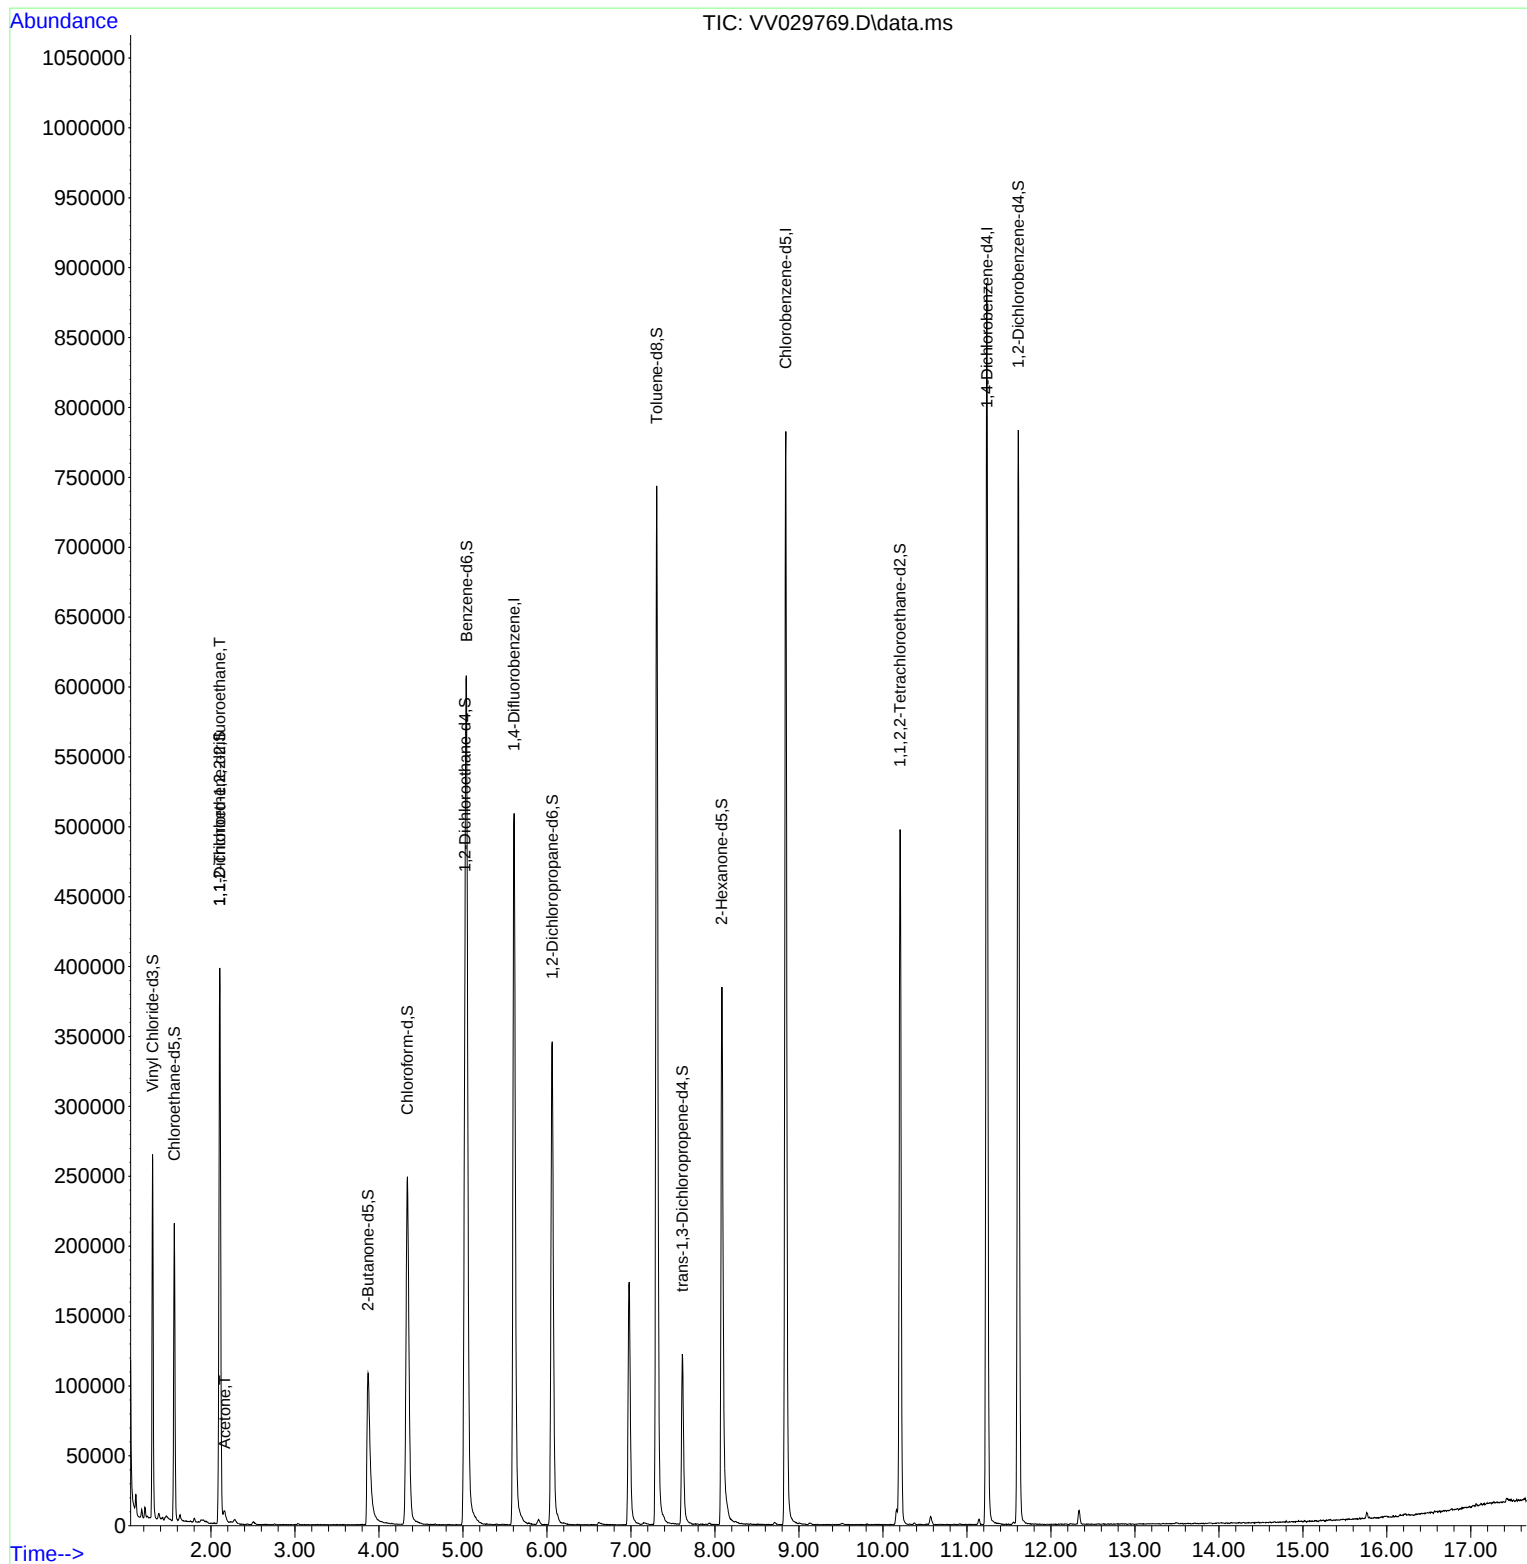


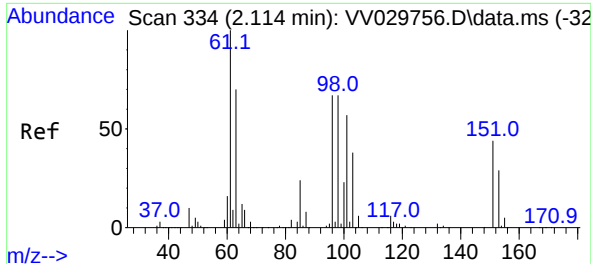

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.786 ug/L
RT: 2.104 min Scan# 331
Delta R.T. -0.010 min
Lab File: VV029769.D
Acq: 22 Dec 2022 19:25

Instrument :
MSVOA_V
ClientSampleId :
BGSN8

Tgt Ion:101 Resp: 1962
Ion Ratio Lower Upper
101 100
85 0.0 33.6 50.4#
151 0.0 63.5 95.3#

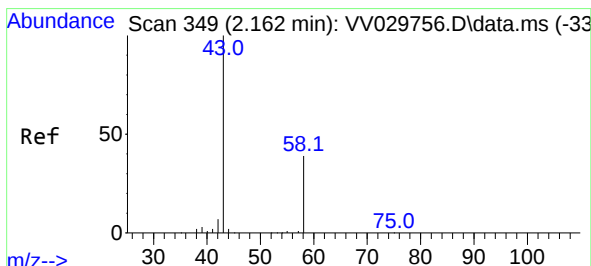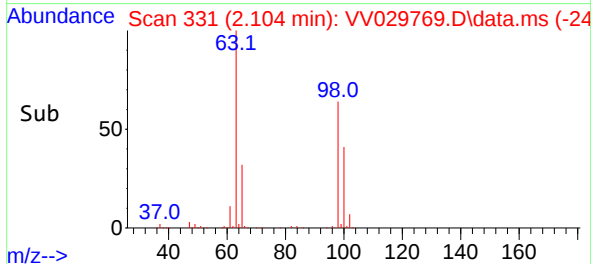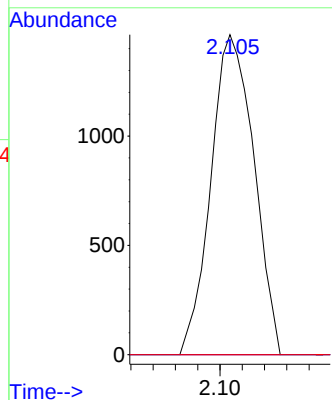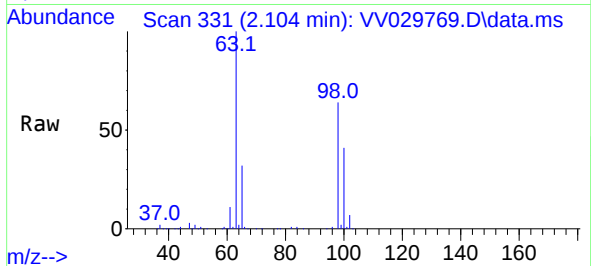

#13
Acetone
Concen: 7.359 ug/L
RT: 2.162 min Scan# 349
Delta R.T. -0.000 min
Lab File: VV029769.D
Acq: 22 Dec 2022 19:25

Tgt Ion: 43 Resp: 8550
Ion Ratio Lower Upper
43 100
58 36.4 0.0 74.8

