

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029761.D
 Acq On : 22 Dec 2022 16:18
 Operator : SY/MD
 Sample : N6193-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN1

Quant Time: Dec 23 02:09:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	483735	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	466551	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	245971	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	148487	50.127	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	100.260%	
7) Chloroethane-d5	1.561	69	126626	56.060	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	112.120%	
11) 1,1-Dichloroethene-d2	2.101	63	189041	40.916	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	81.840%	
21) 2-Butanone-d5	3.873	46	165581	91.632	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.630%	
24) Chloroform-d	4.336	84	243068	43.605	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	87.220%	
26) 1,2-Dichloroethane-d4	5.021	65	150991	47.427	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.860%	
32) Benzene-d6	5.040	84	544672	44.182	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.360%	
36) 1,2-Dichloropropane-d6	6.063	67	169569	45.031	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.060%	
41) Toluene-d8	7.307	98	480816	41.394	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.780%	
43) trans-1,3-Dichloroprop...	7.612	79	71234	37.462	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	74.920%	
47) 2-Hexanone-d5	8.085	63	136516	84.898	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	84.900%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	234339	43.549	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.100%	
66) 1,2-Dichlorobenzene-d4	11.612	152	191017	40.795	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	81.600%	
Target Compounds						
13) Acetone	2.163	43	11391	9.677	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029761.D
Acq On : 22 Dec 2022 16:18
Operator : SY/MD
Sample : N6193-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN1

Quant Time: Dec 23 02:09:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

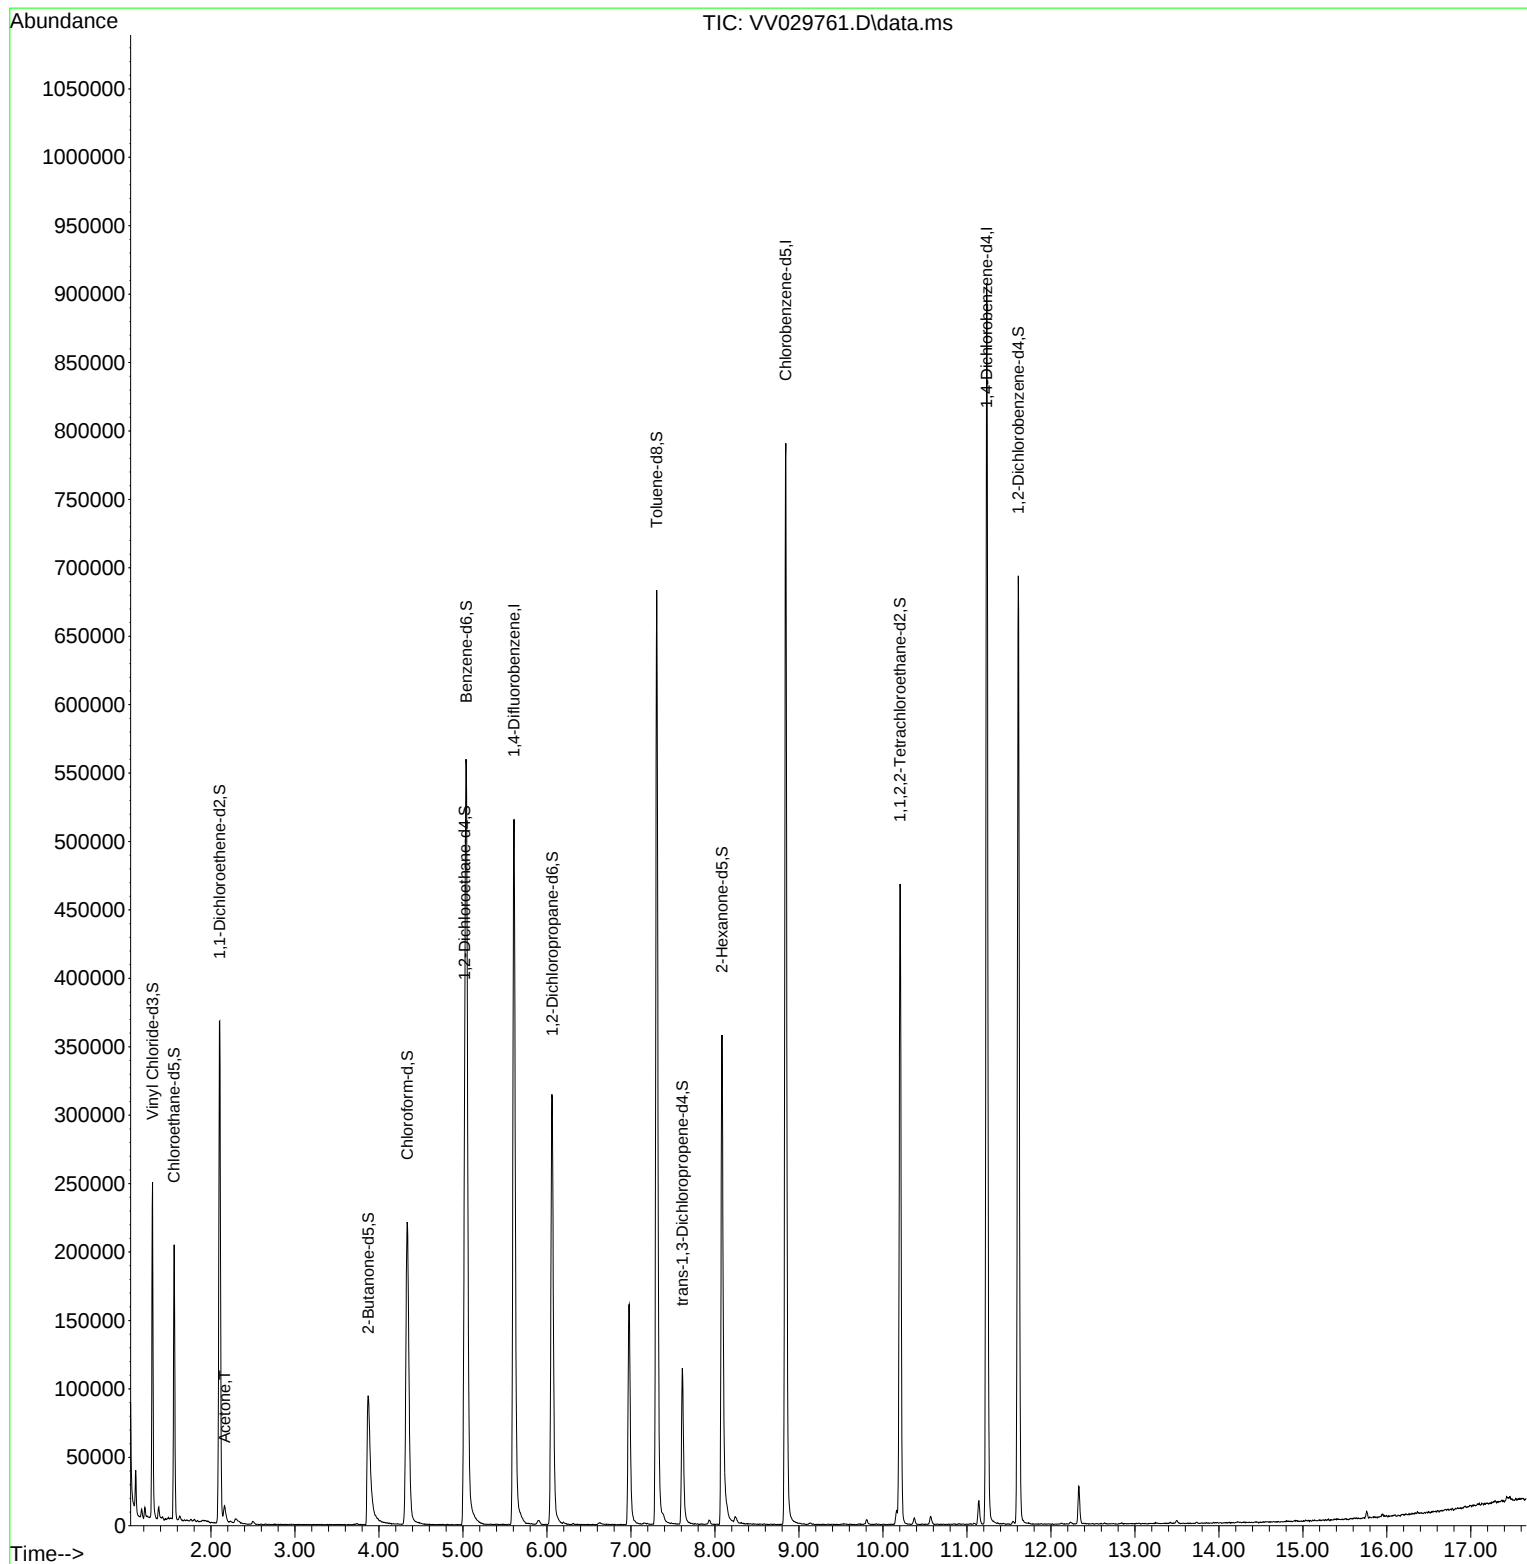

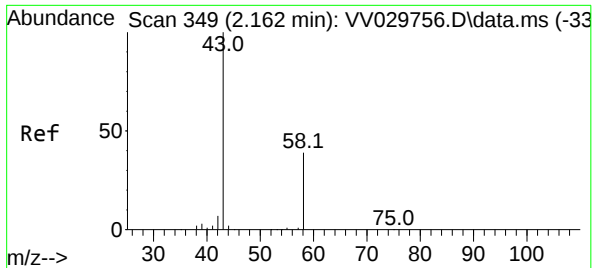

#13
 Acetone
 Concen: 9.677 ug/L
 RT: 2.163 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: VV029761.D
 Acq: 22 Dec 2022 16:18

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN1

Tgt Ion: 43 Resp: 11391
 Ion Ratio Lower Upper
 43 100
 58 40.1 0.0 74.8

