

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029763.D
 Acq On : 22 Dec 2022 17:04
 Operator : SY/MD
 Sample : N6193-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Quant Time: Dec 23 02:09:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	437063	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	424232	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	221231	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	154088	57.573	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	115.140%	
7) Chloroethane-d5	1.565	69	132870	65.106	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	130.220%#	
11) 1,1-Dichloroethene-d2	2.105	63	200995	48.149	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	96.300%	
21) 2-Butanone-d5	3.873	46	187336	114.742	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	114.740%	
24) Chloroform-d	4.339	84	267068	53.027	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.060%	
26) 1,2-Dichloroethane-d4	5.024	65	162430	56.468	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	112.940%	
32) Benzene-d6	5.044	84	588220	52.474	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	104.940%	
36) 1,2-Dichloropropane-d6	6.063	67	180619	52.750	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	105.500%	
41) Toluene-d8	7.307	98	521990	49.422	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.840%	
43) trans-1,3-Dichloroprop...	7.613	79	77539	44.846	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.700%	
47) 2-Hexanone-d5	8.085	63	155112	106.086	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	106.090%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	251795	51.461	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	102.920%	
66) 1,2-Dichlorobenzene-d4	11.612	152	204985	48.674	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.340%	
Target Compounds						
13) Acetone	2.166	43	4799	4.512	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029763.D
Acq On : 22 Dec 2022 17:04
Operator : SY/MD
Sample : N6193-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Time: Dec 23 02:09:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

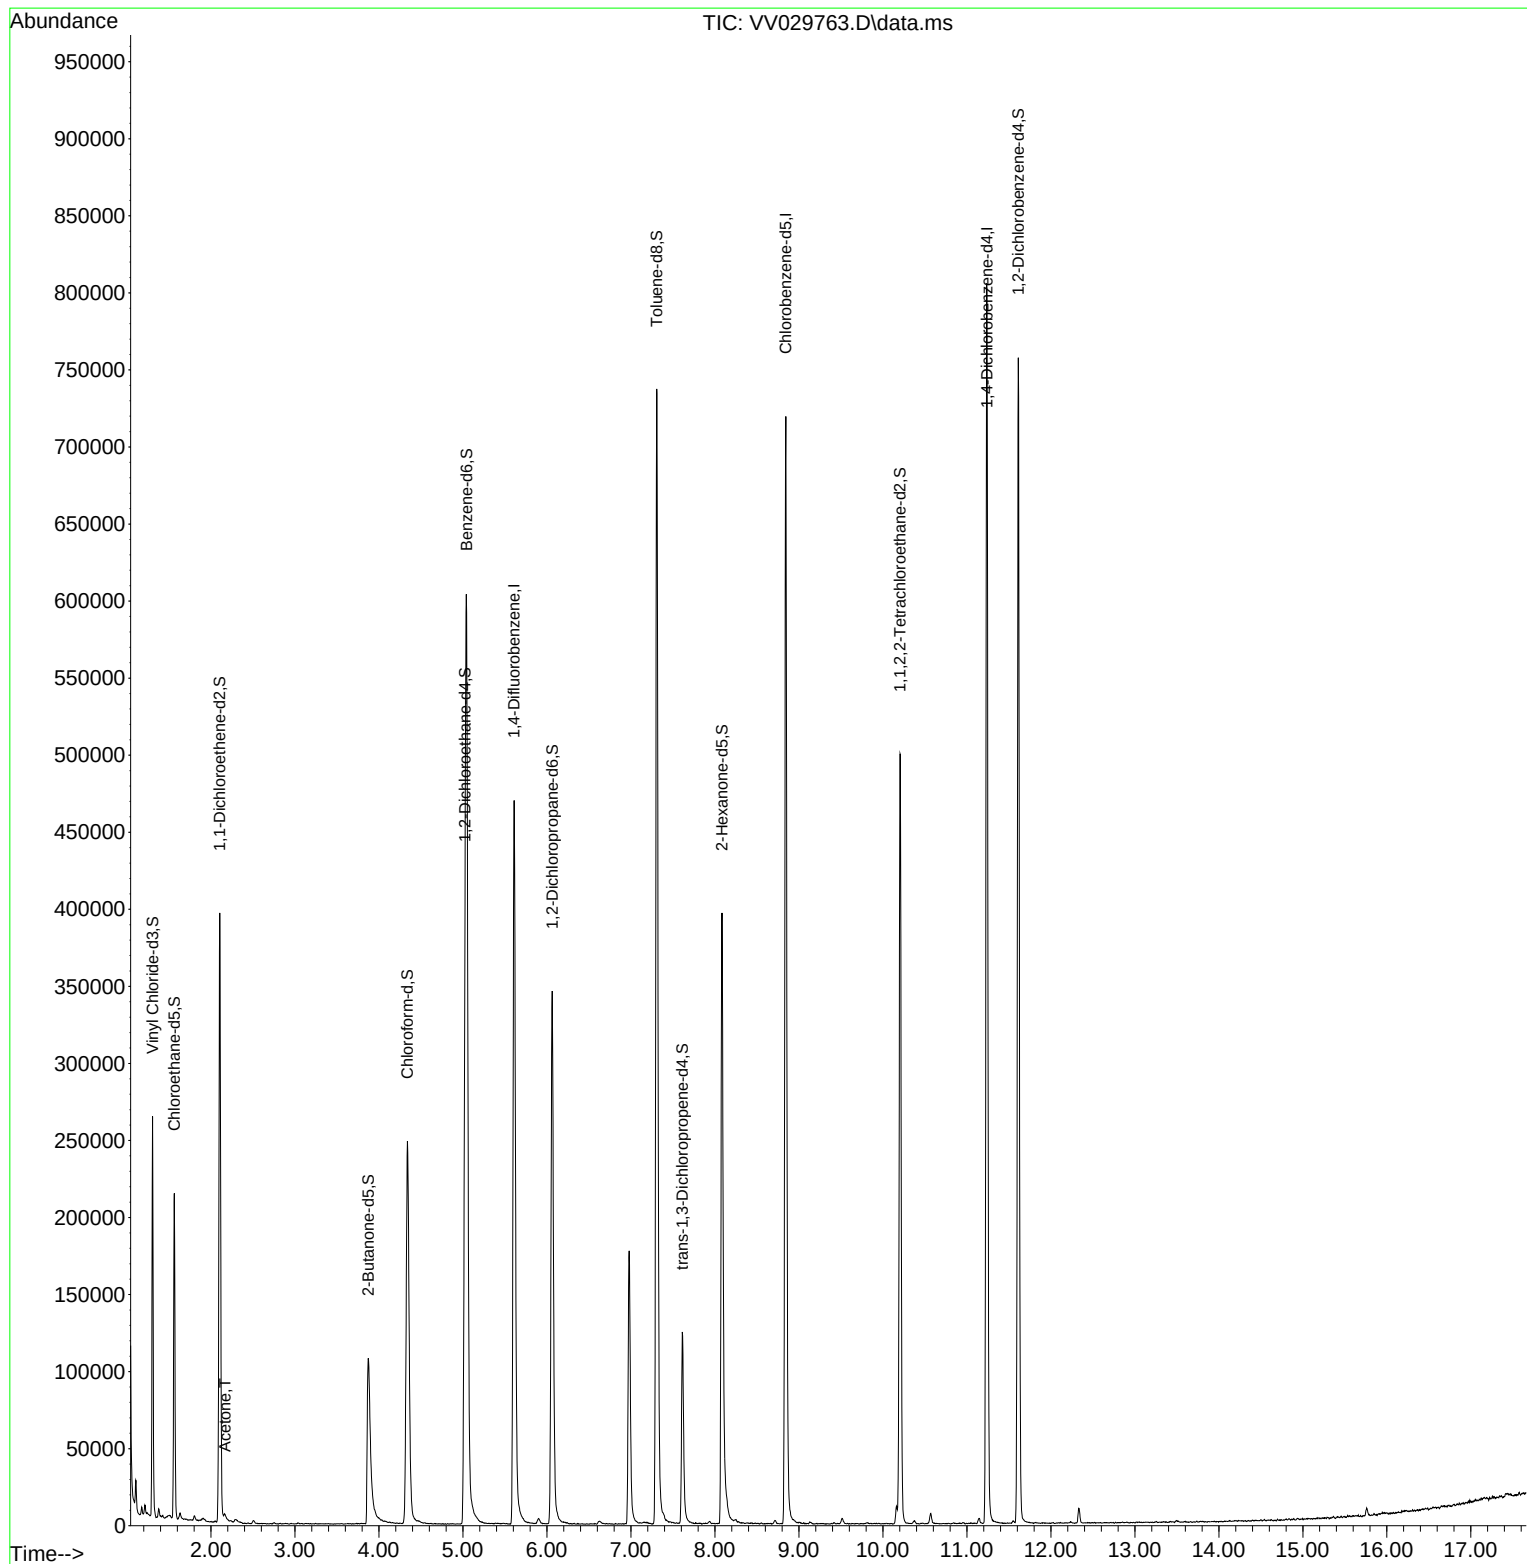

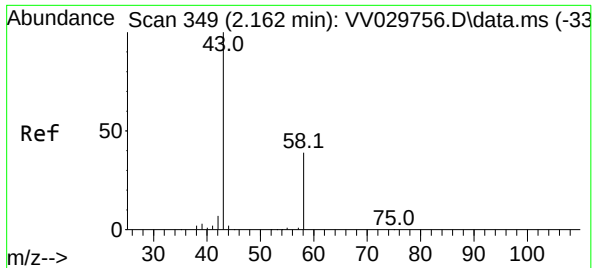

#13
 Acetone
 Concen: 4.512 ug/L
 RT: 2.166 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV029763.D
 Acq: 22 Dec 2022 17:04

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Tgt Ion:	43	Resp:	4799
Ion Ratio	Lower	Upper	
43	100		
58	37.4	0.0	74.8

