

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029764.D
 Acq On : 22 Dec 2022 17:27
 Operator : SY/MD
 Sample : N6193-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Quant Time: Dec 23 02:09:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.609	114	398280	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.844	117	388483	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.239	152	202451	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	167095	68.512	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	137.020%	#
7) Chloroethane-d5		1.564	69	136141	73.205	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	146.400%	#
11) 1,1-Dichloroethene-d2		2.105	63	209966	55.196	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	110.400%	
21) 2-Butanone-d5		3.870	46	184047	123.705	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	123.700%	
24) Chloroform-d		4.339	84	269451	58.710	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	117.420%	
26) 1,2-Dichloroethane-d4		5.024	65	162744	62.086	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	124.180%	
32) Benzene-d6		5.040	84	593319	57.800	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	115.600%	
36) 1,2-Dichloropropane-d6		6.063	67	185455	59.147	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	118.300%	
41) Toluene-d8		7.307	98	531212	54.923	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.840%	
43) trans-1,3-Dichloroprop...		7.612	79	79715	50.347	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.700%	
47) 2-Hexanone-d5		8.082	63	154753	115.580	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	115.580%	
56) 1,1,2,2-Tetrachloroeth...		10.204	84	256127	57.163	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	114.320%	
66) 1,2-Dichlorobenzene-d4		11.612	152	208230	54.031	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.060%	
Target Compounds							Qvalue
13) Acetone		2.162	43	9481	9.782	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029764.D
Acq On : 22 Dec 2022 17:27
Operator : SY/MD
Sample : N6193-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Time: Dec 23 02:09:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

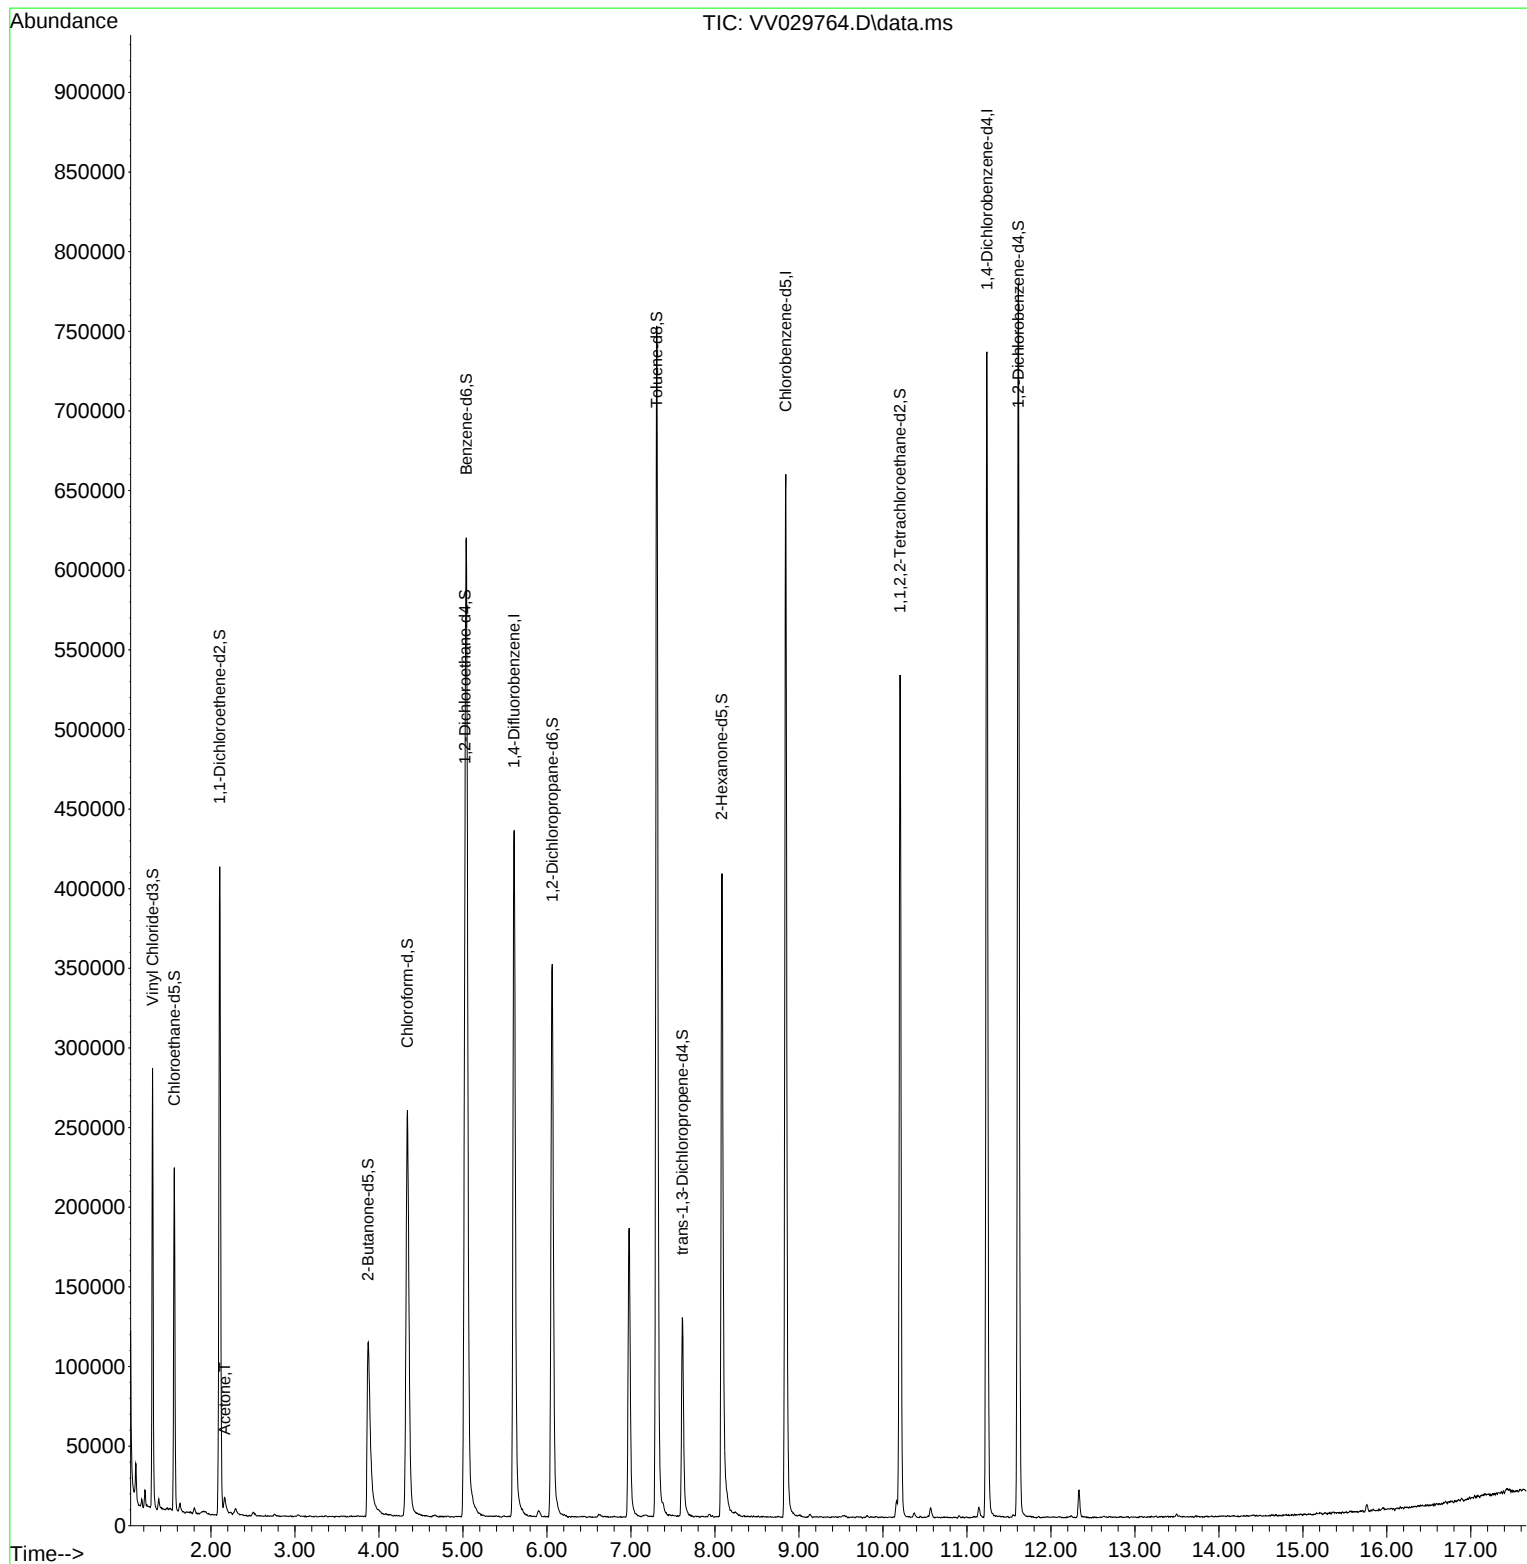

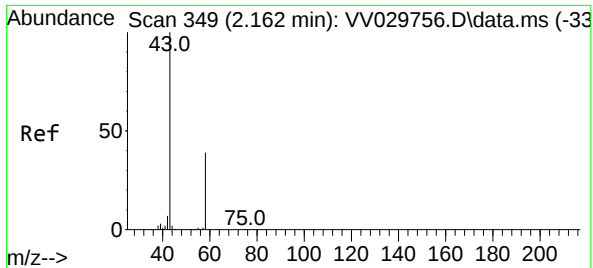

#13
 Acetone
 Concen: 9.782 ug/L
 RT: 2.162 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV029764.D
 Acq: 22 Dec 2022 17:27

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Tgt Ion: 43 Resp: 9481
 Ion Ratio Lower Upper
 43 100
 58 40.9 0.0 74.8

