

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029765.D
 Acq On : 22 Dec 2022 17:51
 Operator : SY/MD
 Sample : N6193-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Quant Time: Dec 23 02:09:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	436003	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	420893	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	220711	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	152760	57.216	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	114.440%	
7) Chloroethane-d5	1.565	69	129699	63.707	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	127.420%	
11) 1,1-Dichloroethene-d2	2.105	63	197648	47.462	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	94.920%	
21) 2-Butanone-d5	3.867	46	179269	110.068	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	110.070%	
24) Chloroform-d	4.339	84	258504	51.451	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.900%	
26) 1,2-Dichloroethane-d4	5.021	65	156647	54.590	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	109.180%	
32) Benzene-d6	5.040	84	564131	50.725	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.440%	
36) 1,2-Dichloropropane-d6	6.060	67	178499	52.545	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	105.080%	
41) Toluene-d8	7.307	98	500130	47.728	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.460%	
43) trans-1,3-Dichloroprop...	7.613	79	74393	43.368	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.740%	
47) 2-Hexanone-d5	8.082	63	140964	97.174	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	97.170%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	244439	50.354	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	100.700%	
66) 1,2-Dichlorobenzene-d4	11.612	152	197732	47.062	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	94.120%	
Target Compounds						
13) Acetone	2.156	43	5645	5.320	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029765.D
Acq On : 22 Dec 2022 17:51
Operator : SY/MD
Sample : N6193-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Time: Dec 23 02:09:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

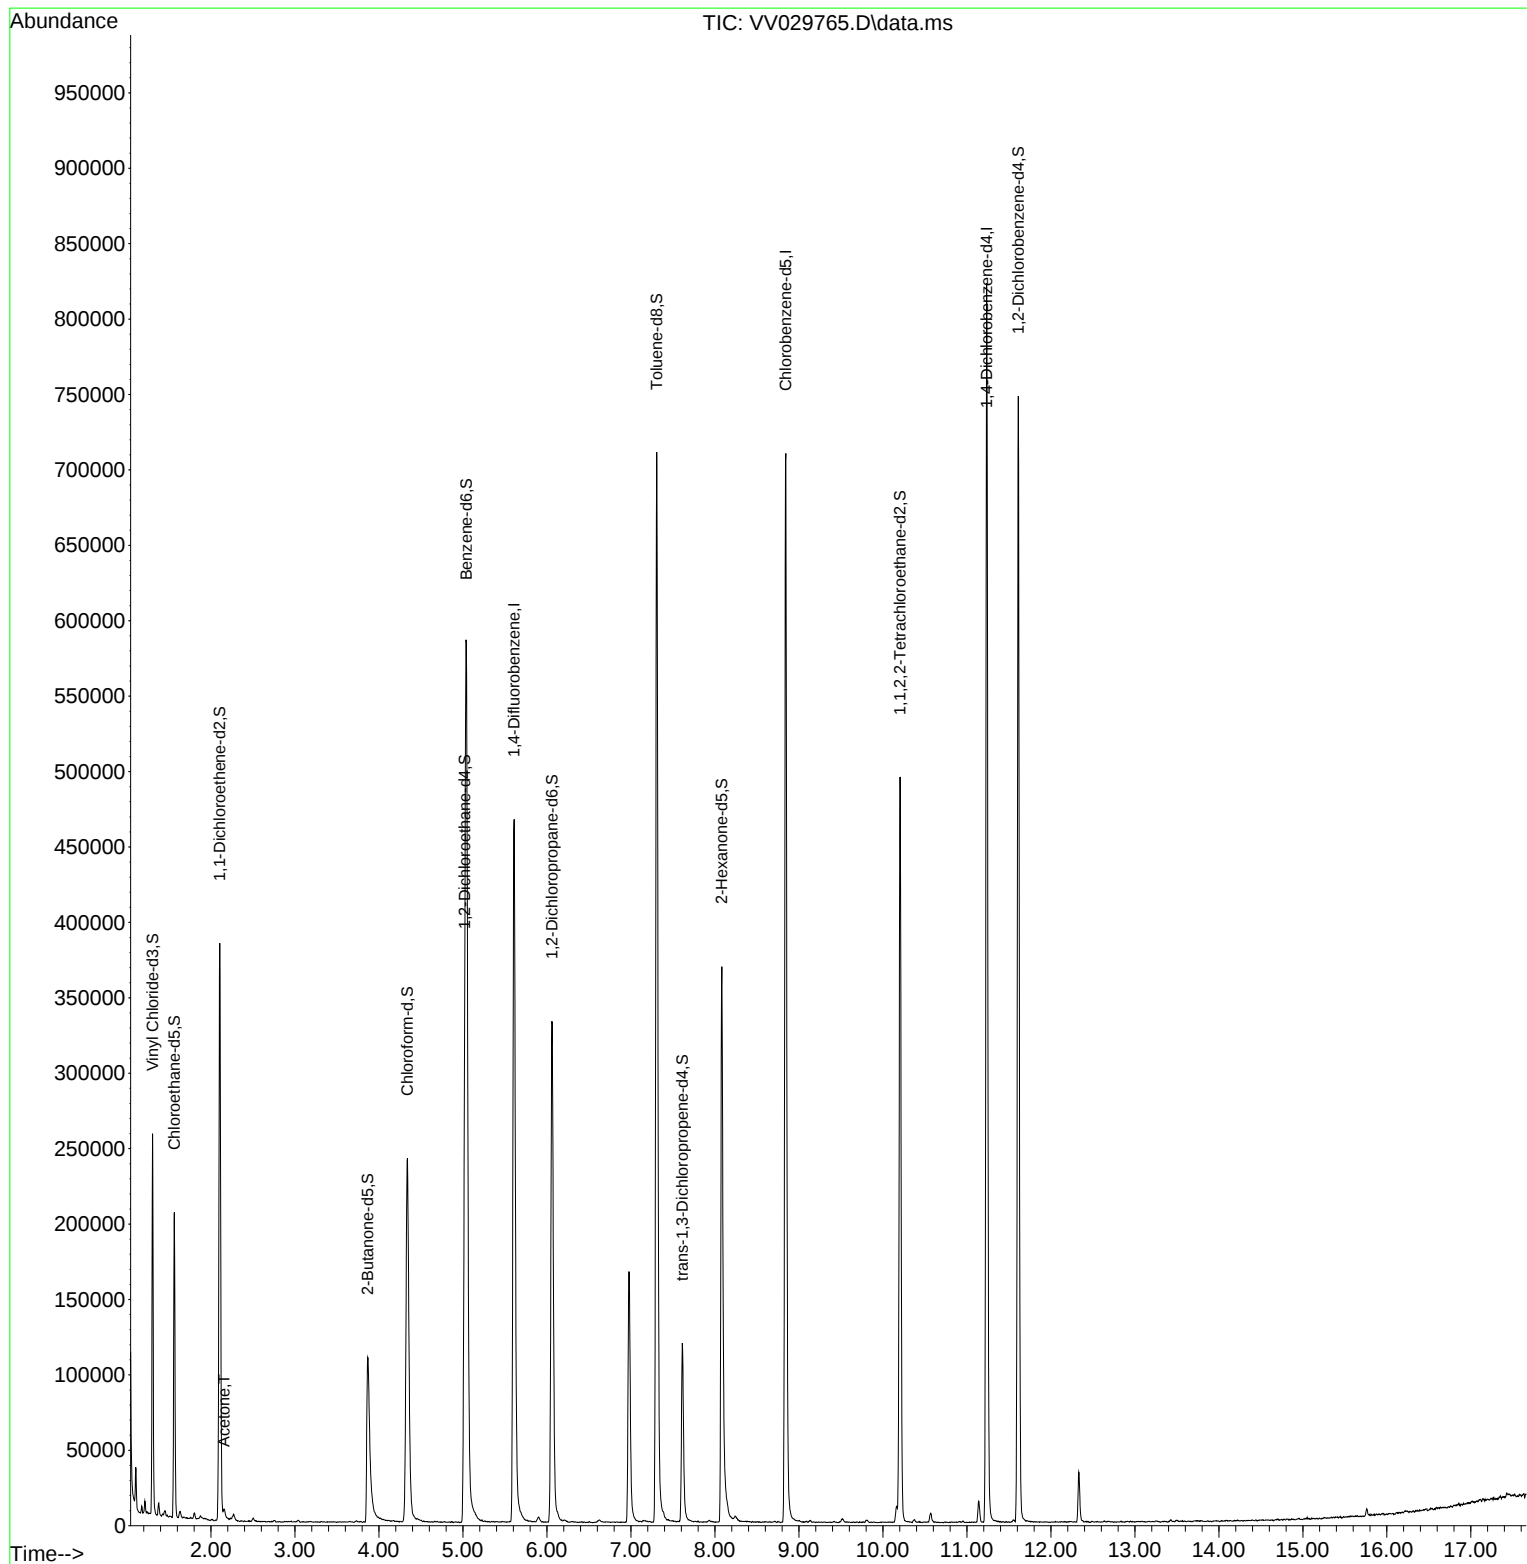

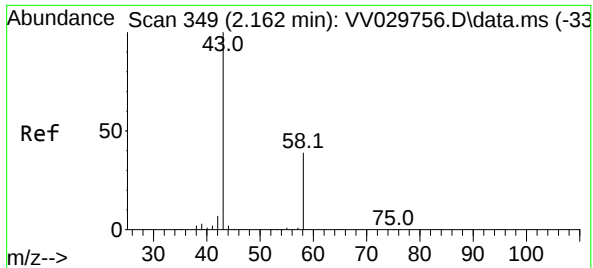

#13
 Acetone
 Concen: 5.320 ug/L
 RT: 2.156 min Scan# 34
 Delta R.T. -0.006 min
 Lab File: VV029765.D
 Acq: 22 Dec 2022 17:51

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Tgt Ion: 43 Resp: 5645
 Ion Ratio Lower Upper
 43 100
 58 38.2 0.0 74.8

