

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029766.D
 Acq On : 22 Dec 2022 18:14
 Operator : SY/MD
 Sample : N6193-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Quant Time: Dec 23 02:10:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.609	114	450608	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.844	117	436477	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.239	152	231016	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	158495	57.440	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	114.880%	
7) Chloroethane-d5		1.565	69	131822	62.651	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	125.300%	
11) 1,1-Dichloroethene-d2		2.105	63	199660	46.391	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.780%	
21) 2-Butanone-d5		3.867	46	172538	102.502	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.500%	
24) Chloroform-d		4.339	84	249772	48.102	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.200%	
26) 1,2-Dichloroethane-d4		5.021	65	155576	52.459	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.920%	
32) Benzene-d6		5.040	84	561937	48.723	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.440%	
36) 1,2-Dichloropropane-d6		6.059	67	176484	50.097	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.200%	
41) Toluene-d8		7.307	98	502063	46.201	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.400%	
43) trans-1,3-Dichloroprop...		7.612	79	74143	41.679	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.360%	
47) 2-Hexanone-d5		8.082	63	145337	96.612	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.610%	
56) 1,1,2,2-Tetrachloroeth...		10.204	84	241920	48.056	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.120%	
66) 1,2-Dichlorobenzene-d4		11.612	152	199515	45.368	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.740%	
Target Compounds							Qvalue
13) Acetone		2.159	43	2814	2.566	ug/L	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029766.D
Acq On : 22 Dec 2022 18:14
Operator : SY/MD
Sample : N6193-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Time: Dec 23 02:10:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

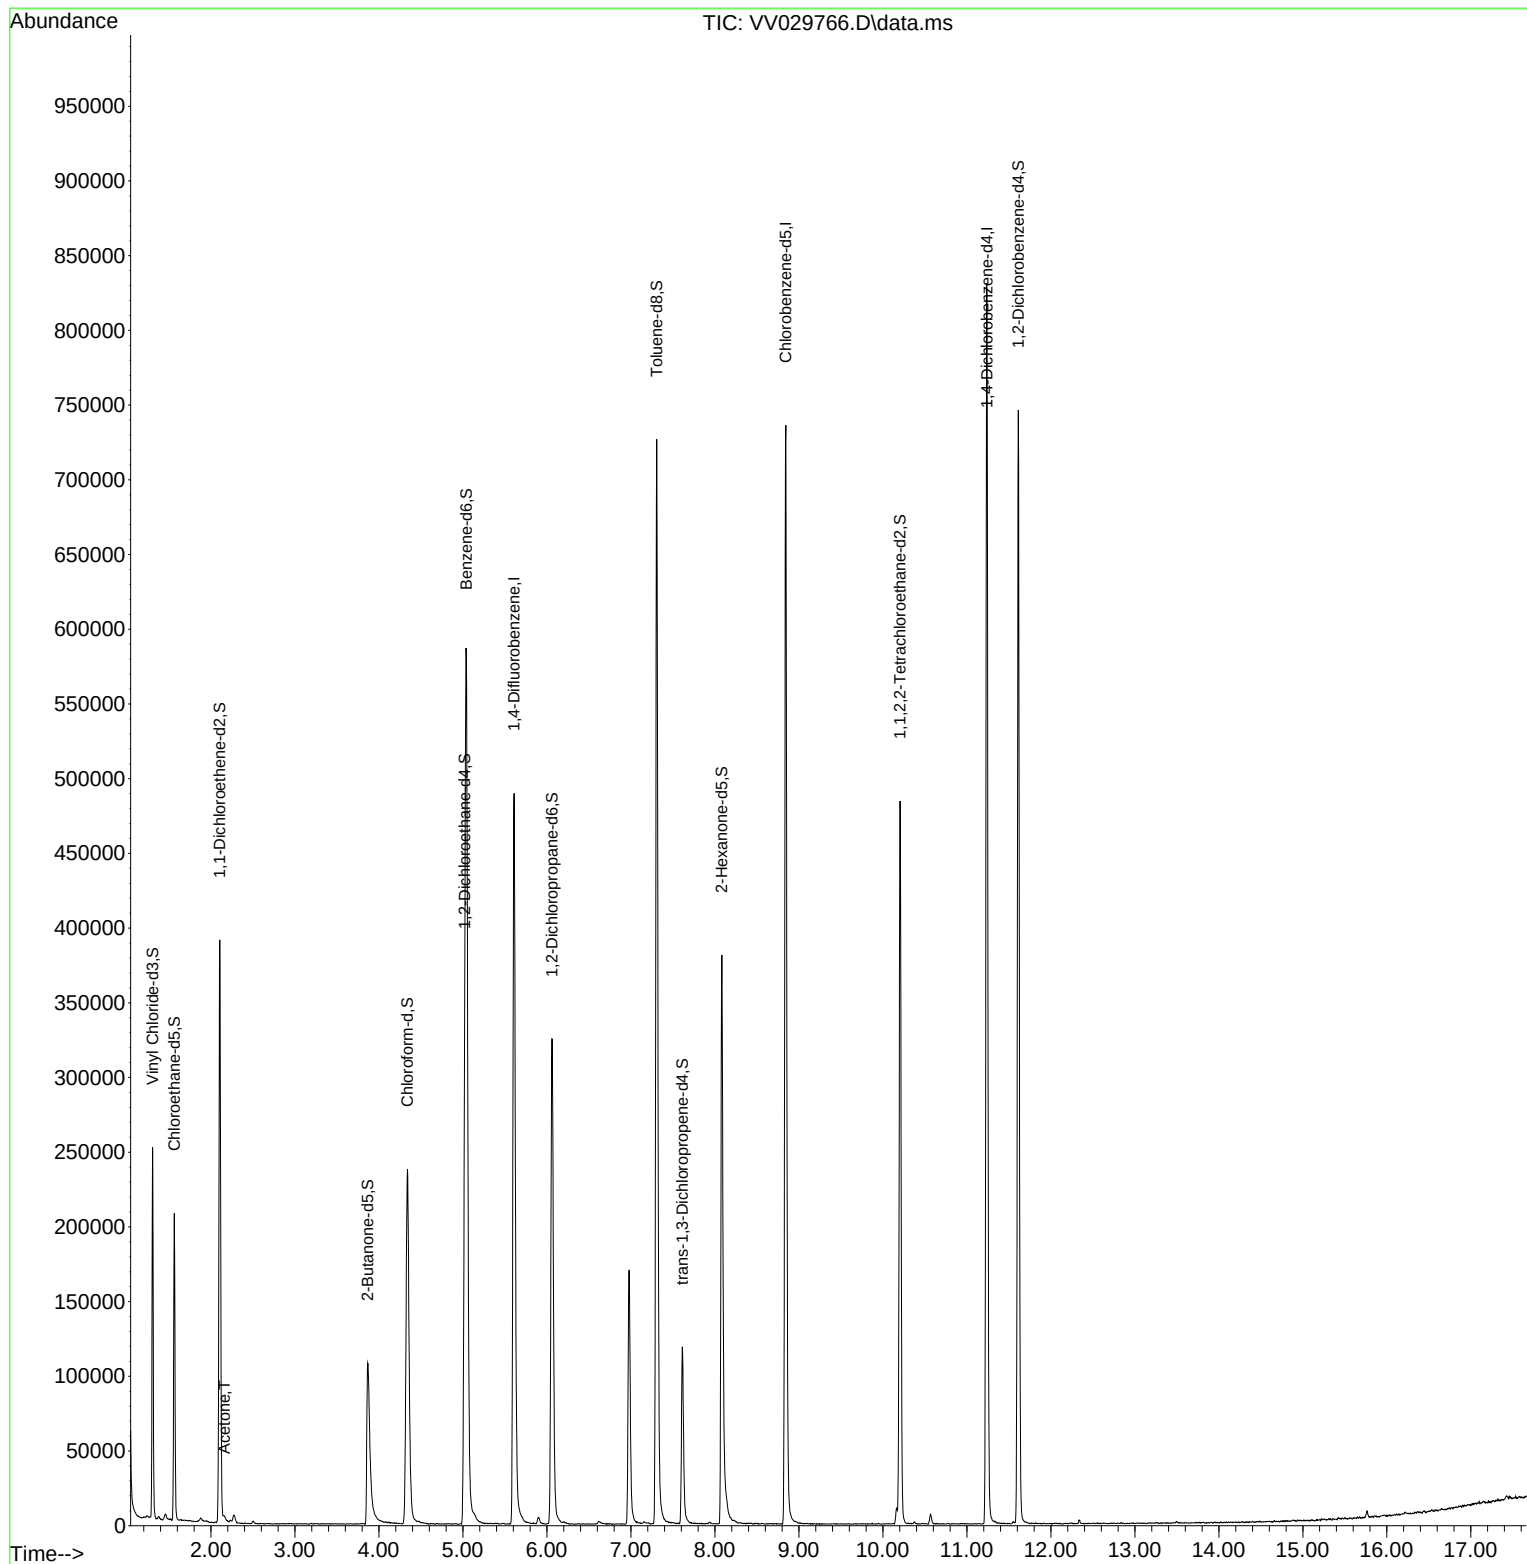

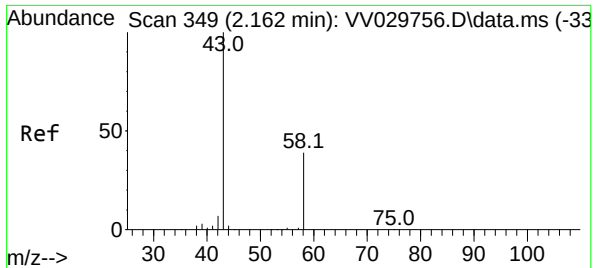

#13
 Acetone
 Concen: 2.566 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. -0.003 min
 Lab File: VV029766.D
 Acq: 22 Dec 2022 18:14

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Tgt Ion: 43 Resp: 2814
 Ion Ratio Lower Upper
 43 100
 58 16.6 0.0 74.8

