

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029767.D
 Acq On : 22 Dec 2022 18:38
 Operator : SY/MD
 Sample : N6195-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Quant Time: Dec 23 02:10:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.609	114	491841	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.844	117	477212	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.236	152	250643	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	159153	52.843	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.680%	
7) Chloroethane-d5		1.564	69	136948	59.631	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	119.260%	
11) 1,1-Dichloroethene-d2		2.105	63	206713	44.004	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.000%	
21) 2-Butanone-d5		3.867	46	179077	97.468	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.470%	
24) Chloroform-d		4.339	84	270825	47.784	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.560%	
26) 1,2-Dichloroethane-d4		5.021	65	163513	50.514	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.020%	
32) Benzene-d6		5.043	84	591827	46.935	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.860%	
36) 1,2-Dichloropropane-d6		6.059	67	188161	48.852	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.700%	
41) Toluene-d8		7.307	98	527835	44.427	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.860%	
43) trans-1,3-Dichloroprop...		7.612	79	77555	39.875	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.760%	
47) 2-Hexanone-d5		8.082	63	149494	90.892	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.890%	
56) 1,1,2,2-Tetrachloroeth...		10.204	84	256020	46.515	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.040%	
66) 1,2-Dichlorobenzene-d4		11.612	152	212261	44.487	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.980%	
Target Compounds							
13) Acetone		2.159	43	6195	5.176	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029767.D
Acq On : 22 Dec 2022 18:38
Operator : SY/MD
Sample : N6195-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN6

Quant Time: Dec 23 02:10:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

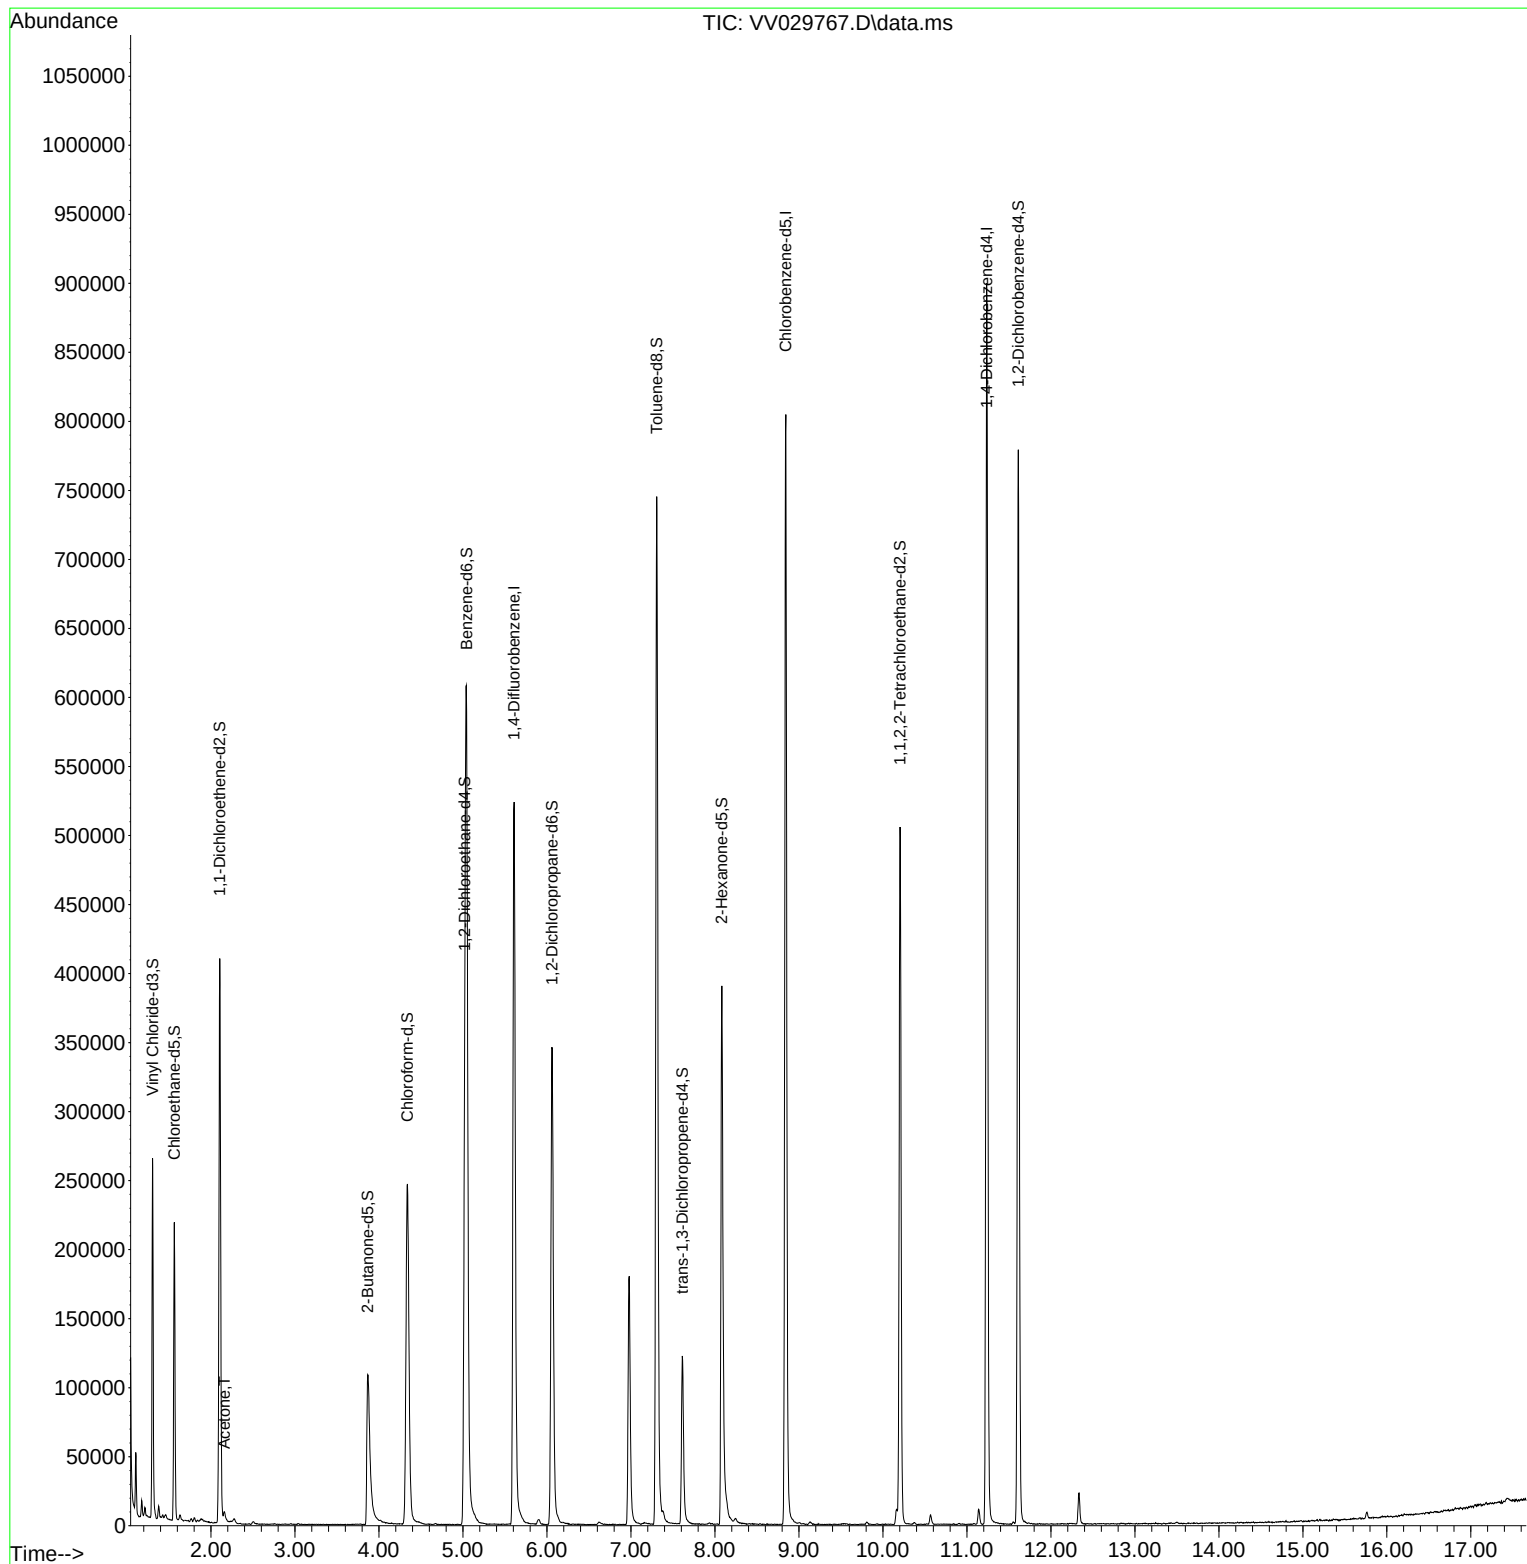

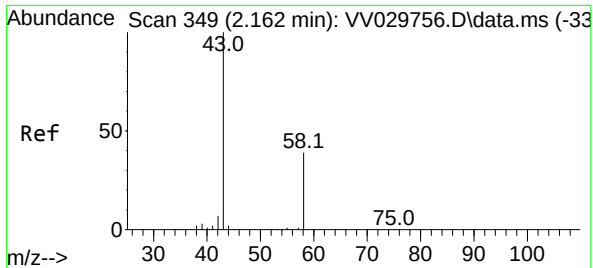

#13
 Acetone
 Concen: 5.176 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. -0.003 min
 Lab File: VV029767.D
 Acq: 22 Dec 2022 18:38

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Tgt Ion:	43	Resp:	6195
Ion	Ratio	Lower	Upper
43	100		
58	36.7	0.0	74.8

