

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029769.D
 Acq On : 22 Dec 2022 19:25
 Operator : SY/MD
 Sample : N6195-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN8

Quant Time: Dec 23 02:10:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	477453	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	460685	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	243441	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	162544	55.595	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	111.180%	
7) Chloroethane-d5	1.564	69	134987	60.548	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	121.100%	
11) 1,1-Dichloroethene-d2	2.104	63	204928	44.938	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.880%	
21) 2-Butanone-d5	3.870	46	179495	100.639	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	100.640%	
24) Chloroform-d	4.339	84	263303	47.857	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.720%	
26) 1,2-Dichloroethane-d4	5.024	65	159219	50.669	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.340%	
32) Benzene-d6	5.043	84	588278	48.327	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.660%	
36) 1,2-Dichloropropane-d6	6.063	67	182760	49.152	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	98.300%	
41) Toluene-d8	7.307	98	516565	45.038	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.080%	
43) trans-1,3-Dichloroprop...	7.612	79	75977	40.466	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.940%	
47) 2-Hexanone-d5	8.082	63	151099	95.164	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	95.160%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	252379	47.499	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	95.000%	
66) 1,2-Dichlorobenzene-d4	11.612	152	209836	45.280	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.560%	
Target Compounds						
13) Acetone	2.162	43	8550	7.359	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029769.D
Acq On : 22 Dec 2022 19:25
Operator : SY/MD
Sample : N6195-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN8

Quant Time: Dec 23 02:10:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

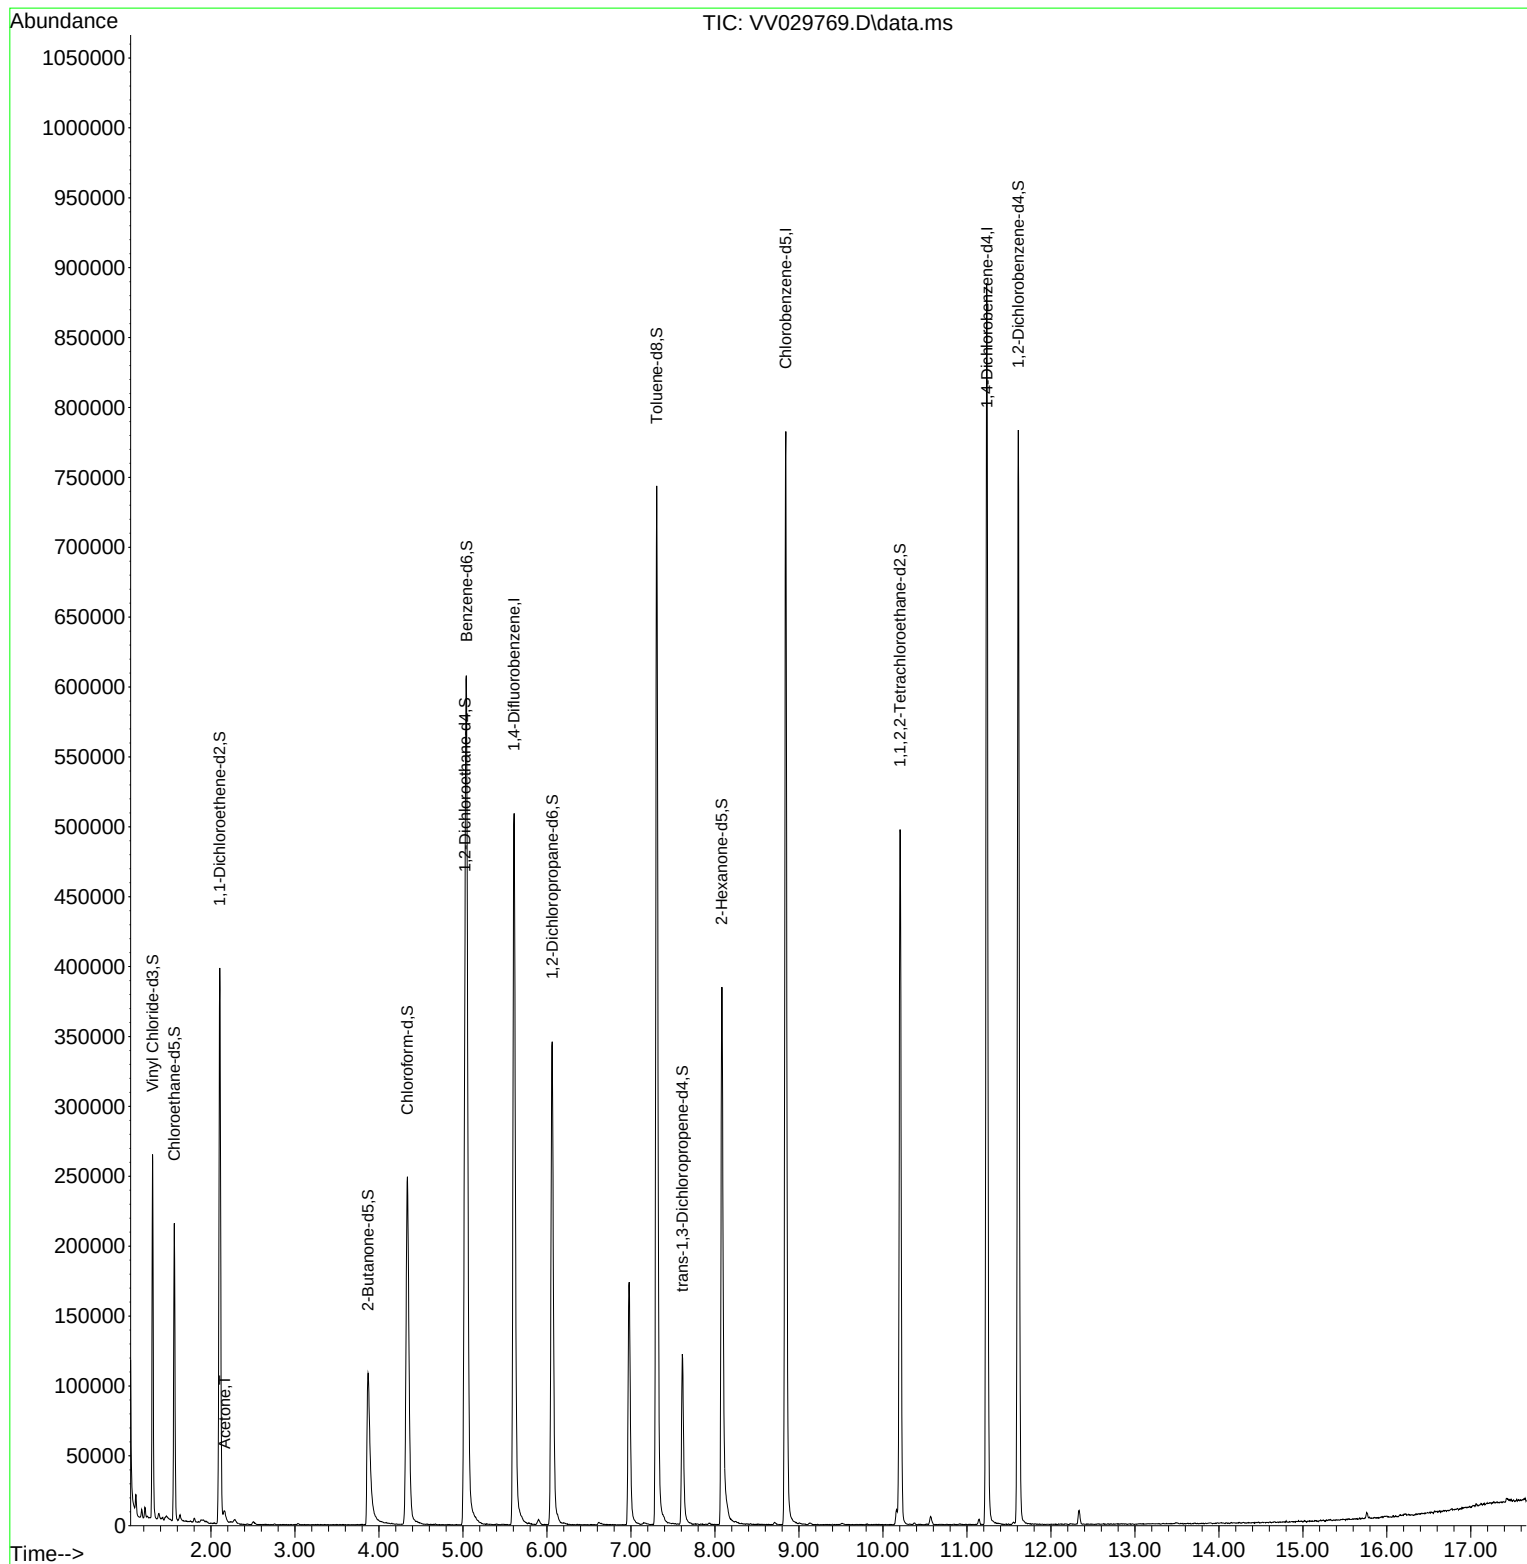

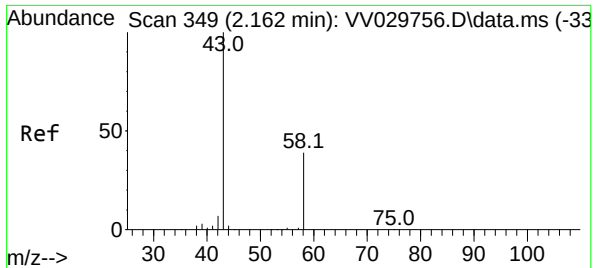

#13
 Acetone
 Concen: 7.359 ug/L
 RT: 2.162 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV029769.D
 Acq: 22 Dec 2022 19:25

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN8

Tgt Ion: 43 Resp: 8550
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 74.8

