

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029770.D
 Acq On : 22 Dec 2022 19:48
 Operator : SY/MD
 Sample : N6195-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN9

Quant Time: Dec 23 02:10:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	495879	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	483969	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	256391	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	160694	52.920	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.840%
7) Chloroethane-d5	1.564	69	138016	59.606	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	119.220%
11) 1,1-Dichloroethene-d2	2.105	63	206846	43.673	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.340%
21) 2-Butanone-d5	3.870	46	178539	96.384	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.380%
24) Chloroform-d	4.339	84	271722	47.552	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.100%
26) 1,2-Dichloroethane-d4	5.024	65	163208	50.009	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.020%
32) Benzene-d6	5.043	84	596219	46.623	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.240%
36) 1,2-Dichloropropane-d6	6.059	67	189280	48.457	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.920%
41) Toluene-d8	7.307	98	529824	43.972	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.940%
43) trans-1,3-Dichloroprop...	7.612	79	77771	39.428	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.860%
47) 2-Hexanone-d5	8.082	63	150009	89.932	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.930%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	258423	46.297	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	11.612	152	212034	43.443	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.880%
Target Compounds						
13) Acetone	2.159	43	10539	8.734	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029770.D
Acq On : 22 Dec 2022 19:48
Operator : SY/MD
Sample : N6195-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN9

Quant Time: Dec 23 02:10:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

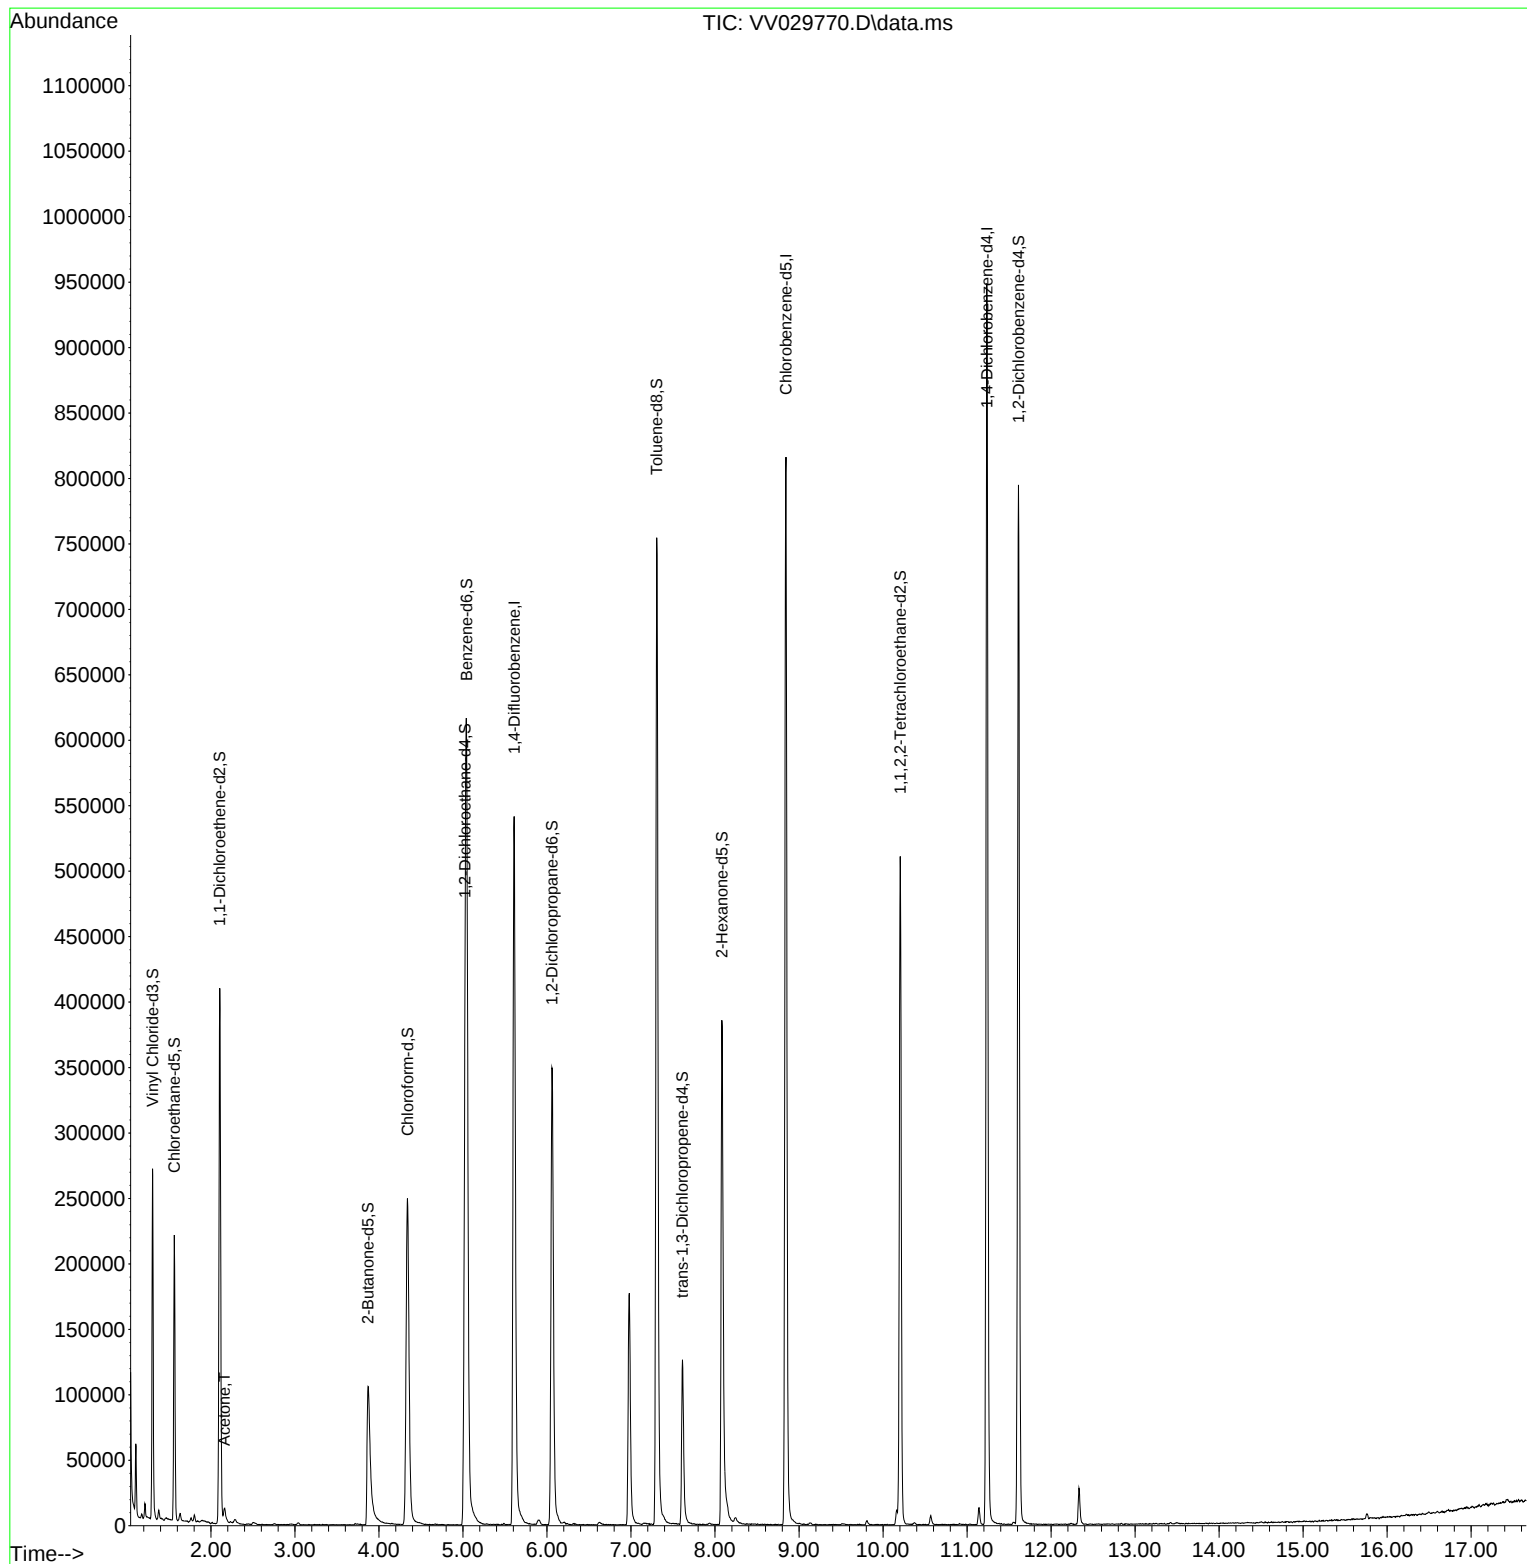

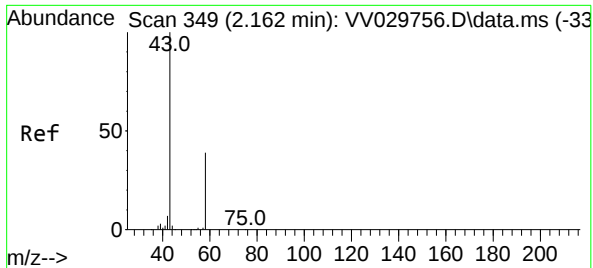

#13
 Acetone
 Concen: 8.734 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. -0.003 min
 Lab File: VV029770.D
 Acq: 22 Dec 2022 19:48

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN9

Tgt Ion: 43	Resp: 10539
Ion Ratio	Lower Upper
43	100
58	36.5 0.0 74.8

