

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029771.D
 Acq On : 22 Dec 2022 20:12
 Operator : SY/MD
 Sample : N6195-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP0

Quant Time: Dec 23 02:10:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	480408	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	467666	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	246143	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	156953	53.352	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	106.700%	
7) Chloroethane-d5	1.564	69	135191	60.266	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	120.540%	
11) 1,1-Dichloroethene-d2	2.104	63	203520	44.355	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	88.700%	
21) 2-Butanone-d5	3.870	46	177263	98.776	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	98.780%	
24) Chloroform-d	4.339	84	266963	48.224	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.440%	
26) 1,2-Dichloroethane-d4	5.024	65	161701	51.143	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.280%	
32) Benzene-d6	5.043	84	593227	48.006	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.020%	
36) 1,2-Dichloropropane-d6	6.063	67	182157	48.259	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	96.520%	
41) Toluene-d8	7.307	98	518112	44.499	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	7.612	79	76532	40.153	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.300%	
47) 2-Hexanone-d5	8.082	63	145307	90.150	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	90.150%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	251964	46.713	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	93.420%	
66) 1,2-Dichlorobenzene-d4	11.612	152	207602	44.306	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	88.620%	
Target Compounds						
13) Acetone	2.162	43	6139	5.251	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029771.D
Acq On : 22 Dec 2022 20:12
Operator : SY/MD
Sample : N6195-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP0

Quant Time: Dec 23 02:10:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

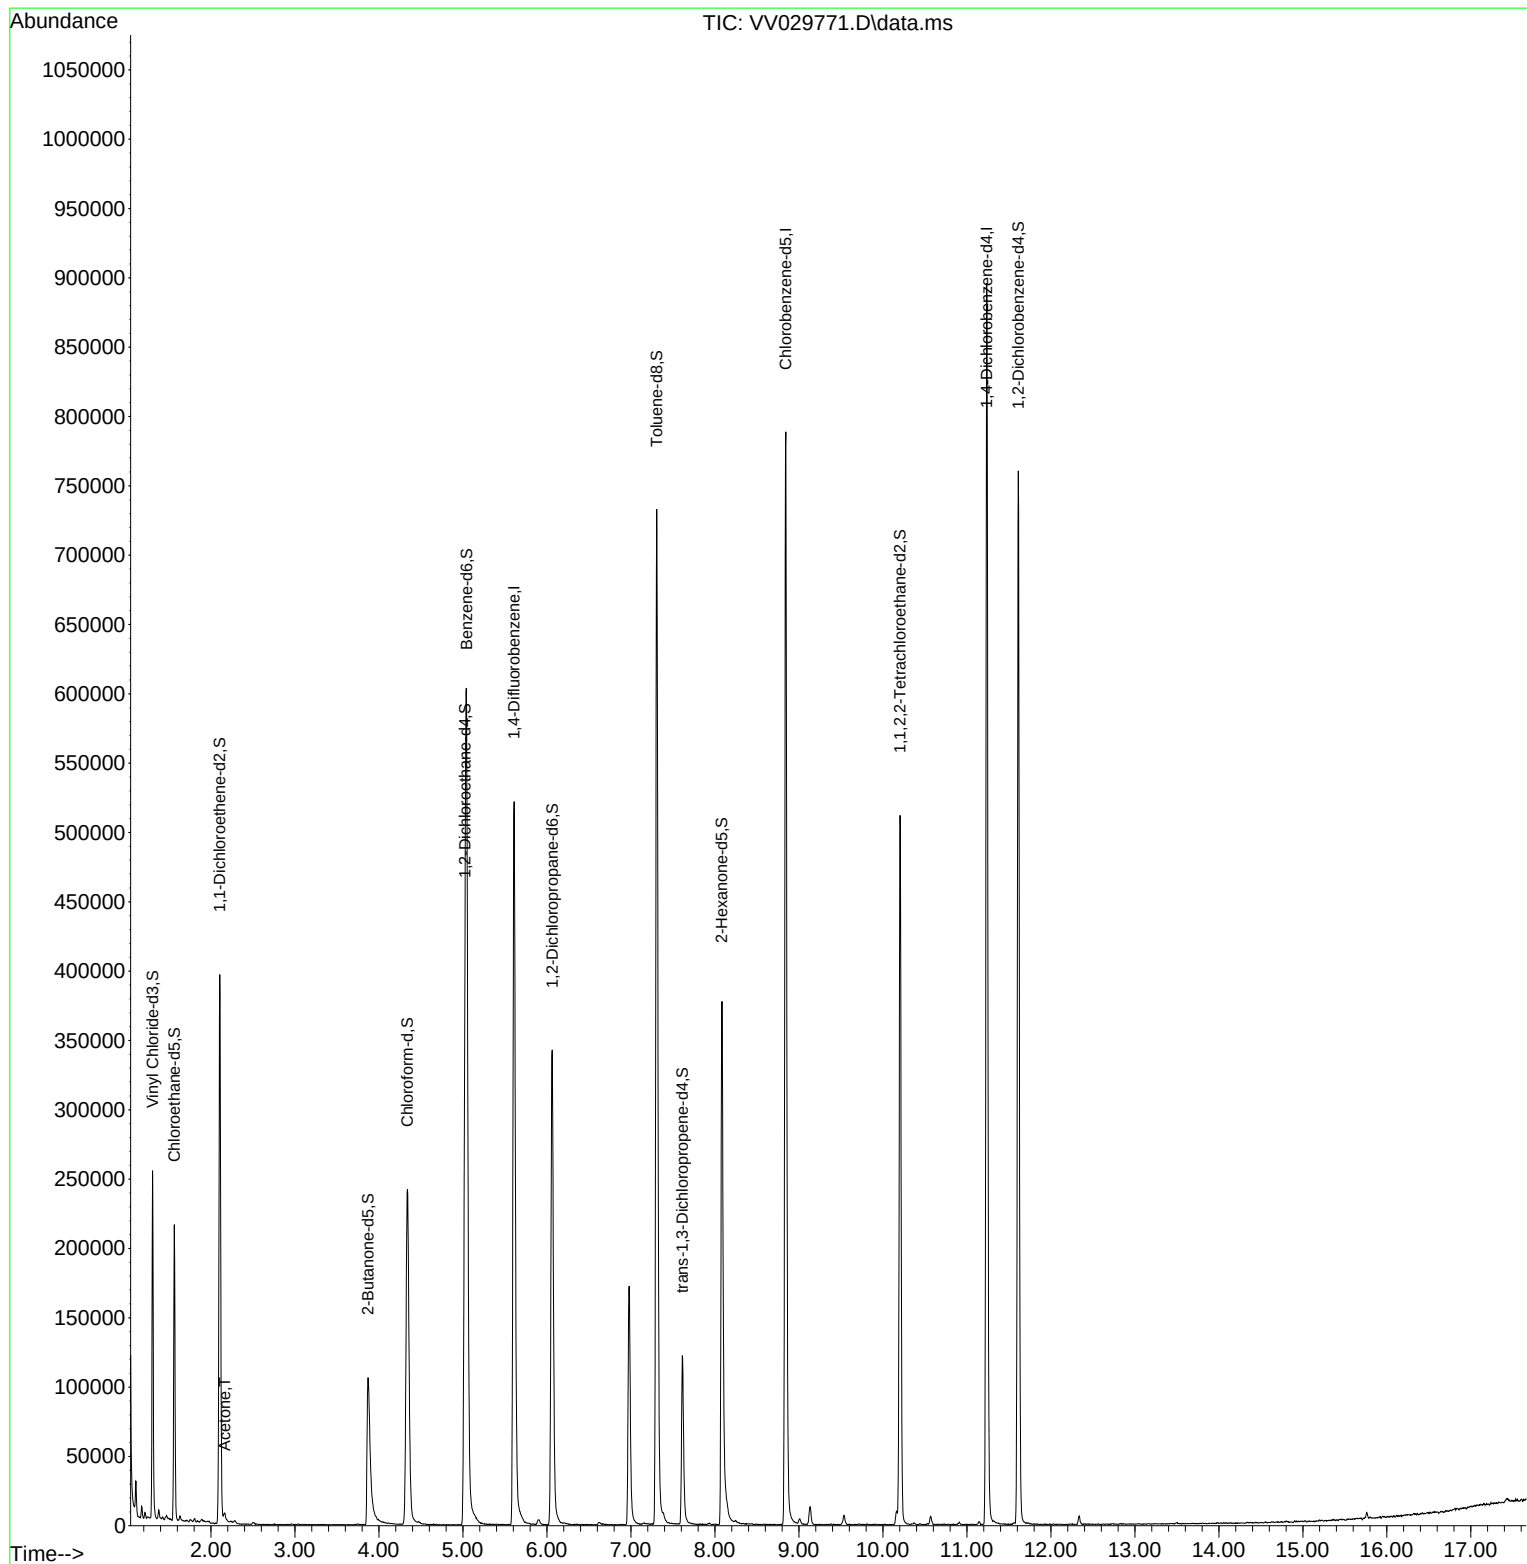

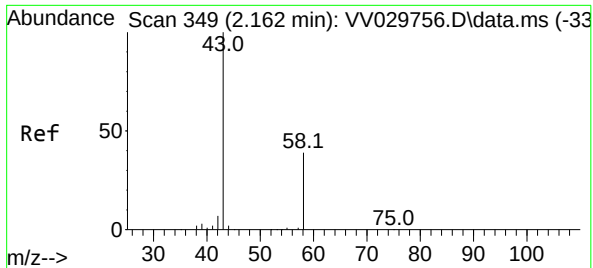

#13
 Acetone
 Concen: 5.251 ug/L
 RT: 2.162 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV029771.D
 Acq: 22 Dec 2022 20:12

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP0

Tgt Ion: 43 Resp: 6139
 Ion Ratio Lower Upper
 43 100
 58 33.2 0.0 74.8

