

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029772.D
 Acq On : 22 Dec 2022 20:36
 Operator : SY/MD
 Sample : N6195-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Quant Time: Dec 23 02:10:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.609	114	475582	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.844	117	465334	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.236	152	243759	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	152035	52.205	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	104.420%	
7) Chloroethane-d5		1.564	69	130903	58.947	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	117.900%	
11) 1,1-Dichloroethene-d2		2.105	63	198049	43.601	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.200%	
21) 2-Butanone-d5		3.870	46	179223	100.882	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.880%	
24) Chloroform-d		4.336	84	260041	47.450	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.900%	
26) 1,2-Dichloroethane-d4		5.021	65	156194	49.902	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.800%	
32) Benzene-d6		5.043	84	572110	46.529	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.060%	
36) 1,2-Dichloropropane-d6		6.063	67	178578	47.548	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.100%	
41) Toluene-d8		7.307	98	506236	43.696	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.400%	
43) trans-1,3-Dichloroprop...		7.612	79	74999	39.546	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.100%	
47) 2-Hexanone-d5		8.082	63	148437	92.553	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.550%	
56) 1,1,2,2-Tetrachloroeth...		10.204	84	247102	46.041	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.080%	
66) 1,2-Dichlorobenzene-d4		11.612	152	205031	44.185	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.380%	
Target Compounds							
13) Acetone		2.162	43	4265	3.685	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029772.D
Acq On : 22 Dec 2022 20:36
Operator : SY/MD
Sample : N6195-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP1

Quant Time: Dec 23 02:10:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

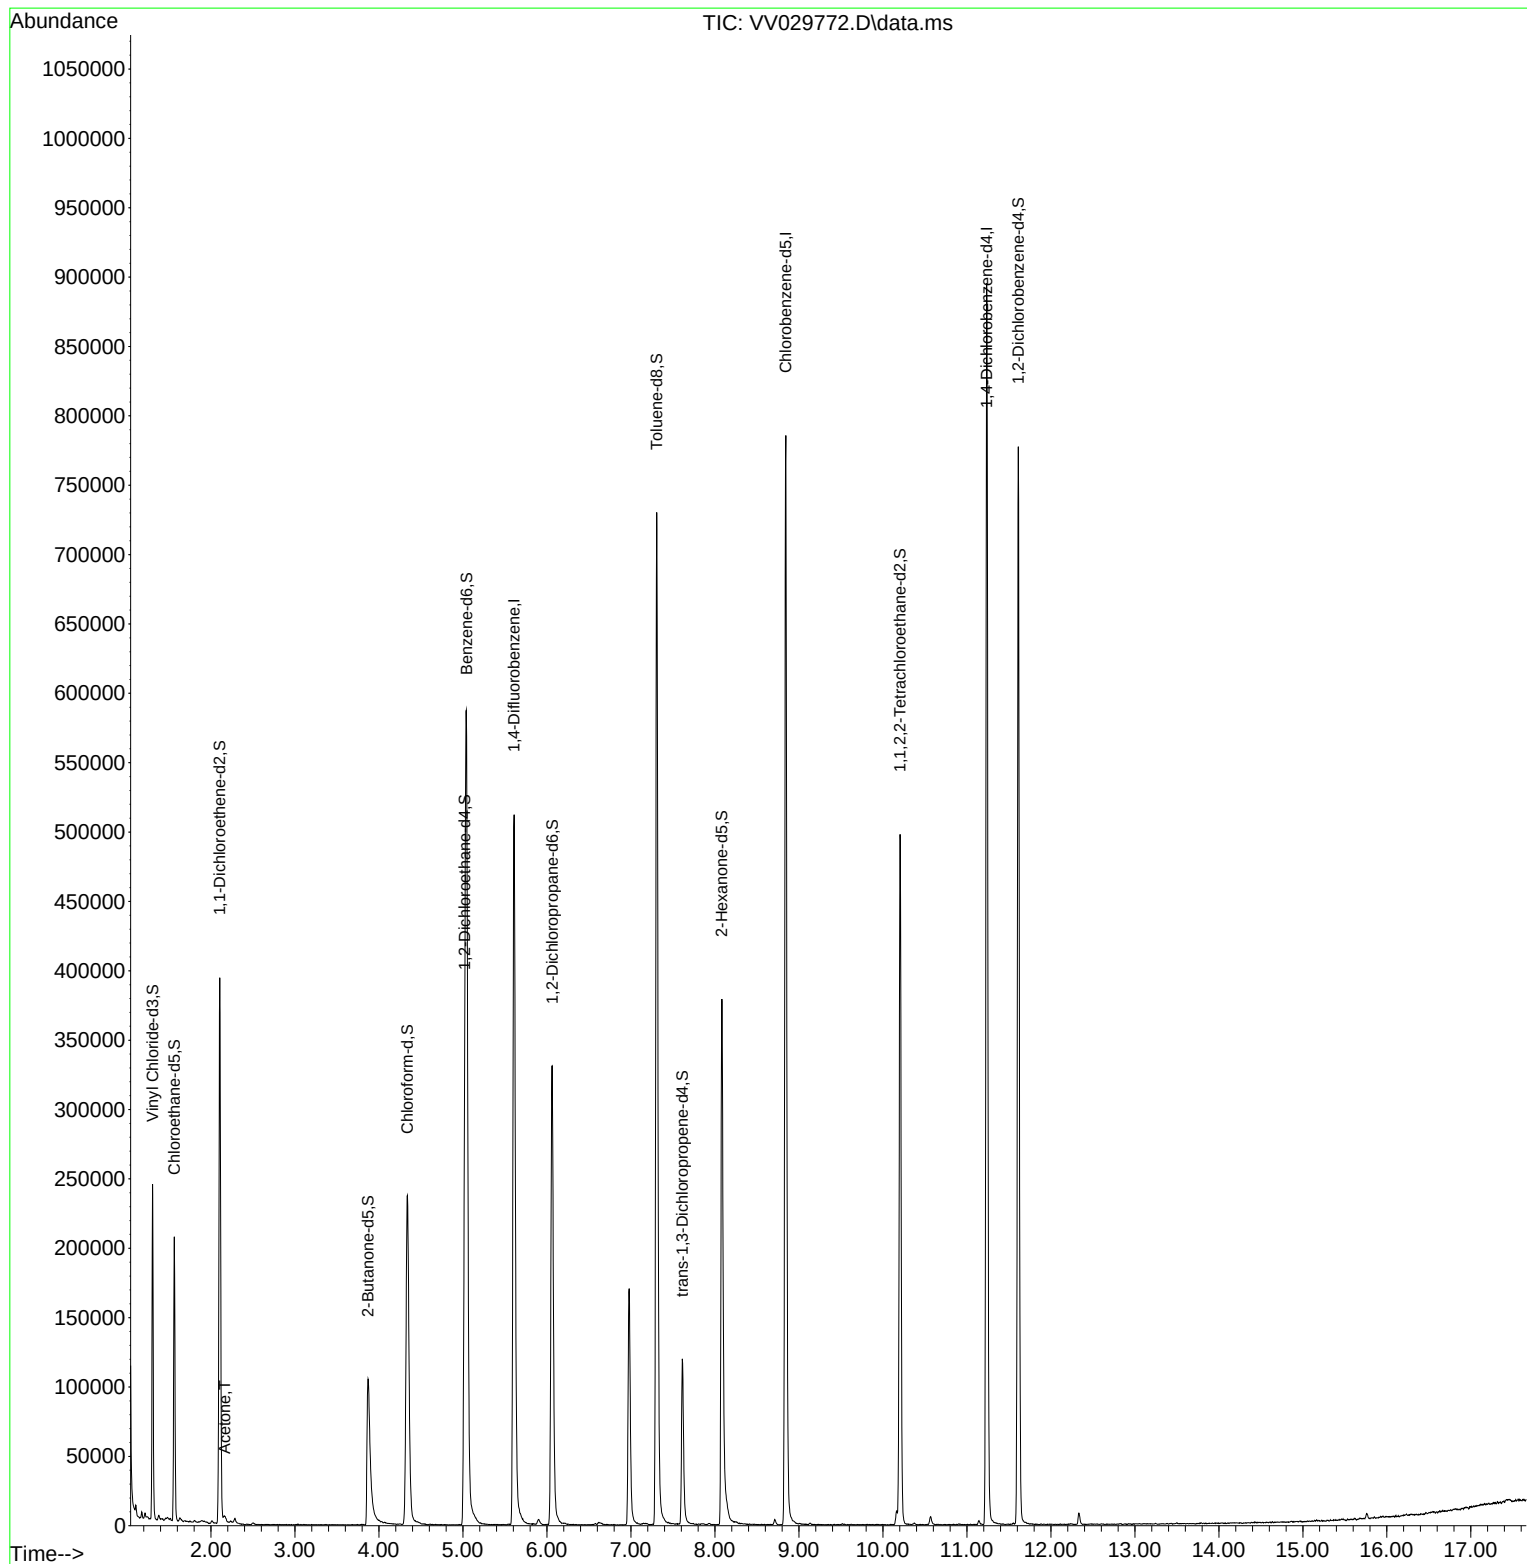

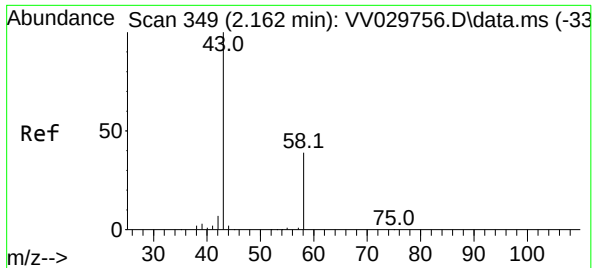

#13
 Acetone
 Concen: 3.685 ug/L
 RT: 2.162 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV029772.D
 Acq: 22 Dec 2022 20:36

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Tgt Ion: 43 Resp: 4265
 Ion Ratio Lower Upper
 43 100
 58 36.5 0.0 74.8

